

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033151.D
 Acq On : 07 Dec 2023 16:58
 Operator : SY/MD
 Sample : 05645-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G68

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VV033151.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	86	rVB	87121	91381	11.03%	1.296%
2	1.420	111	118	126	rVB	5901	8400	1.01%	0.119%
3	1.465	130	132	135	rVB	1257	757	0.09%	0.011%
4	1.490	135	140	144	rBV3	1400	1413	0.17%	0.020%
5	1.532	144	153	163	rBV	74459	83629	10.10%	1.186%
6	1.622	179	181	184	rVV2	1205	803	0.10%	0.011%
7	1.642	184	187	191	rVB	1422	967	0.12%	0.014%
8	1.687	196	201	204	rBV	1620	1551	0.19%	0.022%
9	1.709	204	208	212	rVV3	768	757	0.09%	0.011%
10	1.757	217	223	226	rBV2	1251	1073	0.13%	0.015%
11	1.812	236	240	242	rBV2	1723	1236	0.15%	0.018%
12	1.867	252	257	261	rBV4	812	713	0.09%	0.010%
13	1.953	277	284	291	rBV4	1589	1417	0.17%	0.020%
14	1.982	291	293	296	rVB2	1363	744	0.09%	0.011%
15	2.005	296	300	304	rBV	1522	1327	0.16%	0.019%
16	2.060	307	317	331	rBV	143768	215687	26.04%	3.059%
17	2.143	336	343	345	rBV	2649	2989	0.36%	0.042%
18	2.217	354	366	376	rBV2	12369	24998	3.02%	0.355%
19	2.436	431	434	437	rBV	1059	825	0.10%	0.012%
20	3.191	665	669	673	rBV	2015	1570	0.19%	0.022%
21	3.365	718	723	727	rBV	2422	2887	0.35%	0.041%
22	3.436	739	745	747	rBV2	1515	1856	0.22%	0.026%
23	3.616	798	801	805	rVB2	1222	716	0.09%	0.010%
24	3.783	844	853	880	rBV2	59669	166311	20.08%	2.358%
25	4.249	984	998	1019	rBV	137267	345657	41.74%	4.902%
26	4.474	1065	1068	1069	rBV2	1351	844	0.10%	0.012%
27	4.580	1098	1101	1102	rBV	1578	824	0.10%	0.012%
28	4.722	1142	1145	1151	rBV2	1658	1719	0.21%	0.024%
29	4.957	1203	1218	1245	rBV3	294850	781932	94.42%	11.089%
30	5.104	1262	1264	1267	rBV2	1517	1123	0.14%	0.016%
31	5.420	1360	1362	1365	rBV2	1287	854	0.10%	0.012%
32	5.535	1386	1398	1424	rVV	314035	646262	78.04%	9.165%
33	5.712	1451	1453	1458	rVB2	1555	1096	0.13%	0.016%
34	5.773	1469	1472	1476	rBV	2239	1634	0.20%	0.023%
35	5.834	1480	1491	1515	rVB5	60651	138686	16.75%	1.967%
36	5.989	1526	1539	1563	rBV2	171334	360062	43.48%	5.106%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120723\
 Data File : VW033151.D
 Acq On : 07 Dec 2023 16:58
 Operator : SY/MD
 Sample : 05645-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G68

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	6.326	1641	1644	1648	rVB	1932	1396	0.17%	0.020%
38	6.854	1804	1808	1814	rBV2	2180	2745	0.33%	0.039%
39	6.915	1817	1827	1845	rBV	97501	181144	21.87%	2.569%
40	7.124	1890	1892	1896	rBV	1231	1027	0.12%	0.015%
41	7.243	1919	1929	1949	rBV	355987	630392	76.12%	8.940%
42	7.555	2016	2026	2046	rBV	71313	129942	15.69%	1.843%
43	7.754	2085	2088	2090	rBV	1247	847	0.10%	0.012%
44	7.844	2113	2116	2119	rBV2	969	775	0.09%	0.011%
45	7.876	2123	2126	2130	rBV	2323	2413	0.29%	0.034%
46	8.024	2163	2172	2191	rBV	193664	354224	42.77%	5.023%
47	8.217	2230	2232	2238	rVB	1970	1303	0.16%	0.018%
48	8.603	2349	2352	2357	rBV	1596	1554	0.19%	0.022%
49	8.651	2364	2367	2372	rVB	1365	975	0.12%	0.014%
50	8.783	2398	2408	2429	rBV	496819	815057	98.42%	11.559%
51	9.423	2604	2607	2612	rBV	1355	1590	0.19%	0.023%
52	9.577	2652	2655	2659	rBV	1152	1051	0.13%	0.015%
53	9.644	2672	2676	2679	rBV	1886	1768	0.21%	0.025%
54	9.844	2735	2738	2741	rBV2	893	903	0.11%	0.013%
55	9.879	2746	2749	2753	rVV2	1306	1077	0.13%	0.015%
56	9.940	2765	2768	2770	rBV	1148	827	0.10%	0.012%
57	9.989	2778	2783	2789	rBV	2463	2906	0.35%	0.041%
58	10.085	2811	2813	2816	rBV2	1351	925	0.11%	0.013%
59	10.152	2823	2834	2857	rBV	272808	425372	51.36%	6.032%
60	10.304	2878	2881	2884	rBV	1194	893	0.11%	0.013%
61	10.487	2936	2938	2942	rVB2	1813	1163	0.14%	0.016%
62	10.828	3041	3044	3049	rBV	1120	1233	0.15%	0.017%
63	10.857	3050	3053	3056	rVV2	1220	844	0.10%	0.012%
64	10.934	3073	3077	3079	rBV	1535	1261	0.15%	0.018%
65	11.130	3135	3138	3145	rVV3	1795	1744	0.21%	0.025%
66	11.185	3145	3155	3174	rBV	535817	828154	100.00%	11.744%
67	11.406	3221	3224	3228	rBV	1212	1161	0.14%	0.016%
68	11.484	3245	3248	3250	rVB	1363	731	0.09%	0.010%
69	11.561	3261	3272	3294	rVB	457714	714131	86.23%	10.127%
70	11.641	3295	3297	3300	rVB	1557	783	0.09%	0.011%
71	11.715	3318	3320	3323	rBV2	1042	778	0.09%	0.011%
72	11.741	3326	3328	3334	rVB	2131	1873	0.23%	0.027%
73	11.796	3341	3345	3348	rBV2	1677	1341	0.16%	0.019%
74	12.239	3479	3483	3486	rBV	1746	1448	0.17%	0.021%
75	12.358	3517	3520	3524	rBV2	1369	1197	0.14%	0.017%
76	12.471	3552	3555	3558	rVB3	1307	817	0.10%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033151.D
 Acq On : 07 Dec 2023 16:58
 Operator : SY/MD
 Sample : 05645-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G68

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	12.493	3558	3562	3569	rBV	2526	2939	0.35%	0.042%
78	12.677	3616	3619	3625	rVV2	1488	1280	0.15%	0.018%
79	12.770	3645	3648	3653	rBV	1271	878	0.11%	0.012%
80	12.812	3658	3661	3663	rBV	1298	849	0.10%	0.012%
81	12.860	3673	3676	3678	rBV	1478	1157	0.14%	0.016%
82	12.998	3716	3719	3721	rBV	1203	875	0.11%	0.012%
83	13.104	3749	3752	3758	rBV	1574	1493	0.18%	0.021%
84	13.152	3764	3767	3770	rBV	2001	1225	0.15%	0.017%
85	13.210	3782	3785	3788	rBV2	1436	1104	0.13%	0.016%
86	13.303	3810	3814	3817	rBV	2355	1993	0.24%	0.028%
87	13.644	3918	3920	3924	rVB	1657	1091	0.13%	0.015%
88	13.821	3972	3975	3979	rBV	1563	1278	0.15%	0.018%
89	13.844	3979	3982	3987	rBV	2531	2690	0.32%	0.038%
90	14.602	4213	4218	4219	rBV3	1689	1459	0.18%	0.021%
91	14.693	4244	4246	4249	rVB	1689	829	0.10%	0.012%
92	14.750	4261	4264	4266	rBV2	1530	917	0.11%	0.013%
93	14.959	4323	4329	4333	rBV	2716	3437	0.42%	0.049%
94	15.004	4340	4343	4345	rBV	1750	1211	0.15%	0.017%
95	15.107	4372	4375	4379	rBV2	1388	919	0.11%	0.013%
96	15.130	4379	4382	4385	rBV	1732	1143	0.14%	0.016%
97	15.368	4452	4456	4458	rBV2	1528	1181	0.14%	0.017%
98	15.901	4618	4622	4625	rBV	2300	1970	0.24%	0.028%
99	16.136	4692	4695	4699	rBV3	2849	2414	0.29%	0.034%
100	17.162	5011	5014	5017	rBV2	3024	2782	0.34%	0.039%


Sum of corrected areas: 7051579

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033151.D
Acq On : 07 Dec 2023 16:58
Operator : SY/MD
Sample : 05645-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G68

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

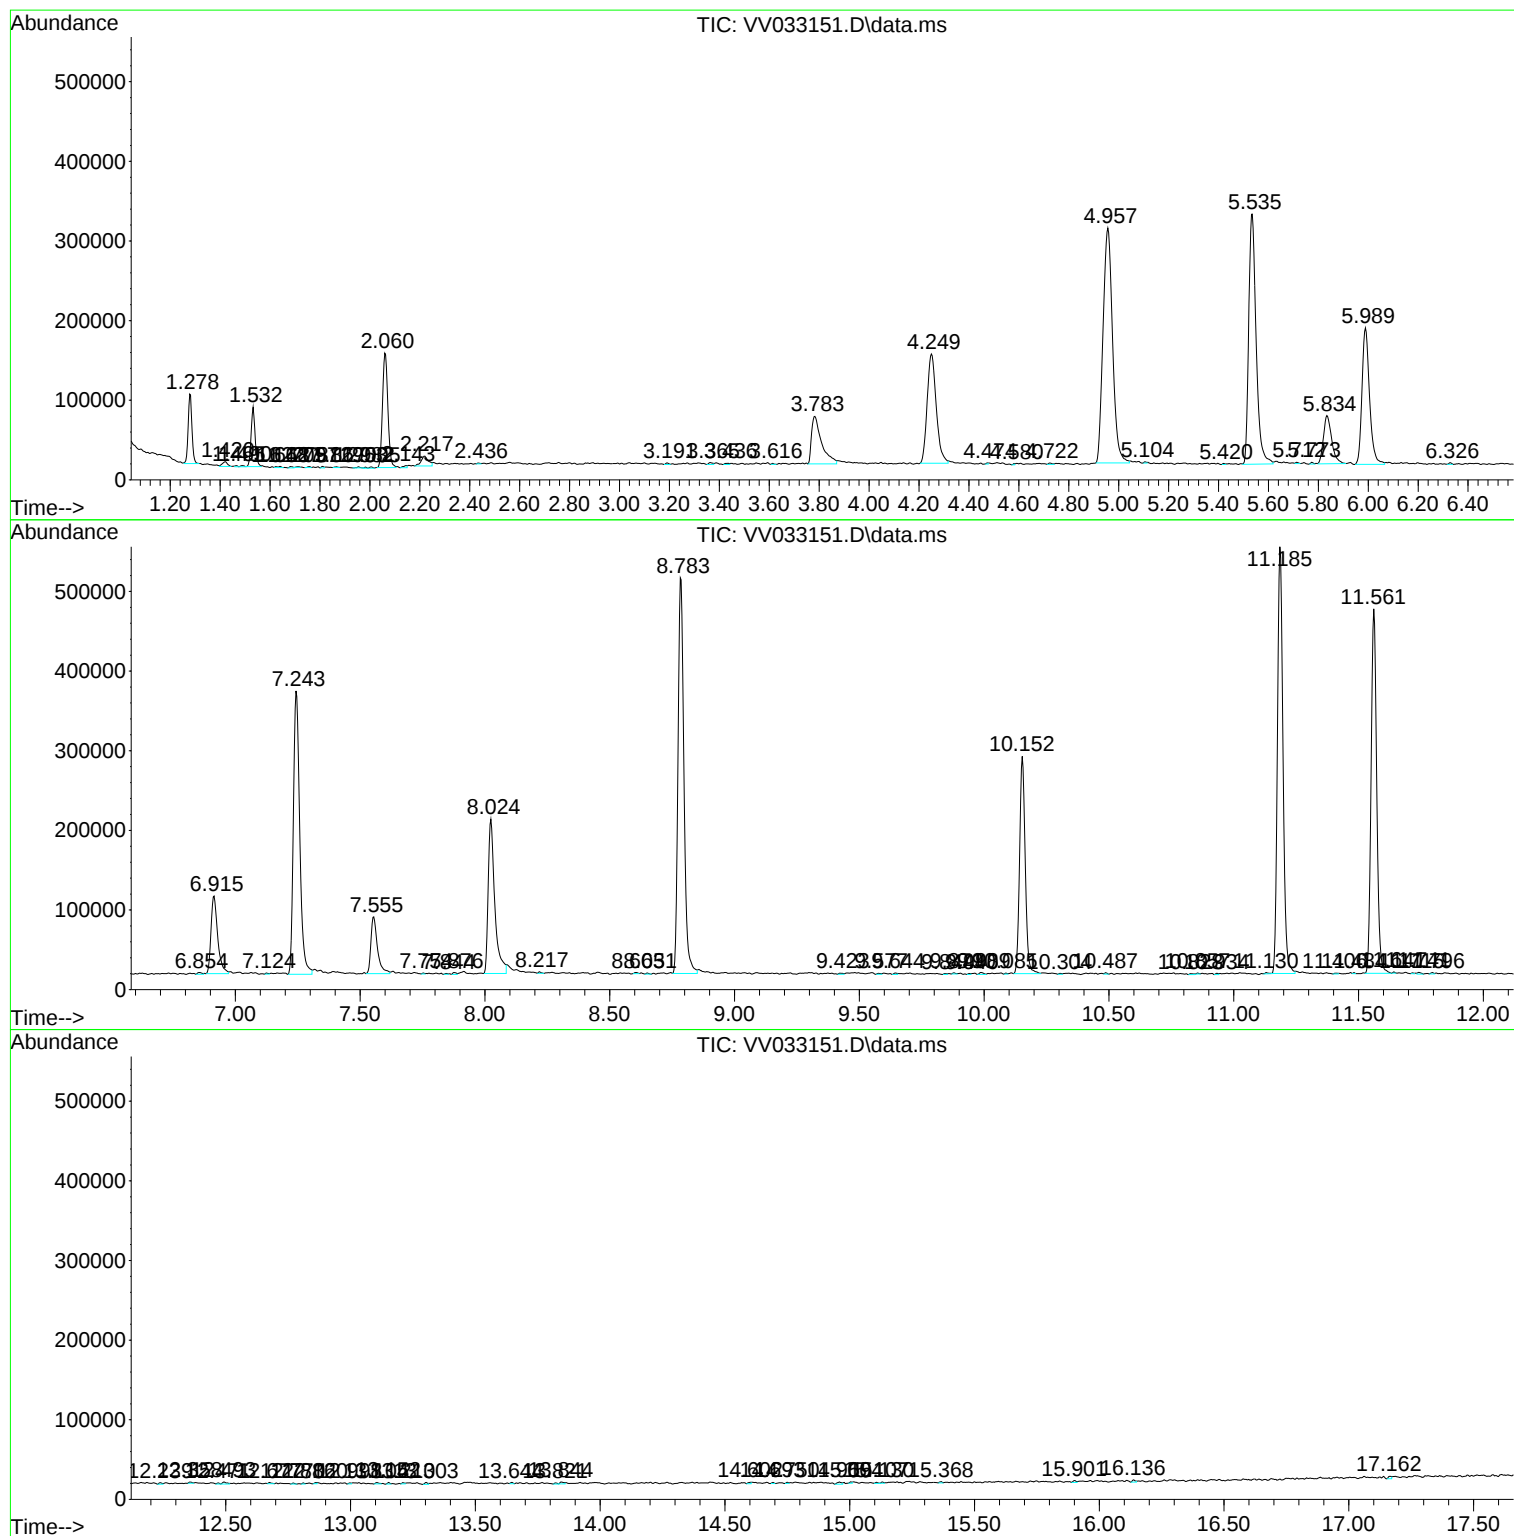

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033151.D
Acq On : 07 Dec 2023 16:58
Operator : SY/MD
Sample : 05645-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G68

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033151.D
Acq On : 07 Dec 2023 16:58
Operator : SY/MD
Sample : 05645-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G68

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------