

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033153.D
 Acq On : 07 Dec 2023 17:45
 Operator : SY/MD
 Sample : 05645-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G71

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VV033153.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	84	rVB	87782	92052	11.39%	1.315%
2	1.320	84	87	93	rVB2	2776	2552	0.32%	0.036%
3	1.349	93	96	98	rVB2	1224	622	0.08%	0.009%
4	1.420	110	118	126	rVB2	7006	11170	1.38%	0.160%
5	1.532	144	153	165	rBV	69876	83598	10.35%	1.194%
6	1.577	165	167	170	rVV2	1706	1058	0.13%	0.015%
7	1.593	170	172	177	rVB2	1275	804	0.10%	0.011%
8	1.619	177	180	186	rVB2	975	709	0.09%	0.010%
9	1.770	223	227	228	rBV	1245	849	0.11%	0.012%
10	1.854	250	253	256	rBV2	858	611	0.08%	0.009%
11	1.876	256	260	263	rVV	1339	1071	0.13%	0.015%
12	1.892	263	265	268	rVV2	1194	802	0.10%	0.011%
13	1.921	271	274	280	rVB3	1181	949	0.12%	0.014%
14	1.963	283	287	290	rBV3	950	792	0.10%	0.011%
15	2.008	296	301	305	rBV	1187	1152	0.14%	0.016%
16	2.060	305	317	332	rVV	144399	215508	26.67%	3.078%
17	2.111	332	333	338	rVB3	1411	892	0.11%	0.013%
18	2.175	341	353	355	rBV	2703	4440	0.55%	0.063%
19	2.220	358	367	382	rBV3	11457	25862	3.20%	0.369%
20	2.346	400	406	414	rBV	1805	3140	0.39%	0.045%
21	2.384	415	418	420	rBV2	1343	944	0.12%	0.013%
22	2.446	434	437	442	rBV3	1385	1427	0.18%	0.020%
23	2.497	449	453	455	rBV	1255	1040	0.13%	0.015%
24	2.732	523	526	536	rVB	2698	2898	0.36%	0.041%
25	2.783	536	542	543	rBV	1764	1883	0.23%	0.027%
26	2.844	555	561	562	rBV	1256	1360	0.17%	0.019%
27	3.027	614	618	622	rBV2	1827	2068	0.26%	0.030%
28	3.175	660	664	665	rBV	1494	1094	0.14%	0.016%
29	3.365	719	723	724	rBV	2060	1291	0.16%	0.018%
30	3.400	732	734	737	rVB	1499	779	0.10%	0.011%
31	3.735	833	838	841	rBV	1373	1281	0.16%	0.018%
32	3.780	844	852	886	rVV	59719	167876	20.78%	2.398%
33	4.114	951	956	958	rBV	1773	1796	0.22%	0.026%
34	4.249	980	998	1021	rBV	138284	353029	43.69%	5.042%
35	4.667	1126	1128	1133	rBV2	1095	602	0.07%	0.009%
36	4.860	1186	1188	1193	rBV3	1133	1028	0.13%	0.015%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120723\
 Data File : VW033153.D
 Acq On : 07 Dec 2023 17:45
 Operator : SY/MD
 Sample : 05645-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G71

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	4.957	1202	1218	1245	rBV2	293515	787243	97.43%	11.244%
38	5.333	1330	1335	1338	rBV	1903	1891	0.23%	0.027%
39	5.436	1364	1367	1369	rBV2	1210	785	0.10%	0.011%
40	5.532	1386	1397	1417	rBV	306153	627754	77.69%	8.966%
41	5.834	1480	1491	1509	rBV3	69300	152306	18.85%	2.175%
42	5.989	1526	1539	1566	rBV	169432	353935	43.80%	5.055%
43	6.291	1630	1633	1637	rBV	1709	952	0.12%	0.014%
44	6.873	1811	1814	1817	rVV	1328	1191	0.15%	0.017%
45	6.915	1817	1827	1845	rVV	94449	175814	21.76%	2.511%
46	7.043	1864	1867	1871	rVB2	1241	1001	0.12%	0.014%
47	7.143	1895	1898	1901	rBV2	1298	1114	0.14%	0.016%
48	7.243	1919	1929	1951	rBV	354623	622845	77.08%	8.896%
49	7.449	1991	1993	1998	rBV	1473	1069	0.13%	0.015%
50	7.555	2017	2026	2047	rBV	70716	126288	15.63%	1.804%
51	7.703	2069	2072	2076	rBV	1709	1127	0.14%	0.016%
52	7.818	2106	2108	2111	rVB2	1249	677	0.08%	0.010%
53	7.834	2111	2113	2118	rBV	1394	1494	0.18%	0.021%
54	8.024	2163	2172	2202	rBV	189491	366376	45.34%	5.233%
55	8.403	2288	2290	2292	rVB2	1456	598	0.07%	0.009%
56	8.432	2296	2299	2307	rVB2	2191	2323	0.29%	0.033%
57	8.600	2348	2351	2354	rBV	1564	988	0.12%	0.014%
58	8.622	2355	2358	2361	rBV	1376	1267	0.16%	0.018%
59	8.683	2374	2377	2382	rBV	1248	829	0.10%	0.012%
60	8.783	2398	2408	2437	rBV	485210	800934	99.12%	11.439%
61	9.047	2487	2490	2496	rBV4	1284	1353	0.17%	0.019%
62	9.346	2580	2583	2586	rVB2	1222	777	0.10%	0.011%
63	9.558	2643	2649	2651	rBV	1612	1832	0.23%	0.026%
64	9.738	2700	2705	2709	rBV	1837	2030	0.25%	0.029%
65	9.764	2710	2713	2715	rBV	1406	1119	0.14%	0.016%
66	10.018	2790	2792	2794	rBV	1051	650	0.08%	0.009%
67	10.153	2823	2834	2854	rBV2	263897	415901	51.47%	5.940%
68	10.284	2872	2875	2878	rBV	1307	777	0.10%	0.011%
69	10.464	2928	2931	2933	rBV	1052	604	0.07%	0.009%
70	10.921	3069	3073	3074	rBV2	2057	1401	0.17%	0.020%
71	11.046	3110	3112	3118	rVB	1688	1227	0.15%	0.018%
72	11.185	3144	3155	3175	rBV	529691	808025	100.00%	11.541%
73	11.355	3205	3208	3210	rBV	1656	1147	0.14%	0.016%
74	11.481	3244	3247	3248	rBV2	1029	673	0.08%	0.010%
75	11.561	3260	3272	3297	rBV	452498	711628	88.07%	10.164%
76	12.271	3490	3493	3497	rVB	1197	897	0.11%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033153.D
 Acq On : 07 Dec 2023 17:45
 Operator : SY/MD
 Sample : 05645-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G71

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	12.497	3561	3563	3567	rBV	1136	905	0.11%	0.013%
78	12.519	3567	3570	3577	rVV2	1239	1291	0.16%	0.018%
79	13.066	3736	3740	3743	rBV2	2172	2197	0.27%	0.031%
80	13.223	3786	3789	3794	rBV	1978	2087	0.26%	0.030%
81	13.590	3899	3903	3908	rBV	1472	1512	0.19%	0.022%
82	13.693	3933	3935	3938	rVB	1188	613	0.08%	0.009%
83	13.818	3971	3974	3981	rBV	1504	1644	0.20%	0.023%
84	13.963	4016	4019	4021	rVB	1583	914	0.11%	0.013%
85	14.030	4036	4040	4046	rBV	2097	2485	0.31%	0.035%
86	14.220	4096	4099	4102	rBV	1581	1293	0.16%	0.018%
87	14.265	4111	4113	4119	rBV	1303	1067	0.13%	0.015%
88	14.410	4155	4158	4160	rBV	1467	937	0.12%	0.013%
89	14.519	4188	4192	4196	rBV2	1789	2035	0.25%	0.029%
90	14.709	4248	4251	4255	rBV2	1601	1309	0.16%	0.019%
91	14.918	4314	4316	4319	rBV	1627	762	0.09%	0.011%
92	14.985	4335	4337	4342	rBV	1363	1032	0.13%	0.015%
93	15.165	4390	4393	4394	rBV	1855	1040	0.13%	0.015%
94	15.304	4434	4436	4438	rBV2	1290	655	0.08%	0.009%
95	15.721	4564	4566	4572	rBV4	1468	1221	0.15%	0.017%
96	15.757	4574	4577	4583	rVB	2373	2329	0.29%	0.033%
97	15.786	4584	4586	4588	rBV	1398	744	0.09%	0.011%
98	15.802	4588	4591	4594	rBV5	1675	1185	0.15%	0.017%
99	16.049	4665	4668	4671	rBV	1871	1287	0.16%	0.018%
100	16.165	4701	4704	4706	rBV3	1787	1161	0.14%	0.017%


Sum of corrected areas: 7001576

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033153.D
Acq On : 07 Dec 2023 17:45
Operator : SY/MD
Sample : 05645-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G71

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

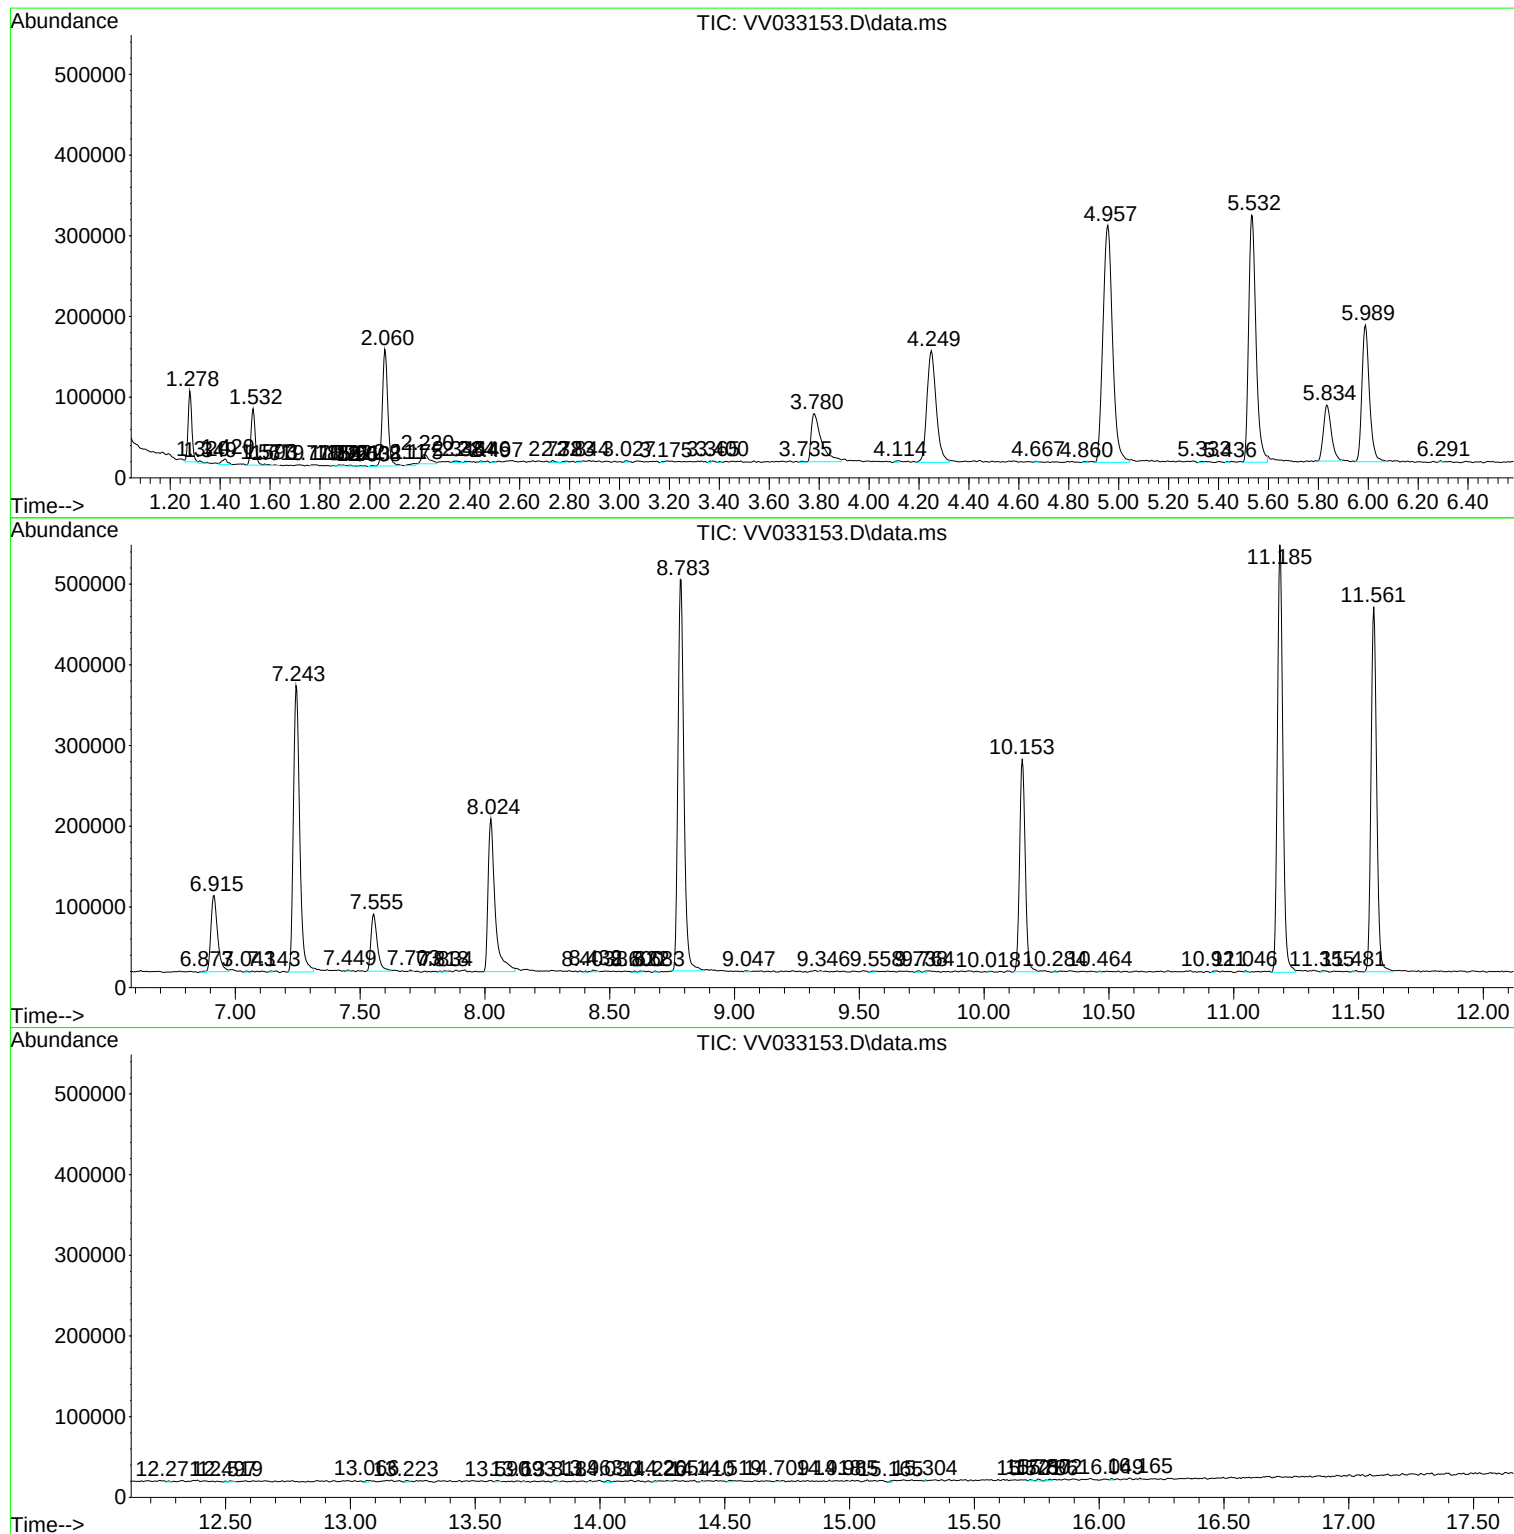

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033153.D
Acq On : 07 Dec 2023 17:45
Operator : SY/MD
Sample : 05645-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G71

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033153.D
Acq On : 07 Dec 2023 17:45
Operator : SY/MD
Sample : 05645-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G71

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc