

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033154.D
 Acq On : 07 Dec 2023 18:08
 Operator : SY/MD
 Sample : 05645-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G73

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M

Title : VOC Analysis

Signal : TIC: VV033154.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	93	rVB	86191	96232	11.70%	1.414%
2	1.417	111	117	124	rVV3	6055	7696	0.94%	0.113%
3	1.458	128	130	132	rVB	823	344	0.04%	0.005%
4	1.500	138	143	146	rBV3	1843	1685	0.20%	0.025%
5	1.532	146	153	166	rVV	67919	81802	9.95%	1.202%
6	1.600	170	174	177	rVB2	900	816	0.10%	0.012%
7	1.635	180	185	188	rBV	1505	1260	0.15%	0.019%
8	1.667	191	195	199	rBV2	1057	876	0.11%	0.013%
9	1.719	207	211	216	rBV3	1045	1149	0.14%	0.017%
10	1.745	216	219	222	rVV2	609	414	0.05%	0.006%
11	1.774	226	228	231	rVB2	882	548	0.07%	0.008%
12	1.831	244	246	248	rVB3	185	70	0.01%	0.001%
13	1.864	248	256	258	rBV3	1354	1775	0.22%	0.026%
14	1.880	258	261	264	rVV2	636	439	0.05%	0.006%
15	1.921	272	274	278	rVB2	934	671	0.08%	0.010%
16	1.941	278	280	286	rVB	1241	1274	0.15%	0.019%
17	1.970	286	289	294	rBV3	1215	1593	0.19%	0.023%
18	1.999	296	298	304	rVB3	1234	937	0.11%	0.014%
19	2.060	304	317	332	rBV	141500	209951	25.53%	3.086%
20	2.114	332	334	339	rVB4	2212	1954	0.24%	0.029%
21	2.150	339	345	346	rBV2	1938	1863	0.23%	0.027%
22	2.182	346	355	358	rBV	2939	3876	0.47%	0.057%
23	2.220	358	367	382	rBV2	8763	20391	2.48%	0.300%
24	2.368	410	413	418	rVB	2461	1994	0.24%	0.029%
25	2.413	424	427	431	rBV	1145	835	0.10%	0.012%
26	2.645	496	499	502	rBV	1697	1203	0.15%	0.018%
27	3.050	621	625	633	rBV	2059	2602	0.32%	0.038%
28	3.098	638	640	642	rBV	909	508	0.06%	0.007%
29	3.230	678	681	686	rBV2	1500	1676	0.20%	0.025%
30	3.301	700	703	705	rVB	1374	782	0.10%	0.011%
31	3.542	775	778	782	rBV	1535	1142	0.14%	0.017%
32	3.732	833	837	842	rBV	1628	2072	0.25%	0.030%
33	3.780	844	852	875	rBV	56406	153925	18.72%	2.262%
34	4.140	961	964	969	rBV	1089	930	0.11%	0.014%
35	4.195	979	981	983	rBV	1009	630	0.08%	0.009%
36	4.249	983	998	1025	rVV2	132634	348935	42.43%	5.128%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120723\
 Data File : VW033154.D
 Acq On : 07 Dec 2023 18:08
 Operator : SY/MD
 Sample : 05645-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G73

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	4.429	1051	1054	1058	rBV3	1326	1159	0.14%	0.017%
38	4.487	1068	1072	1073	rBV2	1330	940	0.11%	0.014%
39	4.574	1097	1099	1101	rBV2	955	493	0.06%	0.007%
40	4.613	1108	1111	1115	rBV	1485	1196	0.15%	0.018%
41	4.844	1180	1183	1186	rBV	1503	1084	0.13%	0.016%
42	4.957	1202	1218	1246	rBV2	289751	774459	94.17%	11.382%
43	5.532	1386	1397	1425	rBV	303395	632751	76.94%	9.300%
44	5.696	1445	1448	1450	rBV	1621	1067	0.13%	0.016%
45	5.831	1482	1490	1500	rVB6	10437	19252	2.34%	0.283%
46	5.989	1527	1539	1565	rVB	166496	348578	42.39%	5.123%
47	6.082	1566	1568	1571	rBV	1274	834	0.10%	0.012%
48	6.362	1651	1655	1658	rBV	1690	1418	0.17%	0.021%
49	6.732	1768	1770	1773	rBV2	946	684	0.08%	0.010%
50	6.777	1781	1784	1786	rBV	1379	792	0.10%	0.012%
51	6.912	1816	1826	1847	rBV	95443	181384	22.06%	2.666%
52	7.243	1916	1929	1948	rBV	342385	614860	74.77%	9.037%
53	7.519	2012	2015	2017	rBV	1671	874	0.11%	0.013%
54	7.555	2017	2026	2044	rBV3	71341	126911	15.43%	1.865%
55	7.706	2071	2073	2074	rBV	1182	556	0.07%	0.008%
56	7.876	2123	2126	2129	rVB	1838	1032	0.13%	0.015%
57	7.989	2158	2161	2163	rBV	1753	1219	0.15%	0.018%
58	8.024	2163	2172	2207	rVV	190614	367542	44.69%	5.402%
59	8.223	2232	2234	2238	rVB	1782	1091	0.13%	0.016%
60	8.375	2278	2281	2283	rBV	1486	786	0.10%	0.012%
61	8.519	2323	2326	2329	rBV	1663	1110	0.13%	0.016%
62	8.783	2398	2408	2430	rBV	491599	801962	97.52%	11.787%
63	9.021	2480	2482	2485	rVB	1345	693	0.08%	0.010%
64	9.162	2524	2526	2528	rBV	1087	561	0.07%	0.008%
65	9.378	2590	2593	2595	rBV	1281	911	0.11%	0.013%
66	9.709	2694	2696	2699	rBV	1112	725	0.09%	0.011%
67	9.776	2714	2717	2728	rBV	1465	2050	0.25%	0.030%
68	9.821	2728	2731	2733	rBV	1287	914	0.11%	0.013%
69	10.098	2814	2817	2819	rBV2	1363	864	0.11%	0.013%
70	10.153	2824	2834	2851	rVV	264759	417080	50.72%	6.130%
71	10.326	2885	2888	2890	rBV	1646	1065	0.13%	0.016%
72	10.506	2942	2944	2947	rBV	1256	835	0.10%	0.012%
73	10.976	3087	3090	3094	rBV	2017	1670	0.20%	0.025%
74	11.001	3095	3098	3100	rBV2	1405	1018	0.12%	0.015%
75	11.185	3144	3155	3172	rBV	536494	822376	100.00%	12.087%
76	11.561	3261	3272	3292	rBV	449794	696734	84.72%	10.240%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033154.D
 Acq On : 07 Dec 2023 18:08
 Operator : SY/MD
 Sample : 05645-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G73

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M

Title : VOC Analysis

77	11.789	3340	3343	3347	rVB2	1482	1009	0.12%	0.015%
78	12.053	3420	3425	3427	rBV2	1330	1417	0.17%	0.021%
79	12.355	3516	3519	3522	rBV	1314	1161	0.14%	0.017%
80	12.503	3563	3565	3568	rBV	1011	641	0.08%	0.009%
81	12.625	3600	3603	3607	rBV	1707	1534	0.19%	0.023%
82	13.313	3813	3817	3824	rBV2	2077	2549	0.31%	0.037%
83	13.484	3867	3870	3873	rBV	1855	1088	0.13%	0.016%
84	13.606	3905	3908	3911	rBV2	1247	973	0.12%	0.014%
85	14.297	4121	4123	4125	rBV	1159	543	0.07%	0.008%
86	14.718	4251	4254	4257	rVB	1805	1085	0.13%	0.016%
87	15.242	4413	4417	4420	rBV	2960	2302	0.28%	0.034%
88	15.265	4421	4424	4431	rVB2	2179	2264	0.28%	0.033%
89	16.873	4922	4924	4925	rBV	2452	1097	0.13%	0.016%




Sum of corrected areas: 6804043

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033154.D
Acq On : 07 Dec 2023 18:08
Operator : SY/MD
Sample : 05645-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G73

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

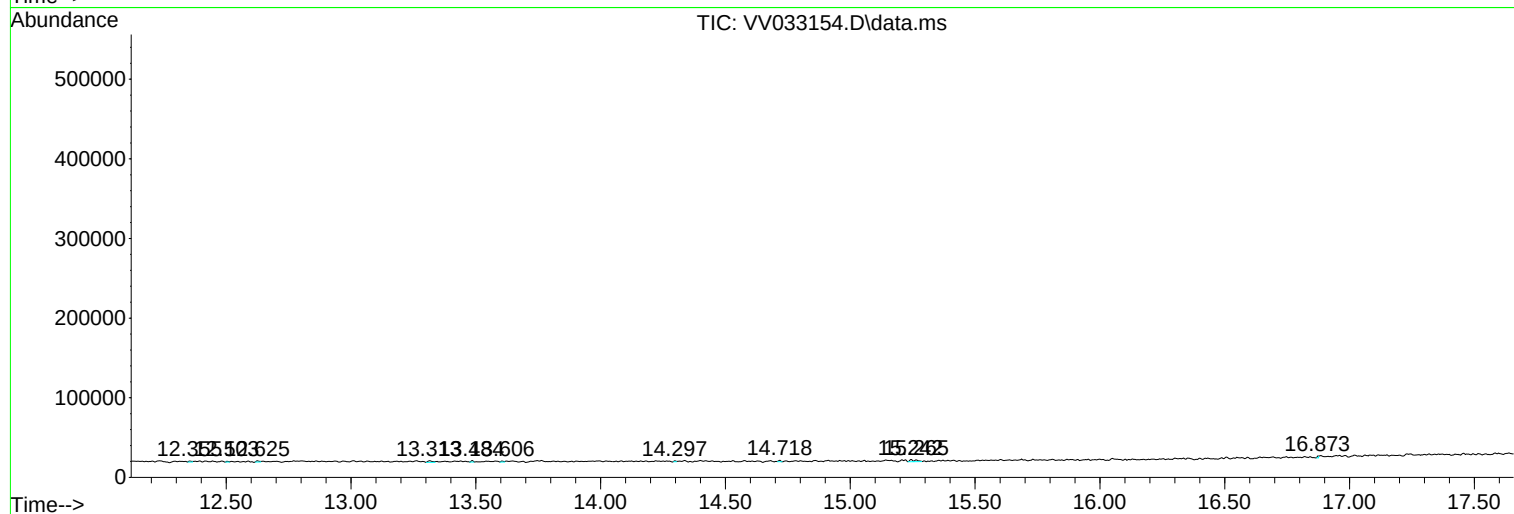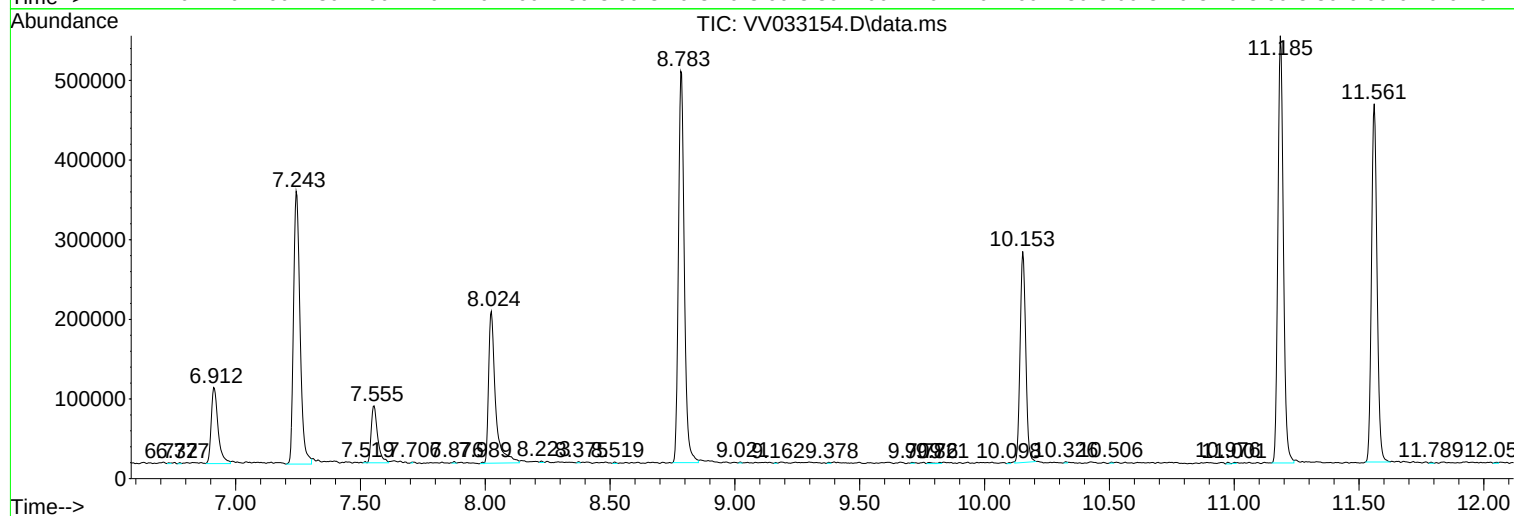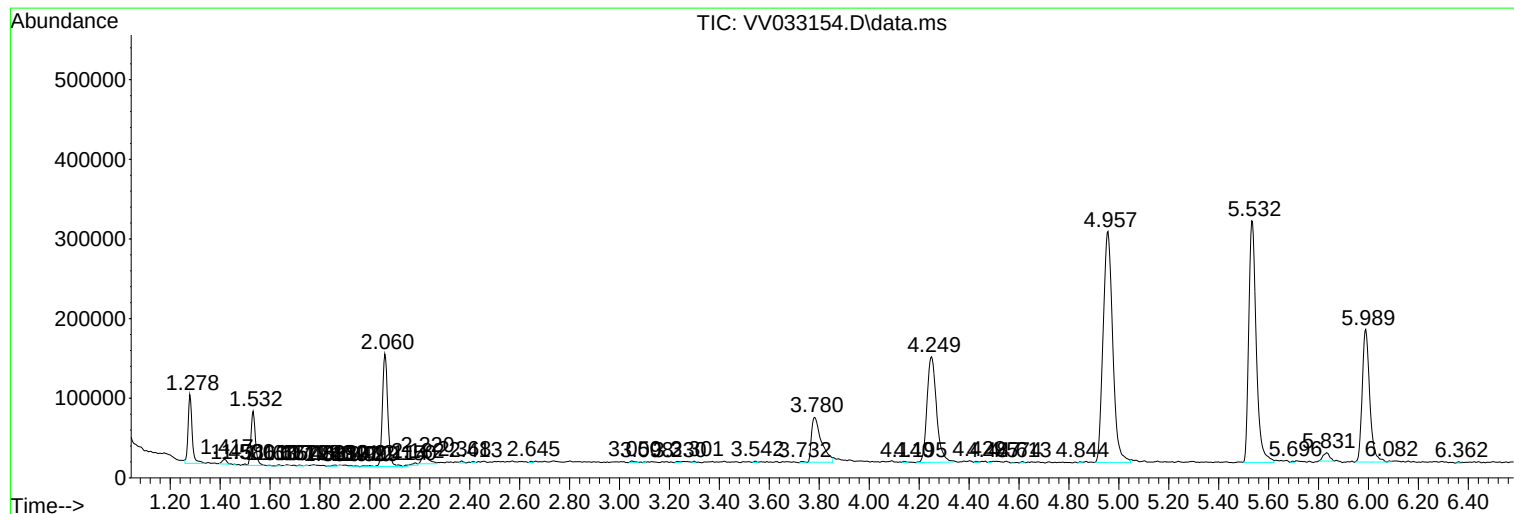

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033154.D
Acq On : 07 Dec 2023 18:08
Operator : SY/MD
Sample : 05645-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G73

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033154.D
Acq On : 07 Dec 2023 18:08
Operator : SY/MD
Sample : 05645-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G73

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------