

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033159.D
 Acq On : 07 Dec 2023 20:27
 Operator : SY/MD
 Sample : VV1207WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK236

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VV033159.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	86	rVB	93490	99862	11.88%	1.385%
2	1.420	109	118	125	rVB3	6185	9952	1.18%	0.138%
3	1.462	126	131	134	rVV5	867	1010	0.12%	0.014%
4	1.481	134	137	143	rVV3	1843	2368	0.28%	0.033%
5	1.532	145	153	166	rVV	75801	89727	10.68%	1.244%
6	1.581	166	168	173	rVB2	1700	1096	0.13%	0.015%
7	1.728	211	214	217	rVB3	1060	748	0.09%	0.010%
8	1.767	220	226	235	rVB3	1694	2487	0.30%	0.034%
9	1.819	235	242	244	rBV2	1494	1415	0.17%	0.020%
10	1.921	272	274	282	rVB6	1257	1183	0.14%	0.016%
11	2.060	306	317	335	rVB	151900	223628	26.61%	3.101%
12	2.153	341	346	347	rBV	2079	1619	0.19%	0.022%
13	2.169	347	351	352	rBV	1373	930	0.11%	0.013%
14	2.211	361	364	368	rBV	1582	1690	0.20%	0.023%
15	2.381	414	417	422	rBV2	1482	1160	0.14%	0.016%
16	2.452	432	439	450	rVB4	3071	6664	0.79%	0.092%
17	2.773	532	539	542	rBV2	2119	2906	0.35%	0.040%
18	3.095	637	639	642	rBV2	1180	734	0.09%	0.010%
19	3.468	753	755	761	rVB	1504	995	0.12%	0.014%
20	3.780	844	852	875	rBV	59544	152983	18.21%	2.121%
21	4.008	920	923	927	rVB	2522	1758	0.21%	0.024%
22	4.031	927	930	932	rBV	1744	1298	0.15%	0.018%
23	4.101	949	952	956	rVB	1710	1202	0.14%	0.017%
24	4.182	975	977	981	rVB2	1455	989	0.12%	0.014%
25	4.249	984	998	1019	rVV	144324	359715	42.81%	4.988%
26	4.346	1026	1028	1038	rVB	1972	2231	0.27%	0.031%
27	4.777	1158	1162	1165	rBV2	1261	1227	0.15%	0.017%
28	4.796	1165	1168	1172	rVB	2281	1703	0.20%	0.024%
29	4.818	1172	1175	1178	rBV	1283	852	0.10%	0.012%
30	4.957	1202	1218	1245	rBV3	313631	840329	100.00%	11.653%
31	5.275	1315	1317	1321	rBV	1137	718	0.09%	0.010%
32	5.532	1386	1397	1423	rBV	312619	644115	76.65%	8.932%
33	5.831	1479	1490	1500	rBV5	13592	28884	3.44%	0.401%
34	5.989	1527	1539	1560	rBV2	179550	369457	43.97%	5.123%
35	6.214	1607	1609	1616	rVB	2237	1952	0.23%	0.027%
36	6.458	1682	1685	1689	rBV	1269	1011	0.12%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033159.D
 Acq On : 07 Dec 2023 20:27
 Operator : SY/MD
 Sample : VV1207WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK236

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	6.516	1700	1703	1706	rBV2	1698	1302	0.15%	0.018%
38	6.706	1759	1762	1766	rBV	1218	1046	0.12%	0.015%
39	6.912	1817	1826	1851	rBV	103536	198380	23.61%	2.751%
40	7.027	1859	1862	1868	rBV	2038	2295	0.27%	0.032%
41	7.243	1918	1929	1955	rBV	370616	659067	78.43%	9.140%
42	7.551	2017	2025	2043	rBV	75338	133658	15.91%	1.853%
43	7.912	2130	2137	2146	rBV6	3856	7130	0.85%	0.099%
44	7.963	2151	2153	2157	rVB	1661	1141	0.14%	0.016%
45	8.024	2163	2172	2206	rBV	207909	400677	47.68%	5.556%
46	8.387	2282	2285	2289	rBV	1766	1213	0.14%	0.017%
47	8.686	2375	2378	2382	rVB2	1494	1299	0.15%	0.018%
48	8.783	2398	2408	2429	rBV	488905	807120	96.05%	11.193%
49	8.989	2469	2472	2476	rBV3	990	843	0.10%	0.012%
50	9.072	2495	2498	2501	rBV2	1336	1222	0.15%	0.017%
51	9.149	2519	2522	2525	rBV	1406	951	0.11%	0.013%
52	9.220	2541	2544	2549	rBV	1295	818	0.10%	0.011%
53	9.272	2557	2560	2563	rBV	1478	1028	0.12%	0.014%
54	9.384	2592	2595	2600	rBV	919	760	0.09%	0.011%
55	9.410	2601	2603	2608	rVV	1093	723	0.09%	0.010%
56	9.455	2613	2617	2625	rVB	1646	2013	0.24%	0.028%
57	9.490	2626	2628	2631	rBV	1135	747	0.09%	0.010%
58	9.580	2653	2656	2660	rVB	1630	1053	0.13%	0.015%
59	9.776	2715	2717	2720	rBV	1348	769	0.09%	0.011%
60	9.963	2773	2775	2777	rBV2	1491	918	0.11%	0.013%
61	10.085	2809	2813	2818	rBV	1794	1926	0.23%	0.027%
62	10.153	2823	2834	2848	rBV	282442	439736	52.33%	6.098%
63	10.391	2905	2908	2914	rVV	1379	1364	0.16%	0.019%
64	10.423	2915	2918	2922	rVB	1438	888	0.11%	0.012%
65	10.545	2953	2956	2965	rVB	1656	2629	0.31%	0.036%
66	10.728	3010	3013	3018	rBV	1540	1319	0.16%	0.018%
67	10.792	3030	3033	3037	rBV	1238	1045	0.12%	0.014%
68	10.992	3092	3095	3098	rBV	1179	900	0.11%	0.012%
69	11.130	3131	3138	3142	rBV2	2949	3179	0.38%	0.044%
70	11.185	3145	3155	3177	rBV	546622	840284	99.99%	11.653%
71	11.561	3261	3272	3290	rBV	483263	750286	89.28%	10.405%
72	11.818	3347	3352	3355	rBV	2027	1779	0.21%	0.025%
73	12.005	3407	3410	3417	rBV	1940	2345	0.28%	0.033%
74	12.516	3563	3569	3572	rBV	2333	2732	0.33%	0.038%
75	12.538	3573	3576	3580	rVB	1915	1377	0.16%	0.019%
76	12.564	3580	3584	3586	rBV	1291	1225	0.15%	0.017%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033159.D
 Acq On : 07 Dec 2023 20:27
 Operator : SY/MD
 Sample : VV1207WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK236

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	12.590	3587	3592	3603	rVB5	3274	5760	0.69%	0.080%
78	12.670	3614	3617	3620	rBV	1689	1363	0.16%	0.019%
79	13.207	3778	3784	3793	rVB6	5235	7599	0.90%	0.105%
80	13.313	3811	3817	3821	rBV	2350	3116	0.37%	0.043%
81	13.397	3840	3843	3847	rVB	2048	1425	0.17%	0.020%
82	13.445	3851	3858	3866	rBV	14896	21416	2.55%	0.297%
83	13.545	3885	3889	3893	rVB2	1481	1433	0.17%	0.020%
84	13.689	3925	3934	3940	rBV4	5857	9319	1.11%	0.129%
85	13.754	3950	3954	3955	rBV	1417	1013	0.12%	0.014%
86	13.947	4011	4014	4018	rVB2	1492	1208	0.14%	0.017%
87	14.140	4071	4074	4076	rBV2	1451	1021	0.12%	0.014%
88	14.271	4112	4115	4118	rBV2	1347	919	0.11%	0.013%
89	14.458	4169	4173	4176	rBV	1908	1815	0.22%	0.025%
90	14.583	4209	4212	4214	rBV	1090	812	0.10%	0.011%
91	14.747	4260	4263	4264	rBV	1462	892	0.11%	0.012%
92	14.802	4277	4280	4283	rVB2	1880	1228	0.15%	0.017%
93	15.091	4368	4370	4374	rVB	2383	1626	0.19%	0.023%
94	15.304	4434	4436	4440	rVB	2176	1268	0.15%	0.018%
95	15.377	4456	4459	4462	rBV3	1345	836	0.10%	0.012%
96	15.506	4495	4499	4502	rBV5	1787	1819	0.22%	0.025%
97	15.570	4515	4519	4522	rBV2	1782	1783	0.21%	0.025%
98	15.731	4566	4569	4570	rBV4	1514	1026	0.12%	0.014%
99	16.040	4662	4665	4668	rBV3	1997	1342	0.16%	0.019%
100	16.680	4862	4864	4869	rBV2	1961	1333	0.16%	0.018%




Sum of corrected areas: 7211157

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033159.D
Acq On : 07 Dec 2023 20:27
Operator : SY/MD
Sample : VV1207WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK236

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

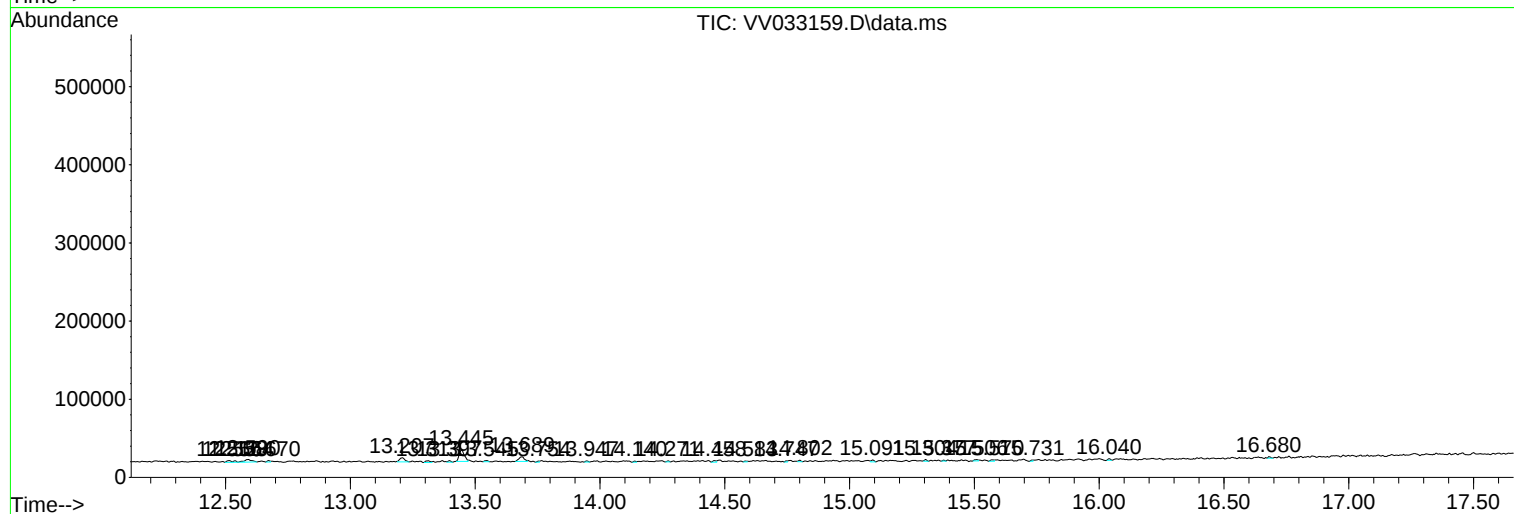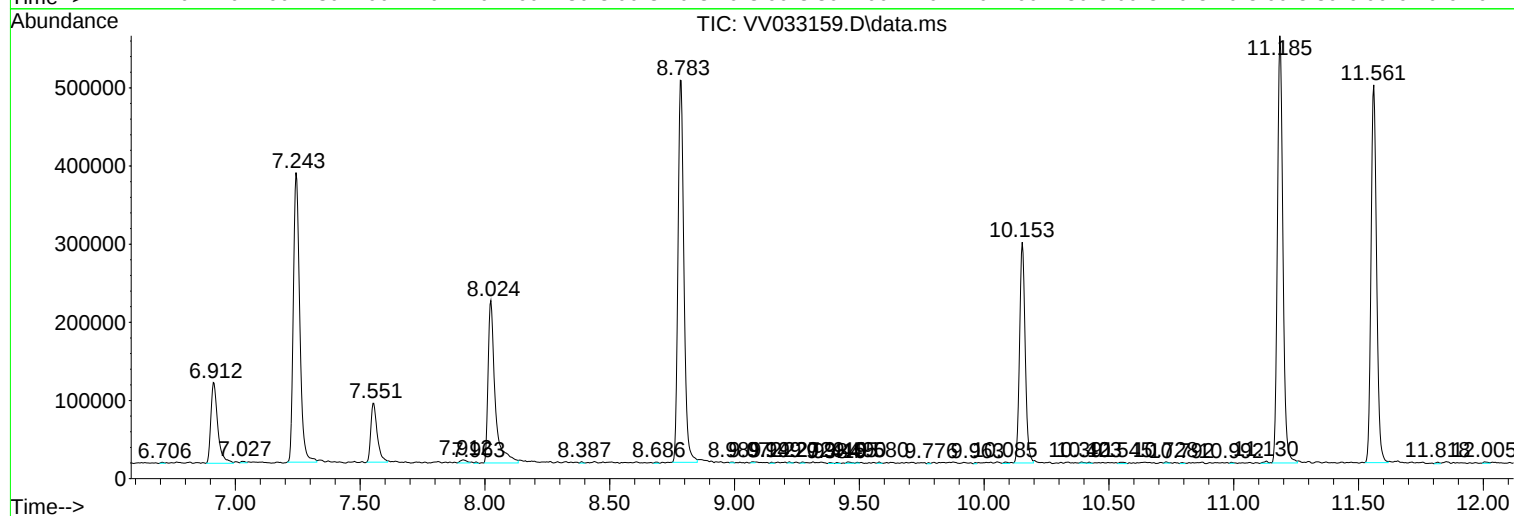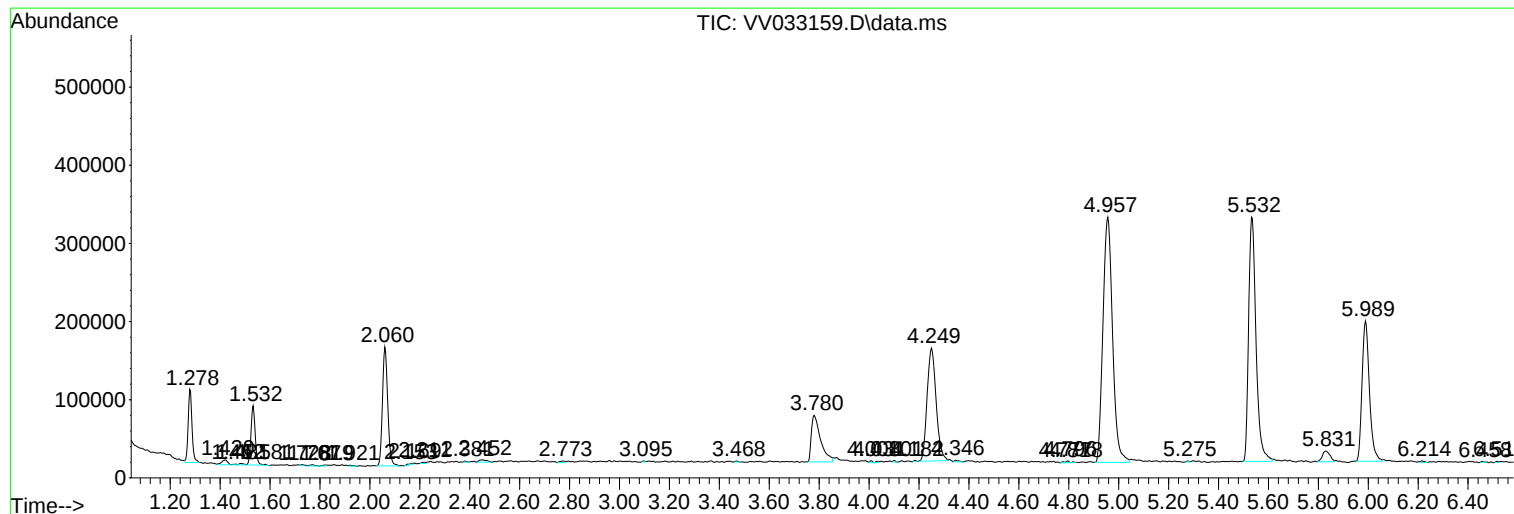

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033159.D
Acq On : 07 Dec 2023 20:27
Operator : SY/MD
Sample : VV1207WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK236

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033159.D
Acq On : 07 Dec 2023 20:27
Operator : SY/MD
Sample : VV1207WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK236

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------