

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033161.D
 Acq On : 07 Dec 2023 21:13
 Operator : SY/MD
 Sample : 05689-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G77

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VV033161.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	86	rVB	84792	89466	4.29%	0.988%
2	1.420	109	118	123	rBV3	5016	6943	0.33%	0.077%
3	1.532	145	153	164	rVB	67147	79373	3.81%	0.877%
4	1.613	173	178	181	rBV2	945	915	0.04%	0.010%
5	1.645	184	188	191	rVV2	1386	1059	0.05%	0.012%
6	1.664	191	194	201	rVV3	1273	1292	0.06%	0.014%
7	1.699	203	205	207	rVB	997	415	0.02%	0.005%
8	1.715	207	210	214	rVB	1184	743	0.04%	0.008%
9	1.748	214	220	222	rVB3	1123	1086	0.05%	0.012%
10	1.764	222	225	228	rBV	1227	907	0.04%	0.010%
11	1.783	229	231	232	rBV	248	104	0.00%	0.001%
12	1.796	232	235	240	rVB2	878	577	0.03%	0.006%
13	1.834	244	247	250	rBV	1259	995	0.05%	0.011%
14	1.854	250	253	254	rBV	806	403	0.02%	0.004%
15	1.867	254	257	260	rVB	1427	889	0.04%	0.010%
16	1.883	260	262	263	rVB	333	114	0.01%	0.001%
17	1.896	263	266	268	rBV3	983	668	0.03%	0.007%
18	1.963	282	287	289	rBV2	1669	1503	0.07%	0.017%
19	1.976	289	291	293	rVB3	870	373	0.02%	0.004%
20	1.998	294	298	304	rVB4	1021	806	0.04%	0.009%
21	2.063	304	318	336	rBV3	172835	288757	13.86%	3.189%
22	2.159	340	348	349	rBV	2581	2629	0.13%	0.029%
23	2.172	349	352	354	rBV	1338	899	0.04%	0.010%
24	2.220	358	367	374	rBV	8403	15258	0.73%	0.169%
25	2.288	386	388	391	rBV2	1225	617	0.03%	0.007%
26	2.371	411	414	418	rVB	1843	1296	0.06%	0.014%
27	2.397	419	422	424	rBV	1226	787	0.04%	0.009%
28	2.413	425	427	429	rBV	1164	615	0.03%	0.007%
29	2.551	468	470	476	rBV2	1256	1068	0.05%	0.012%
30	3.021	613	616	621	rBV2	1268	1268	0.06%	0.014%
31	3.214	674	676	682	rVB	1541	1389	0.07%	0.015%
32	3.500	762	765	768	rBV	1654	981	0.05%	0.011%
33	3.783	844	853	881	rBV3	59682	222535	10.68%	2.458%
34	4.249	983	998	1023	rBV2	131244	338898	16.26%	3.743%
35	4.516	1068	1081	1099	rVB4	25343	68699	3.30%	0.759%
36	4.583	1099	1102	1103	rBV3	1194	765	0.04%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033161.D
 Acq On : 07 Dec 2023 21:13
 Operator : SY/MD
 Sample : 05689-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G77

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	4.619	1110	1113	1115	rBV2	1725	1213	0.06%	0.013%
38	4.661	1124	1126	1133	rVB	1638	1747	0.08%	0.019%
39	4.780	1161	1163	1165	rBV	1471	896	0.04%	0.010%
40	4.847	1181	1184	1187	rBV	1568	975	0.05%	0.011%
41	4.902	1198	1201	1202	rBV	1352	827	0.04%	0.009%
42	4.956	1202	1218	1246	rVV2	287482	774267	37.15%	8.551%
43	5.458	1370	1374	1380	rBV2	1706	2055	0.10%	0.023%
44	5.532	1387	1397	1422	rBV	305504	629504	30.20%	6.952%
45	5.831	1477	1490	1520	rBV	1059875	2084117	100.00%	23.016%
46	5.989	1528	1539	1561	rVB	170187	348467	16.72%	3.848%
47	6.227	1610	1613	1615	rBV2	1104	836	0.04%	0.009%
48	6.262	1621	1624	1629	rBV3	1816	1782	0.09%	0.020%
49	6.915	1817	1827	1849	rBV	96257	183766	8.82%	2.029%
50	7.021	1857	1860	1864	rBV	1758	1428	0.07%	0.016%
51	7.178	1907	1909	1912	rVB	1102	537	0.03%	0.006%
52	7.243	1919	1929	1950	rBV	343816	597583	28.67%	6.599%
53	7.554	2016	2026	2042	rBV	69852	127027	6.10%	1.403%
54	7.898	2131	2133	2135	rBV	1361	799	0.04%	0.009%
55	8.024	2163	2172	2203	rBV	186244	356131	17.09%	3.933%
56	8.275	2248	2250	2253	rVB	1065	452	0.02%	0.005%
57	8.361	2274	2277	2281	rBV3	1138	1049	0.05%	0.012%
58	8.410	2289	2292	2294	rBV	979	513	0.02%	0.006%
59	8.497	2316	2319	2321	rBV	1235	689	0.03%	0.008%
60	8.554	2334	2337	2339	rBV	1354	938	0.05%	0.010%
61	8.783	2398	2408	2436	rBV	488026	802373	38.50%	8.861%
62	9.239	2545	2550	2552	rBV	1650	1685	0.08%	0.019%
63	9.519	2635	2637	2640	rVB2	1048	482	0.02%	0.005%
64	9.751	2706	2709	2711	rBV	1341	937	0.04%	0.010%
65	9.943	2766	2769	2773	rBV	1334	1184	0.06%	0.013%
66	9.992	2781	2784	2790	rVB	1281	1019	0.05%	0.011%
67	10.091	2813	2815	2822	rVB	1408	1267	0.06%	0.014%
68	10.152	2822	2834	2854	rBV	271988	426820	20.48%	4.714%
69	10.416	2912	2916	2921	rBV	1850	2236	0.11%	0.025%
70	10.625	2978	2981	2985	rVB	2089	1553	0.07%	0.017%
71	10.651	2986	2989	2990	rBV	1266	826	0.04%	0.009%
72	10.808	3034	3038	3043	rVB	1998	2120	0.10%	0.023%
73	10.850	3048	3051	3054	rVV	1381	1034	0.05%	0.011%
74	10.950	3079	3082	3084	rBV	1474	1030	0.05%	0.011%
75	11.078	3119	3122	3123	rBV	1065	554	0.03%	0.006%
76	11.120	3133	3135	3137	rBV	1168	554	0.03%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033161.D
 Acq On : 07 Dec 2023 21:13
 Operator : SY/MD
 Sample : 05689-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G77

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	11.185	3145	3155	3175	rBV	525129	822397	39.46%	9.082%
78	11.561	3260	3272	3291	rBV	446307	704903	33.82%	7.785%
79	11.731	3322	3325	3329	rVB	1596	843	0.04%	0.009%
80	11.824	3351	3354	3358	rBV2	1481	991	0.05%	0.011%
81	12.078	3429	3433	3437	rBV	1719	1790	0.09%	0.020%
82	12.194	3465	3469	3473	rBV	1966	1465	0.07%	0.016%
83	12.310	3500	3505	3507	rBV2	1825	1793	0.09%	0.020%
84	12.516	3566	3569	3572	rBV	1589	1282	0.06%	0.014%
85	12.680	3618	3620	3622	rBV	1010	576	0.03%	0.006%
86	12.705	3625	3628	3632	rVV	1954	1613	0.08%	0.018%
87	13.082	3742	3745	3748	rVB	1655	965	0.05%	0.011%
88	13.159	3765	3769	3773	rBV	1490	1467	0.07%	0.016%
89	13.451	3856	3860	3871	rVB4	5299	7739	0.37%	0.085%
90	13.496	3871	3874	3878	rBV	1198	925	0.04%	0.010%
91	13.522	3879	3882	3884	rBV	1246	869	0.04%	0.010%
92	13.689	3929	3934	3943	rVB4	3190	5171	0.25%	0.057%
93	14.323	4127	4131	4137	rBV2	1637	1985	0.10%	0.022%




Sum of corrected areas: 9055138

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033161.D
Acq On : 07 Dec 2023 21:13
Operator : SY/MD
Sample : 05689-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G77

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

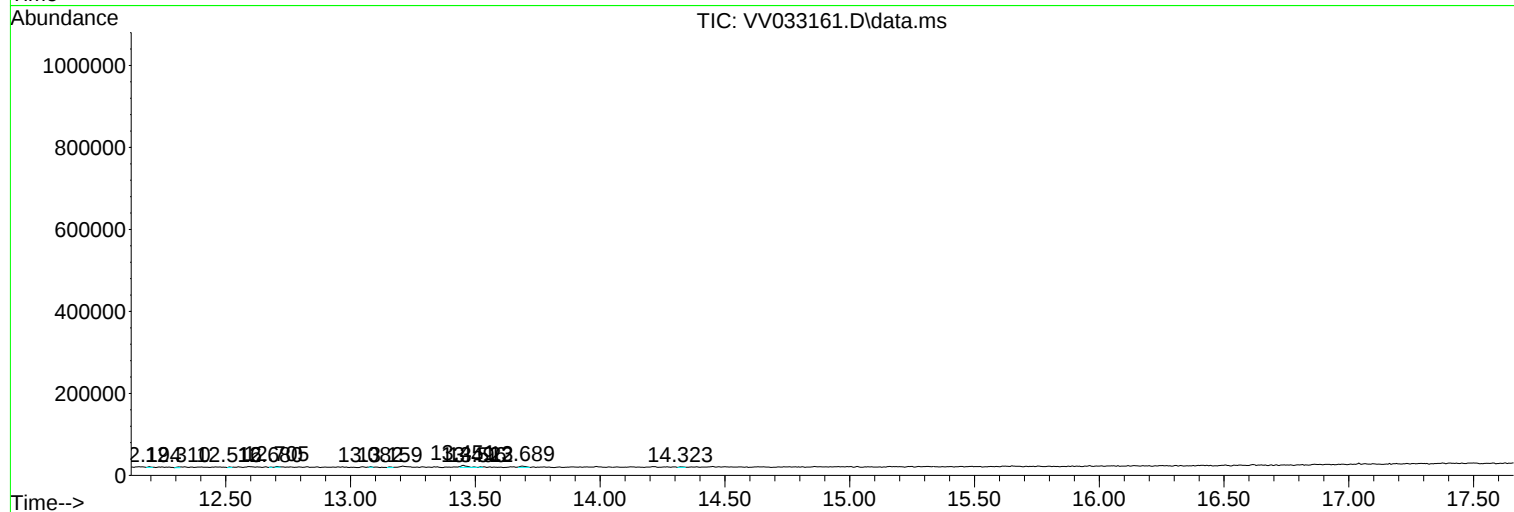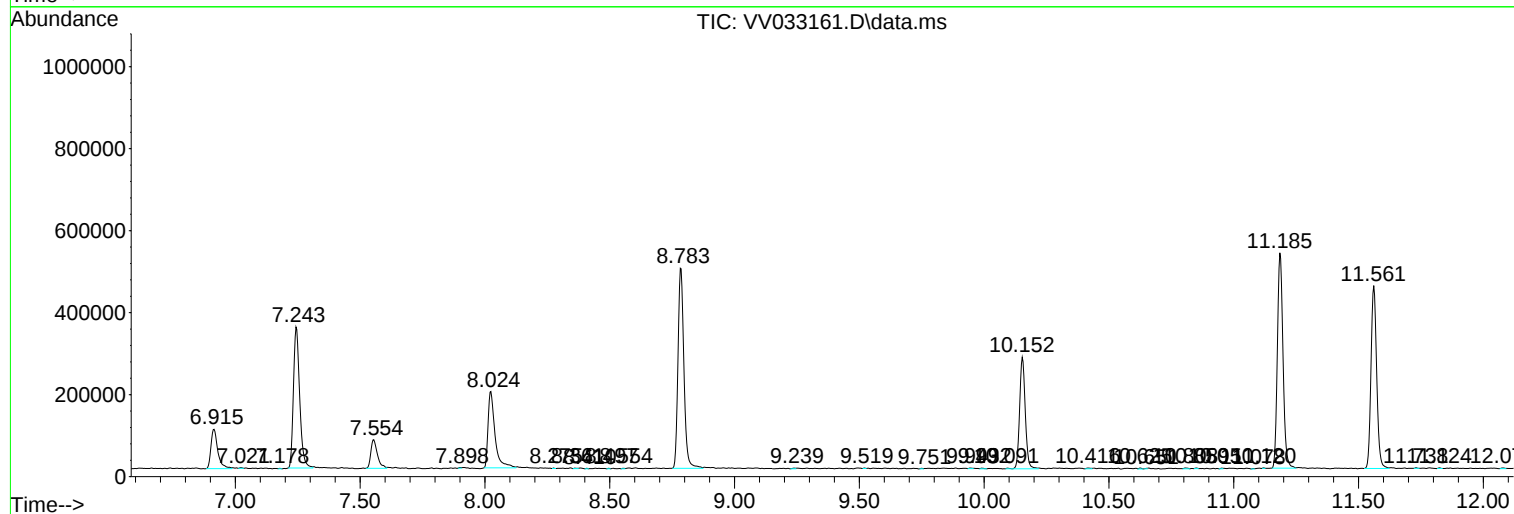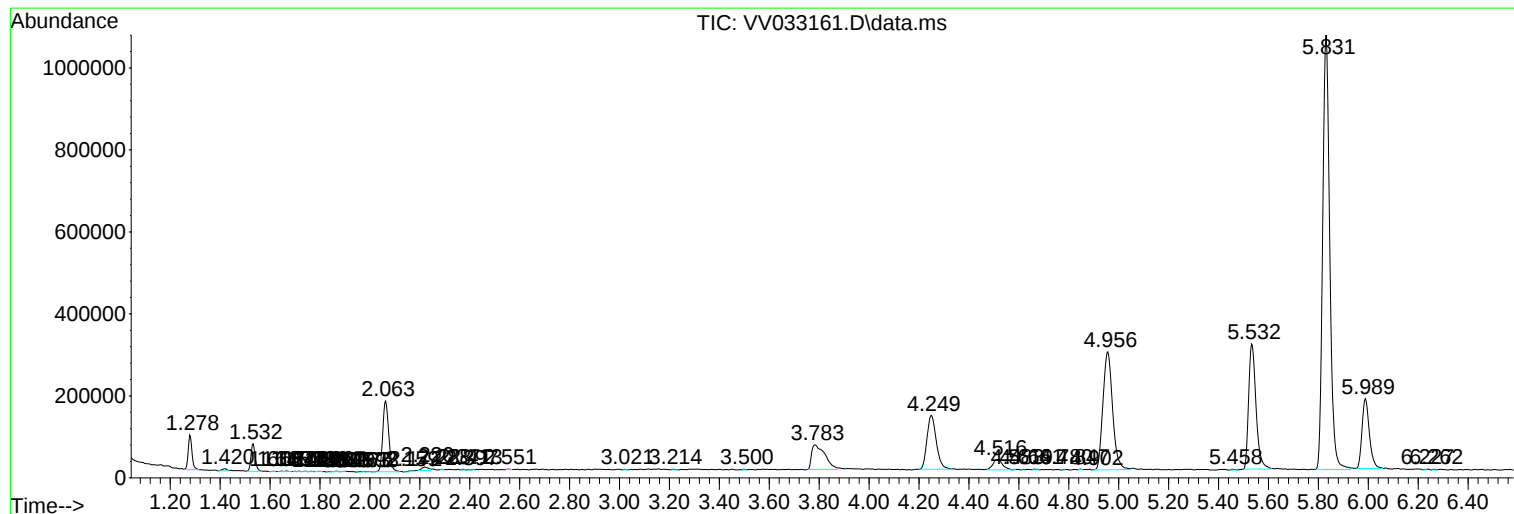

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033161.D
Acq On : 07 Dec 2023 21:13
Operator : SY/MD
Sample : 05689-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G77

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033161.D
Acq On : 07 Dec 2023 21:13
Operator : SY/MD
Sample : 05689-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G77

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------