

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033162.D
 Acq On : 07 Dec 2023 21:37
 Operator : SY/MD
 Sample : 05689-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G79

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VV033162.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	86	rVB	81713	87915	10.92%	1.299%
2	1.420	112	118	129	rVB2	5333	8562	1.06%	0.127%
3	1.481	134	137	141	rBV3	733	658	0.08%	0.010%
4	1.532	145	153	166	rVB	68939	83216	10.34%	1.230%
5	1.584	166	169	175	rVB2	2137	1757	0.22%	0.026%
6	1.609	175	177	179	rBV	491	273	0.03%	0.004%
7	1.629	179	183	187	rBV	1488	1091	0.14%	0.016%
8	1.651	187	190	193	rBV2	1331	809	0.10%	0.012%
9	1.677	193	198	204	rVB	1084	1377	0.17%	0.020%
10	1.706	204	207	210	rVB	1463	912	0.11%	0.013%
11	1.725	210	213	217	rVB2	948	731	0.09%	0.011%
12	1.767	217	226	227	rBV2	1045	1376	0.17%	0.020%
13	1.793	231	234	237	rVB2	1059	630	0.08%	0.009%
14	1.825	240	244	245	rBV	559	341	0.04%	0.005%
15	1.854	250	253	256	rVB2	1304	796	0.10%	0.012%
16	1.873	256	259	261	rBV2	668	447	0.06%	0.007%
17	1.892	261	265	269	rBV3	1099	1167	0.14%	0.017%
18	1.915	269	272	278	rVB3	1601	1815	0.23%	0.027%
19	1.941	278	280	284	rBV	971	648	0.08%	0.010%
20	1.976	288	291	292	rBV	891	492	0.06%	0.007%
21	1.986	292	294	298	rVB3	1834	1207	0.15%	0.018%
22	2.015	298	303	308	rBV	1666	2043	0.25%	0.030%
23	2.060	308	317	336	rBV	142614	211233	26.23%	3.122%
24	2.127	336	338	340	rBV2	371	187	0.02%	0.003%
25	2.143	340	343	344	rBV	730	371	0.05%	0.005%
26	2.179	349	354	355	rBV2	1925	1522	0.19%	0.022%
27	2.220	359	367	378	rBV3	12555	24597	3.05%	0.364%
28	2.349	405	407	409	rBV2	1162	766	0.10%	0.011%
29	2.764	533	536	538	rBV	1213	859	0.11%	0.013%
30	3.076	630	633	635	rBV2	2014	1384	0.17%	0.020%
31	3.288	696	699	702	rBV	1022	723	0.09%	0.011%
32	3.635	803	807	813	rBV	1464	1417	0.18%	0.021%
33	3.780	844	852	876	rBV3	60006	158567	19.69%	2.343%
34	4.249	983	998	1022	rBV	136574	348982	43.34%	5.157%
35	4.635	1115	1118	1121	rBV	1555	880	0.11%	0.013%
36	4.680	1130	1132	1136	rVB2	1714	1052	0.13%	0.016%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033162.D
 Acq On : 07 Dec 2023 21:37
 Operator : SY/MD
 Sample : 05689-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G79

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	4.703	1136	1139	1143	rBV	1540	1408	0.17%	0.021%
38	4.796	1165	1168	1174	rBV	1767	2051	0.25%	0.030%
39	4.957	1203	1218	1246	rBV3	287806	759509	94.33%	11.225%
40	5.149	1276	1278	1281	rBV2	999	617	0.08%	0.009%
41	5.214	1295	1298	1303	rVB	2040	1574	0.20%	0.023%
42	5.368	1343	1346	1353	rBV3	1277	1351	0.17%	0.020%
43	5.465	1373	1376	1379	rBV2	1517	1147	0.14%	0.017%
44	5.532	1386	1397	1426	rBV	302646	622765	77.35%	9.204%
45	5.834	1482	1491	1508	rVB7	13984	30445	3.78%	0.450%
46	5.944	1522	1525	1527	rVB	1514	805	0.10%	0.012%
47	5.989	1527	1539	1559	rBV	167823	346534	43.04%	5.121%
48	6.108	1573	1576	1581	rVB2	1351	1014	0.13%	0.015%
49	6.371	1655	1658	1663	rBV2	1122	1135	0.14%	0.017%
50	6.606	1728	1731	1734	rBV	1265	815	0.10%	0.012%
51	6.629	1734	1738	1742	rVB	1801	1641	0.20%	0.024%
52	6.770	1779	1782	1787	rBV	1416	1601	0.20%	0.024%
53	6.870	1810	1813	1817	rBV	1040	854	0.11%	0.013%
54	6.911	1817	1826	1840	rBV2	95610	176775	21.96%	2.613%
55	7.082	1876	1879	1883	rVB	2511	2069	0.26%	0.031%
56	7.108	1884	1887	1889	rBV	1476	1099	0.14%	0.016%
57	7.185	1905	1911	1913	rBV4	1580	1952	0.24%	0.029%
58	7.243	1918	1929	1952	rBV	341103	606228	75.29%	8.959%
59	7.555	2017	2026	2051	rVB	71083	126940	15.77%	1.876%
60	7.908	2133	2136	2139	rBV2	2166	1712	0.21%	0.025%
61	8.024	2163	2172	2195	rBV	192503	362436	45.01%	5.356%
62	8.320	2261	2264	2267	rBV	1901	1175	0.15%	0.017%
63	8.783	2398	2408	2432	rBV	473143	779471	96.81%	11.520%
64	9.021	2479	2482	2483	rBV2	1153	624	0.08%	0.009%
65	9.056	2490	2493	2494	rBV	1766	1074	0.13%	0.016%
66	9.223	2543	2545	2549	rVB	1598	880	0.11%	0.013%
67	9.365	2586	2589	2591	rBV	1051	778	0.10%	0.011%
68	9.599	2659	2662	2665	rBV2	1097	958	0.12%	0.014%
69	9.661	2678	2681	2684	rBV	1400	1040	0.13%	0.015%
70	9.696	2690	2692	2694	rBV2	941	505	0.06%	0.007%
71	9.937	2763	2767	2769	rBV	1244	1038	0.13%	0.015%
72	10.046	2798	2801	2803	rBV	974	695	0.09%	0.010%
73	10.153	2822	2834	2860	rBV	273512	427392	53.08%	6.316%
74	10.593	2967	2971	2974	rVB	2219	1506	0.19%	0.022%
75	10.616	2975	2978	2980	rBV	2354	1397	0.17%	0.021%
76	10.805	3034	3037	3039	rBV	1369	960	0.12%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033162.D
 Acq On : 07 Dec 2023 21:37
 Operator : SY/MD
 Sample : 05689-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G79

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	11.185	3145	3155	3174	rBV	523525	805164	100.00%	11.899%
78	11.361	3207	3210	3214	rBV	1817	1273	0.16%	0.019%
79	11.561	3260	3272	3291	rBV	456520	711808	88.41%	10.520%
80	11.725	3321	3323	3326	rVB2	1315	695	0.09%	0.010%
81	12.014	3411	3413	3419	rVB2	1225	991	0.12%	0.015%
82	12.278	3493	3495	3498	rVB	1261	664	0.08%	0.010%
83	12.471	3552	3555	3557	rBV	1245	788	0.10%	0.012%
84	12.632	3603	3605	3608	rBV	1023	585	0.07%	0.009%
85	13.352	3827	3829	3832	rVB2	1316	699	0.09%	0.010%
86	13.500	3872	3875	3878	rBV	1281	811	0.10%	0.012%
87	13.831	3975	3978	3981	rVB	1928	1113	0.14%	0.016%
88	13.892	3994	3997	4003	rVB	1746	1231	0.15%	0.018%
89	13.927	4003	4008	4010	rBV3	2030	2056	0.26%	0.030%
90	13.998	4026	4030	4037	rBV	1567	1714	0.21%	0.025%
91	14.265	4111	4113	4115	rBV	1202	765	0.10%	0.011%
92	14.390	4146	4152	4154	rBV2	2025	2263	0.28%	0.033%
93	14.744	4260	4262	4266	rBV	1783	1102	0.14%	0.016%
94	15.120	4377	4379	4382	rVB	1699	888	0.11%	0.013%
95	15.236	4413	4415	4418	rBV	1078	713	0.09%	0.011%
96	15.255	4418	4421	4423	rBV2	1423	1043	0.13%	0.015%
97	15.583	4518	4523	4525	rBV	2057	2260	0.28%	0.033%
98	15.821	4594	4597	4600	rBV5	2228	1849	0.23%	0.027%
99	15.856	4605	4608	4610	rBV3	1851	1248	0.15%	0.018%




Sum of corrected areas: 6766496

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033162.D
Acq On : 07 Dec 2023 21:37
Operator : SY/MD
Sample : 05689-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G79

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

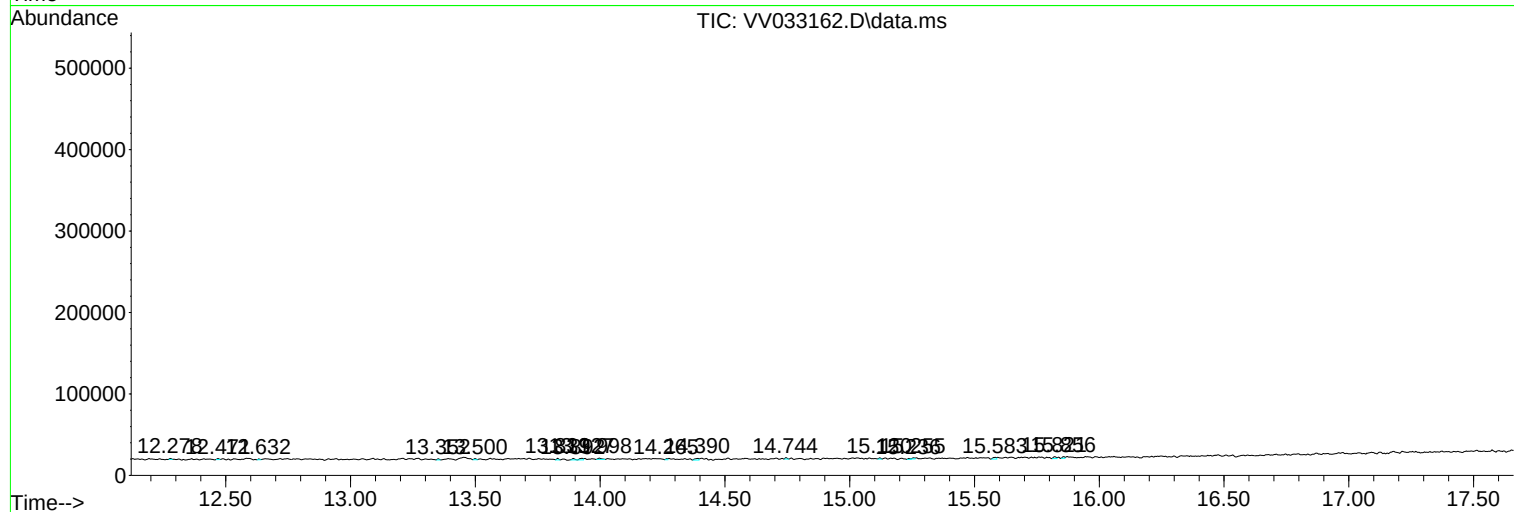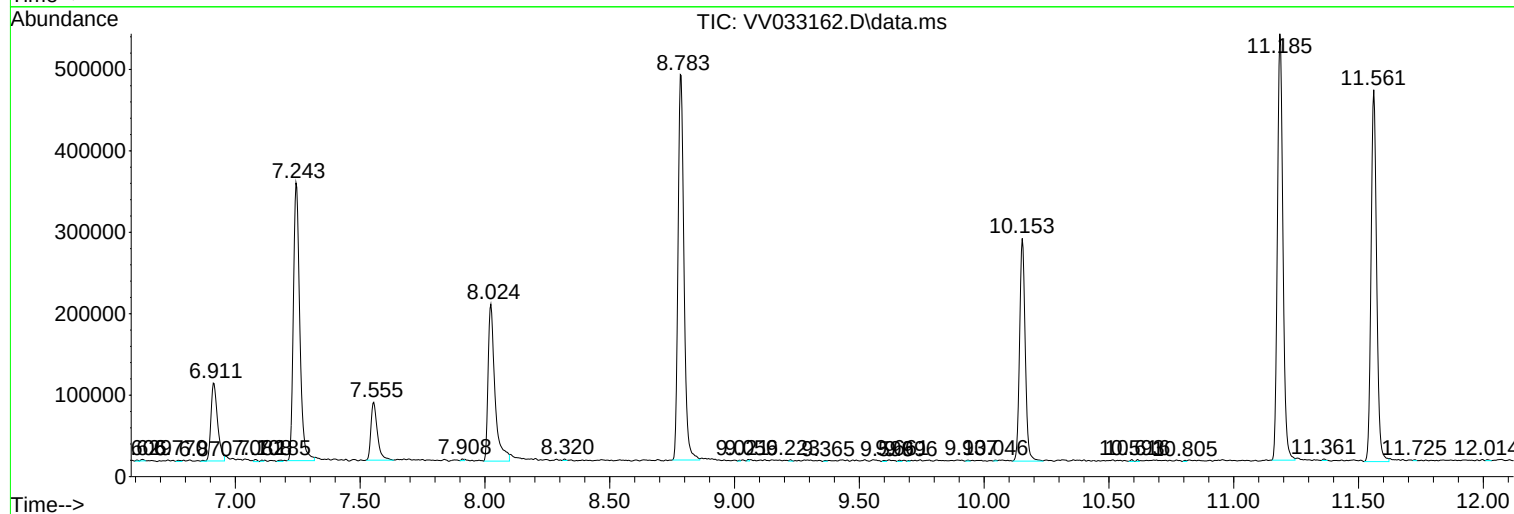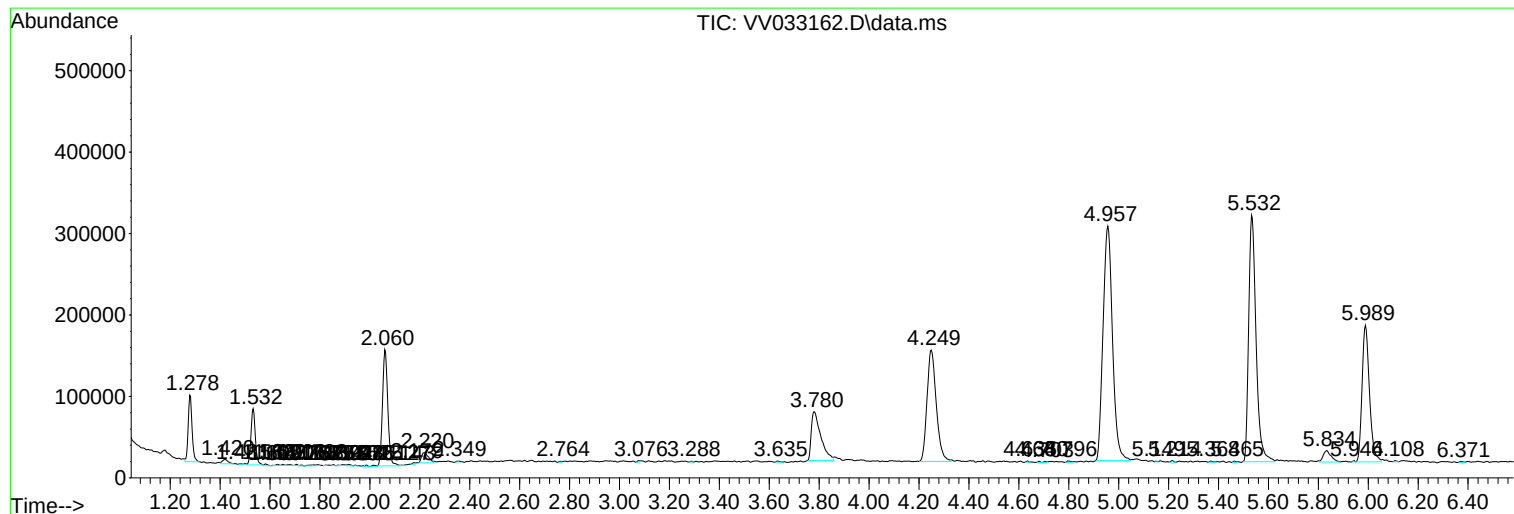

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033162.D
Acq On : 07 Dec 2023 21:37
Operator : SY/MD
Sample : 05689-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G79

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033162.D
Acq On : 07 Dec 2023 21:37
Operator : SY/MD
Sample : 05689-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G79

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------