

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033165.D
 Acq On : 07 Dec 2023 22:46
 Operator : SY/MD
 Sample : 05689-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G83

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M

Title : VOC Analysis

Signal : TIC: VV033165.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	86	rVB	77506	81808	10.42%	1.245%
2	1.417	110	117	122	rBV	5274	6199	0.79%	0.094%
3	1.458	128	130	133	rVB3	1138	667	0.08%	0.010%
4	1.478	133	136	144	rVV	2312	2602	0.33%	0.040%
5	1.532	144	153	170	rVB	64938	80404	10.24%	1.224%
6	1.610	171	177	182	rVB2	1414	1804	0.23%	0.027%
7	1.648	182	189	193	rBV2	1172	1762	0.22%	0.027%
8	1.671	193	196	200	rBV2	738	491	0.06%	0.007%
9	1.706	205	207	208	rBV2	222	73	0.01%	0.001%
10	1.719	208	211	214	rBV2	1328	896	0.11%	0.014%
11	1.735	214	216	222	rVB2	828	655	0.08%	0.010%
12	1.777	226	229	230	rVV3	893	492	0.06%	0.007%
13	1.786	230	232	235	rVV2	910	464	0.06%	0.007%
14	1.828	239	245	248	rBV3	1436	1668	0.21%	0.025%
15	1.854	248	253	256	rBV	1293	1013	0.13%	0.015%
16	1.883	259	262	265	rBV2	773	629	0.08%	0.010%
17	1.909	267	270	273	rVV2	623	357	0.05%	0.005%
18	1.937	277	279	280	rVB2	293	107	0.01%	0.002%
19	1.963	285	287	290	rVB	985	515	0.07%	0.008%
20	1.989	290	295	303	rVB	2024	3187	0.41%	0.049%
21	2.060	303	317	332	rBV	134855	201105	25.62%	3.061%
22	2.140	337	342	344	rBV	2390	1896	0.24%	0.029%
23	2.175	348	353	356	rBV	1240	1270	0.16%	0.019%
24	2.220	360	367	375	rBV	5923	10640	1.36%	0.162%
25	2.394	418	421	424	rBV	1325	1029	0.13%	0.016%
26	2.552	466	470	472	rBV	1984	1734	0.22%	0.026%
27	2.609	485	488	491	rBV	1282	1071	0.14%	0.016%
28	2.648	497	500	502	rBV	1320	947	0.12%	0.014%
29	2.934	586	589	591	rBV	1769	1082	0.14%	0.016%
30	3.265	687	692	697	rBV	2279	2769	0.35%	0.042%
31	3.336	711	714	717	rBV	1458	962	0.12%	0.015%
32	3.671	813	818	822	rBV	1961	2254	0.29%	0.034%
33	3.783	844	853	887	rBV	54139	149731	19.08%	2.279%
34	4.005	919	922	927	rVB	1678	1459	0.19%	0.022%
35	4.249	984	998	1020	rBV	130068	332136	42.32%	5.055%
36	4.658	1122	1125	1132	rVB2	1631	1726	0.22%	0.026%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120723\
 Data File : VW033165.D
 Acq On : 07 Dec 2023 22:46
 Operator : SY/MD
 Sample : 05689-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G83

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	4.693	1133	1136	1138	rBV	1276	960	0.12%	0.015%
38	4.732	1145	1148	1156	rVB	2275	2647	0.34%	0.040%
39	4.957	1202	1218	1248	rBV2	275839	744661	94.87%	11.333%
40	5.339	1335	1337	1341	rBV	1354	895	0.11%	0.014%
41	5.532	1386	1397	1423	rBV	293730	608464	77.52%	9.261%
42	5.831	1482	1490	1509	rVB7	12520	30613	3.90%	0.466%
43	5.989	1527	1539	1556	rBV	161641	332537	42.37%	5.061%
44	6.105	1572	1575	1579	rBV	1668	1335	0.17%	0.020%
45	6.249	1617	1620	1622	rBV	1575	876	0.11%	0.013%
46	6.307	1636	1638	1644	rVB2	1579	1104	0.14%	0.017%
47	6.461	1683	1686	1690	rBV	1413	1144	0.15%	0.017%
48	6.490	1693	1695	1701	rBV	1360	1237	0.16%	0.019%
49	6.712	1762	1764	1766	rBV	1111	624	0.08%	0.009%
50	6.793	1787	1789	1791	rBV2	953	506	0.06%	0.008%
51	6.857	1806	1809	1810	rBV	1339	717	0.09%	0.011%
52	6.915	1817	1827	1849	rBV	89241	168397	21.45%	2.563%
53	7.153	1897	1901	1905	rBV	2053	1742	0.22%	0.027%
54	7.243	1919	1929	1952	rBV	328575	585683	74.62%	8.914%
55	7.555	2017	2026	2045	rBV2	66379	117118	14.92%	1.782%
56	7.876	2123	2126	2133	rBV3	1824	1917	0.24%	0.029%
57	8.024	2163	2172	2207	rBV2	188714	362889	46.23%	5.523%
58	8.481	2311	2314	2316	rBV	1165	776	0.10%	0.012%
59	8.551	2333	2336	2340	rBV	1330	1035	0.13%	0.016%
60	8.574	2341	2343	2346	rBV2	1151	749	0.10%	0.011%
61	8.786	2397	2409	2430	rBV	467277	771835	98.33%	11.747%
62	9.043	2486	2489	2491	rVB	1280	728	0.09%	0.011%
63	9.140	2517	2519	2527	rVB	1837	2037	0.26%	0.031%
64	9.201	2533	2538	2540	rBV	1369	1457	0.19%	0.022%
65	9.349	2581	2584	2587	rBV	1492	1160	0.15%	0.018%
66	9.686	2685	2689	2694	rBV	2102	2389	0.30%	0.036%
67	9.818	2727	2730	2733	rVB	1213	605	0.08%	0.009%
68	10.037	2795	2798	2799	rBV2	1270	792	0.10%	0.012%
69	10.111	2818	2821	2823	rBV	1267	978	0.12%	0.015%
70	10.153	2823	2834	2855	rVV2	267138	422133	53.78%	6.425%
71	10.320	2884	2886	2889	rBV2	1157	691	0.09%	0.011%
72	10.394	2907	2909	2914	rBV	1343	963	0.12%	0.015%
73	10.554	2957	2959	2961	rBV	1254	785	0.10%	0.012%
74	10.976	3087	3090	3095	rBV	1554	1804	0.23%	0.027%
75	11.043	3107	3111	3112	rBV	1168	936	0.12%	0.014%
76	11.185	3145	3155	3174	rBV	510074	784905	100.00%	11.946%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033165.D
 Acq On : 07 Dec 2023 22:46
 Operator : SY/MD
 Sample : 05689-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G83

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	11.349	3204	3206	3208	rBV	1083	518	0.07%	0.008%
78	11.561	3260	3272	3291	rBV	436562	679895	86.62%	10.348%
79	11.799	3343	3346	3349	rVB	1293	875	0.11%	0.013%
80	12.387	3527	3529	3533	rVB	1503	885	0.11%	0.013%
81	12.410	3533	3536	3540	rBV	1645	1385	0.18%	0.021%
82	12.500	3561	3564	3570	rBV	1427	1418	0.18%	0.022%
83	12.574	3585	3587	3590	rVB	1213	565	0.07%	0.009%
84	12.625	3600	3603	3605	rBV	1195	739	0.09%	0.011%
85	12.741	3636	3639	3644	rVB	1875	1824	0.23%	0.028%
86	12.773	3645	3649	3652	rBV	1925	1477	0.19%	0.022%
87	12.956	3703	3706	3708	rBV2	1178	802	0.10%	0.012%
88	13.705	3936	3939	3941	rBV2	1697	1181	0.15%	0.018%
89	13.786	3961	3964	3968	rBV	2192	2080	0.27%	0.032%
90	13.831	3974	3978	3981	rBV	1997	1785	0.23%	0.027%
91	13.895	3994	3998	4001	rVB	1547	1208	0.15%	0.018%
92	14.300	4121	4124	4129	rVB3	1840	1600	0.20%	0.024%
93	14.773	4268	4271	4274	rBV2	1577	1199	0.15%	0.018%
94	15.024	4346	4349	4354	rBV3	1481	1356	0.17%	0.021%
95	15.676	4549	4552	4557	rBV4	1555	1716	0.22%	0.026%
96	16.056	4667	4670	4672	rBV2	1667	1045	0.13%	0.016%
97	16.168	4702	4705	4711	rBV5	1936	2343	0.30%	0.036%
98	16.246	4726	4729	4732	rBV3	2067	1787	0.23%	0.027%
99	16.393	4771	4775	4778	rBV4	2203	2335	0.30%	0.036%


Sum of corrected areas: 6570446

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033165.D
Acq On : 07 Dec 2023 22:46
Operator : SY/MD
Sample : 05689-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G83

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

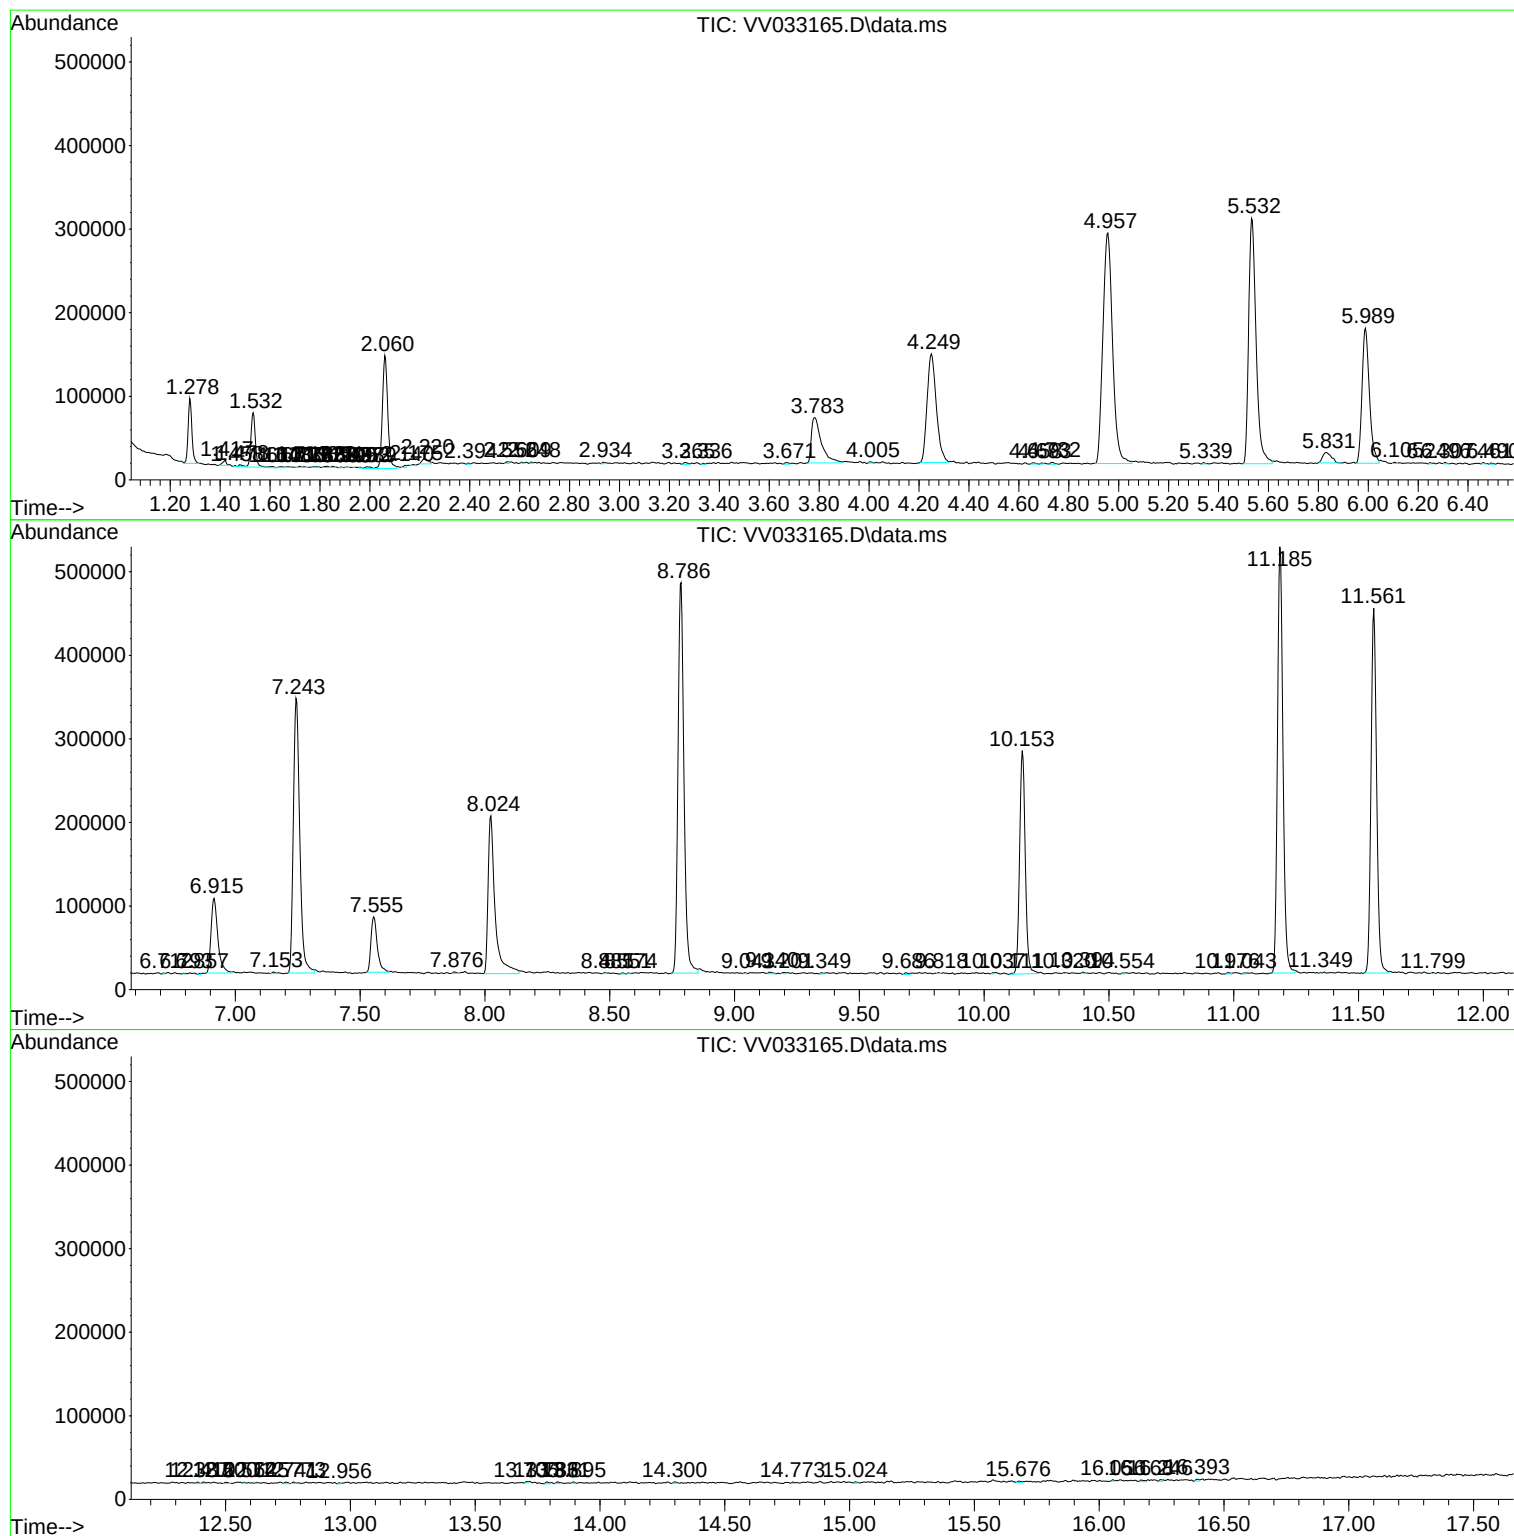

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033165.D
Acq On : 07 Dec 2023 22:46
Operator : SY/MD
Sample : 05689-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G83

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033165.D
Acq On : 07 Dec 2023 22:46
Operator : SY/MD
Sample : 05689-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G83

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------