

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033167.D
 Acq On : 07 Dec 2023 23:33
 Operator : SY/MD
 Sample : 05689-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G86

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VV033167.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	92	rVB	82580	84836	10.47%	1.193%
2	1.420	112	118	123	rVB3	5230	6139	0.76%	0.086%
3	1.458	128	130	135	rVB3	1512	1228	0.15%	0.017%
4	1.491	135	140	145	rBV4	1647	2046	0.25%	0.029%
5	1.532	145	153	167	rVB	66179	80780	9.97%	1.136%
6	1.590	167	171	176	rBV	1294	1365	0.17%	0.019%
7	1.622	179	181	185	rVB2	1094	736	0.09%	0.010%
8	1.645	185	188	190	rBV	884	684	0.08%	0.010%
9	1.754	218	222	226	rVB	1621	1254	0.15%	0.018%
10	1.893	259	265	268	rBV2	1328	1873	0.23%	0.026%
11	1.928	274	276	280	rVB3	1265	735	0.09%	0.010%
12	2.002	296	299	302	rBV	1312	734	0.09%	0.010%
13	2.060	302	317	335	rBV2	140581	217109	26.80%	3.054%
14	2.172	345	352	354	rBV2	2233	2392	0.30%	0.034%
15	2.220	359	367	381	rBV2	6759	15159	1.87%	0.213%
16	2.294	387	390	392	rBV	1924	1301	0.16%	0.018%
17	2.507	452	456	461	rBV	1815	1739	0.21%	0.024%
18	2.632	493	495	499	rVB	1769	1111	0.14%	0.016%
19	3.021	611	616	619	rBV	1752	1824	0.23%	0.026%
20	3.118	643	646	651	rBV	1576	1384	0.17%	0.019%
21	3.269	689	693	697	rBV	2206	2138	0.26%	0.030%
22	3.391	728	731	733	rBV	1431	917	0.11%	0.013%
23	3.642	806	809	812	rBV	1455	1077	0.13%	0.015%
24	3.780	844	852	880	rBV2	55286	173790	21.45%	2.444%
25	4.008	920	923	929	rBV	2257	2873	0.35%	0.040%
26	4.249	984	998	1019	rBV	130659	325502	40.18%	4.578%
27	4.516	1071	1081	1082	rBV5	4658	5953	0.73%	0.084%
28	4.719	1140	1144	1148	rBV2	1309	1398	0.17%	0.020%
29	4.754	1152	1155	1161	rVB	1762	1913	0.24%	0.027%
30	4.957	1201	1218	1244	rBV2	277941	747666	92.30%	10.516%
31	5.249	1305	1309	1313	rBV3	1172	1234	0.15%	0.017%
32	5.474	1376	1379	1381	rBV	1187	749	0.09%	0.011%
33	5.532	1386	1397	1422	rBV	297998	622529	76.85%	8.756%
34	5.712	1451	1453	1456	rBV	945	725	0.09%	0.010%
35	5.834	1477	1491	1515	rBV2	235044	489713	60.46%	6.888%
36	5.989	1527	1539	1561	rVB	162722	331309	40.90%	4.660%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033167.D
 Acq On : 07 Dec 2023 23:33
 Operator : SY/MD
 Sample : 05689-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G86

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	6.143	1584	1587	1589	rBV	1098	675	0.08%	0.009%
38	6.185	1593	1600	1605	rBV2	1940	2317	0.29%	0.033%
39	6.387	1660	1663	1665	rBV	1444	899	0.11%	0.013%
40	6.670	1749	1751	1760	rVB3	1383	1143	0.14%	0.016%
41	6.709	1760	1763	1765	rBV	1564	1191	0.15%	0.017%
42	6.915	1817	1827	1844	rBV	90430	166233	20.52%	2.338%
43	7.243	1919	1929	1954	rBV	326884	579548	71.55%	8.151%
44	7.503	2007	2010	2013	rBV	1702	1278	0.16%	0.018%
45	7.555	2017	2026	2047	rVB	65592	118803	14.67%	1.671%
46	7.744	2082	2085	2089	rBV	1276	1145	0.14%	0.016%
47	8.024	2163	2172	2190	rBV	183497	339663	41.93%	4.777%
48	8.272	2247	2249	2252	rBV	1380	768	0.09%	0.011%
49	8.670	2370	2373	2379	rBV2	1859	1867	0.23%	0.026%
50	8.783	2398	2408	2433	rBV	480019	795416	98.19%	11.187%
51	9.259	2553	2556	2559	rBV	1354	1114	0.14%	0.016%
52	9.439	2609	2612	2615	rBV	1370	814	0.10%	0.011%
53	9.622	2666	2669	2671	rBV3	1294	938	0.12%	0.013%
54	9.760	2709	2712	2717	rBV2	1788	1511	0.19%	0.021%
55	9.847	2736	2739	2742	rBV2	1393	764	0.09%	0.011%
56	9.866	2742	2745	2749	rBV	1181	1129	0.14%	0.016%
57	9.979	2776	2780	2782	rBV	1728	1427	0.18%	0.020%
58	10.072	2806	2809	2812	rBV	1506	1060	0.13%	0.015%
59	10.153	2823	2834	2852	rBV	261804	409584	50.56%	5.761%
60	10.278	2867	2873	2878	rBV	1356	1934	0.24%	0.027%
61	10.307	2879	2882	2885	rBV	1041	671	0.08%	0.009%
62	10.403	2909	2912	2914	rBV	1185	710	0.09%	0.010%
63	10.490	2936	2939	2942	rBV2	1038	872	0.11%	0.012%
64	10.529	2949	2951	2955	rBV2	938	674	0.08%	0.009%
65	10.686	2994	3000	3002	rBV	1412	1559	0.19%	0.022%
66	10.722	3008	3011	3015	rBV	1514	1159	0.14%	0.016%
67	10.828	3038	3044	3047	rBV	1827	1887	0.23%	0.027%
68	10.895	3061	3065	3067	rBV	1519	1283	0.16%	0.018%
69	10.966	3081	3087	3093	rBV	1939	3083	0.38%	0.043%
70	11.001	3096	3098	3101	rBV	1095	726	0.09%	0.010%
71	11.185	3145	3155	3176	rBV	523816	810043	100.00%	11.393%
72	11.561	3260	3272	3302	rBV	432595	686099	84.70%	9.650%
73	11.725	3320	3323	3331	rVB3	1194	1501	0.19%	0.021%
74	11.972	3396	3400	3403	rBV3	1567	1617	0.20%	0.023%
75	12.053	3422	3425	3427	rBV	1668	1181	0.15%	0.017%
76	12.246	3482	3485	3488	rVB	1490	1069	0.13%	0.015%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033167.D
 Acq On : 07 Dec 2023 23:33
 Operator : SY/MD
 Sample : 05689-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G86

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	12.387	3526	3529	3531	rBV2	1231	797	0.10%	0.011%
78	12.905	3687	3690	3694	rBV	1646	1381	0.17%	0.019%
79	13.021	3723	3726	3728	rBV	1165	738	0.09%	0.010%
80	13.082	3742	3745	3751	rVB	1474	1376	0.17%	0.019%
81	13.124	3752	3758	3761	rBV2	1681	1898	0.23%	0.027%
82	13.185	3774	3777	3781	rBV	1189	1235	0.15%	0.017%
83	13.413	3845	3848	3851	rBV	1590	1010	0.12%	0.014%
84	13.654	3920	3923	3924	rBV2	1123	683	0.08%	0.010%
85	13.796	3964	3967	3969	rBV	1479	914	0.11%	0.013%
86	13.873	3987	3991	3994	rBV2	1505	1350	0.17%	0.019%
87	14.017	4033	4036	4037	rBV3	1084	703	0.09%	0.010%
88	14.378	4145	4148	4151	rBV2	1098	960	0.12%	0.014%
89	14.615	4219	4222	4226	rBV2	1468	1223	0.15%	0.017%
90	14.718	4251	4254	4256	rBV2	1279	819	0.10%	0.012%
91	15.001	4340	4342	4347	rBV2	1226	1177	0.15%	0.017%
92	15.027	4347	4350	4353	rBV	1465	1021	0.13%	0.014%
93	15.233	4411	4414	4420	rBV	2187	2493	0.31%	0.035%
94	15.320	4438	4441	4444	rBV	1623	960	0.12%	0.014%
95	15.381	4456	4460	4462	rBV3	1479	1302	0.16%	0.018%
96	15.487	4489	4493	4498	rBV	2097	2423	0.30%	0.034%
97	15.702	4557	4560	4563	rBV2	2007	1339	0.17%	0.019%
98	16.233	4722	4725	4727	rBV2	1832	1284	0.16%	0.018%
99	16.294	4741	4744	4746	rBV2	1943	1257	0.16%	0.018%
100	16.422	4781	4784	4791	rBV2	1864	2476	0.31%	0.035%




Sum of corrected areas: 7110089

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033167.D
Acq On : 07 Dec 2023 23:33
Operator : SY/MD
Sample : 05689-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G86

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

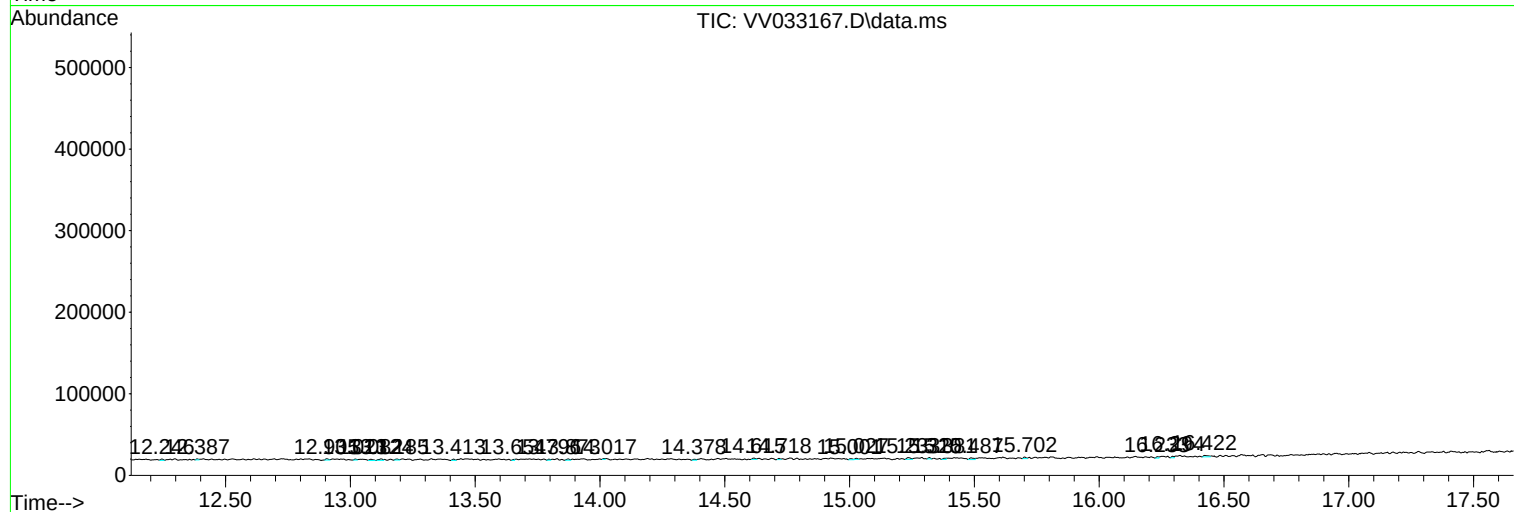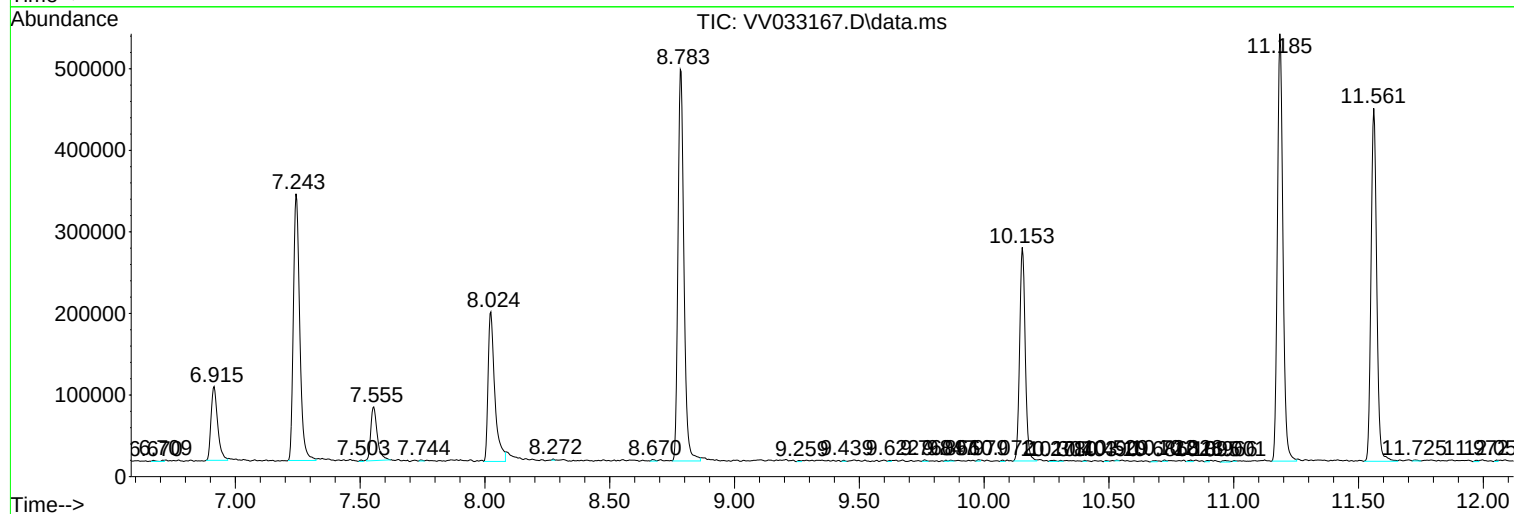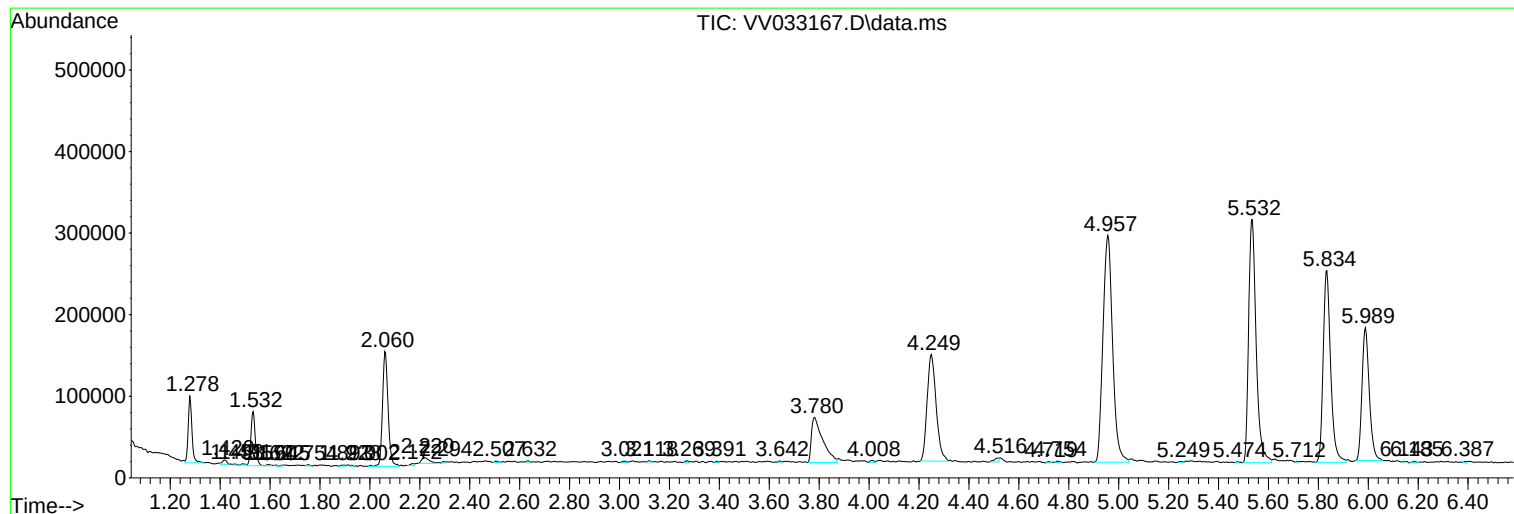

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033167.D
Acq On : 07 Dec 2023 23:33
Operator : SY/MD
Sample : 05689-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G86

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033167.D
Acq On : 07 Dec 2023 23:33
Operator : SY/MD
Sample : 05689-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G86

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc