

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033168.D
 Acq On : 07 Dec 2023 23:56
 Operator : SY/MD
 Sample : 05689-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G88

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VV033168.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	87	rVB	76818	81891	10.14%	1.242%
2	1.375	100	104	106	rBV	1069	811	0.10%	0.012%
3	1.420	106	118	123	rVV3	5078	7386	0.91%	0.112%
4	1.532	145	153	164	rVB	67773	76663	9.50%	1.163%
5	1.638	182	186	190	rVB	1360	1087	0.13%	0.016%
6	1.677	190	198	202	rVB2	1466	1660	0.21%	0.025%
7	1.767	222	226	230	rVB3	1813	1439	0.18%	0.022%
8	1.799	230	236	243	rBV	2102	2625	0.33%	0.040%
9	1.831	243	246	248	rBV3	1081	774	0.10%	0.012%
10	1.841	248	249	256	rVB2	1199	846	0.10%	0.013%
11	1.902	265	268	275	rBV2	1162	982	0.12%	0.015%
12	1.973	287	290	295	rVV3	1003	1041	0.13%	0.016%
13	2.060	304	317	331	rBV	130409	193146	23.93%	2.929%
14	2.166	340	350	351	rBV	2812	3446	0.43%	0.052%
15	2.188	352	357	359	rVV2	2800	2948	0.37%	0.045%
16	2.214	361	365	378	rVB2	4929	10889	1.35%	0.165%
17	2.291	386	389	392	rBV	1936	1390	0.17%	0.021%
18	2.761	533	535	538	rBV2	1216	837	0.10%	0.013%
19	2.886	569	574	578	rVB	1658	1773	0.22%	0.027%
20	3.040	619	622	625	rBV3	1346	1136	0.14%	0.017%
21	3.060	625	628	634	rVV2	1704	2109	0.26%	0.032%
22	3.198	668	671	675	rBV2	2007	1669	0.21%	0.025%
23	3.404	733	735	739	rVB	1414	834	0.10%	0.013%
24	3.513	765	769	774	rBV3	2032	2566	0.32%	0.039%
25	3.780	844	852	880	rBV2	52951	142588	17.66%	2.162%
26	4.008	920	923	927	rVB	2217	1724	0.21%	0.026%
27	4.034	927	931	933	rBV3	1457	1344	0.17%	0.020%
28	4.249	983	998	1026	rBV	127489	328263	40.67%	4.978%
29	4.580	1098	1101	1104	rBV2	1251	1143	0.14%	0.017%
30	4.625	1112	1115	1118	rBV2	1488	1275	0.16%	0.019%
31	4.770	1157	1160	1163	rBV2	1139	1014	0.13%	0.015%
32	4.818	1173	1175	1182	rVB	1493	1371	0.17%	0.021%
33	4.854	1182	1186	1190	rBV	1504	1472	0.18%	0.022%
34	4.957	1202	1218	1241	rBV2	276307	736331	91.22%	11.167%
35	5.095	1258	1261	1263	rBV4	1743	1320	0.16%	0.020%
36	5.243	1305	1307	1312	rBV	1088	929	0.12%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120723\
 Data File : VW033168.D
 Acq On : 07 Dec 2023 23:56
 Operator : SY/MD
 Sample : 05689-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G88

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	5.423	1360	1363	1366	rBV2	1184	891	0.11%	0.014%
38	5.474	1375	1379	1385	rVB	2281	2052	0.25%	0.031%
39	5.532	1385	1397	1422	rBV	299757	626790	77.65%	9.505%
40	5.831	1480	1490	1502	rBV5	11033	21499	2.66%	0.326%
41	5.989	1526	1539	1565	rBV	164445	345203	42.76%	5.235%
42	6.281	1628	1630	1635	rBV2	871	1007	0.12%	0.015%
43	6.426	1673	1675	1677	rBV	1340	818	0.10%	0.012%
44	6.725	1765	1768	1770	rBV2	1320	973	0.12%	0.015%
45	6.915	1817	1827	1842	rBV	88611	164037	20.32%	2.488%
46	7.243	1918	1929	1947	rBV	328029	579595	71.80%	8.790%
47	7.458	1993	1996	1999	rBV2	2307	1788	0.22%	0.027%
48	7.503	2008	2010	2013	rBV	1251	773	0.10%	0.012%
49	7.555	2017	2026	2044	rBV	69202	120021	14.87%	1.820%
50	7.719	2073	2077	2079	rBV2	1327	1007	0.12%	0.015%
51	7.976	2154	2157	2160	rBV	1649	1188	0.15%	0.018%
52	8.024	2163	2172	2202	rBV	187079	351602	43.56%	5.332%
53	8.275	2248	2250	2253	rBV2	1613	862	0.11%	0.013%
54	8.294	2253	2256	2262	rVV	1599	1635	0.20%	0.025%
55	8.474	2310	2312	2316	rBV	1596	1121	0.14%	0.017%
56	8.558	2335	2338	2341	rBV	1502	1267	0.16%	0.019%
57	8.786	2398	2409	2432	rBV	479659	799076	98.99%	12.118%
58	9.027	2482	2484	2489	rVB	1427	1004	0.12%	0.015%
59	9.072	2493	2498	2501	rBV	1964	1977	0.24%	0.030%
60	9.542	2641	2644	2649	rBV	1294	1356	0.17%	0.021%
61	9.744	2704	2707	2711	rBV2	1377	965	0.12%	0.015%
62	9.857	2739	2742	2744	rBV	1089	757	0.09%	0.011%
63	9.972	2775	2778	2781	rBV	1029	740	0.09%	0.011%
64	10.153	2824	2834	2851	rBV	262790	405802	50.27%	6.154%
65	10.435	2918	2922	2923	rBV	1728	1270	0.16%	0.019%
66	10.480	2933	2936	2943	rVB	2686	2706	0.34%	0.041%
67	10.519	2944	2948	2950	rBV2	1402	1135	0.14%	0.017%
68	10.538	2951	2954	2957	rBV3	1257	1168	0.14%	0.018%
69	10.596	2969	2972	2974	rBV	1849	1355	0.17%	0.021%
70	10.725	3009	3012	3013	rBV	1272	753	0.09%	0.011%
71	10.863	3050	3055	3058	rBV	2097	1940	0.24%	0.029%
72	10.915	3067	3071	3074	rBV	1639	1375	0.17%	0.021%
73	11.088	3122	3125	3129	rVB	1521	1127	0.14%	0.017%
74	11.143	3138	3142	3144	rBV3	1095	1012	0.13%	0.015%
75	11.185	3144	3155	3181	rVV	517979	807234	100.00%	12.242%
76	11.297	3188	3190	3198	rBV2	1200	1294	0.16%	0.020%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033168.D
 Acq On : 07 Dec 2023 23:56
 Operator : SY/MD
 Sample : 05689-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G88

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	11.365	3208	3211	3216	rBV	2180	2069	0.26%	0.031%
78	11.561	3260	3272	3290	rBV	436881	683833	84.71%	10.370%
79	11.683	3306	3310	3312	rBV3	1395	1104	0.14%	0.017%
80	11.770	3334	3337	3341	rVB	1461	863	0.11%	0.013%
81	12.278	3492	3495	3500	rBV	1898	1700	0.21%	0.026%
82	12.712	3627	3630	3637	rVB	2106	2057	0.25%	0.031%
83	12.824	3662	3665	3667	rBV2	1234	891	0.11%	0.014%
84	12.902	3685	3689	3691	rBV	2081	1712	0.21%	0.026%
85	13.024	3724	3727	3731	rVB	2046	1435	0.18%	0.022%
86	13.050	3731	3735	3738	rBV	1716	1566	0.19%	0.024%
87	13.451	3855	3860	3863	rBV2	1967	2173	0.27%	0.033%
88	13.593	3901	3904	3906	rBV2	1249	915	0.11%	0.014%
89	13.644	3917	3920	3923	rBV	2119	1718	0.21%	0.026%
90	13.699	3934	3937	3940	rBV	1252	1053	0.13%	0.016%
91	13.821	3970	3975	3980	rBV2	1781	2542	0.31%	0.039%
92	13.950	4012	4015	4020	rBV	1619	1330	0.16%	0.020%
93	14.004	4028	4032	4035	rVB2	1717	1386	0.17%	0.021%
94	14.168	4080	4083	4087	rVB	2184	1475	0.18%	0.022%
95	14.252	4107	4109	4115	rVB2	1355	894	0.11%	0.014%
96	14.516	4186	4191	4193	rBV2	1319	1376	0.17%	0.021%
97	14.644	4229	4231	4234	rVB	1643	788	0.10%	0.012%
98	15.049	4353	4357	4360	rBV2	1751	1349	0.17%	0.020%
99	15.853	4605	4607	4610	rBV4	1627	1097	0.14%	0.017%
100	16.011	4651	4656	4659	rBV4	1769	1828	0.23%	0.028%




Sum of corrected areas: 6594051

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033168.D
Acq On : 07 Dec 2023 23:56
Operator : SY/MD
Sample : 05689-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G88

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

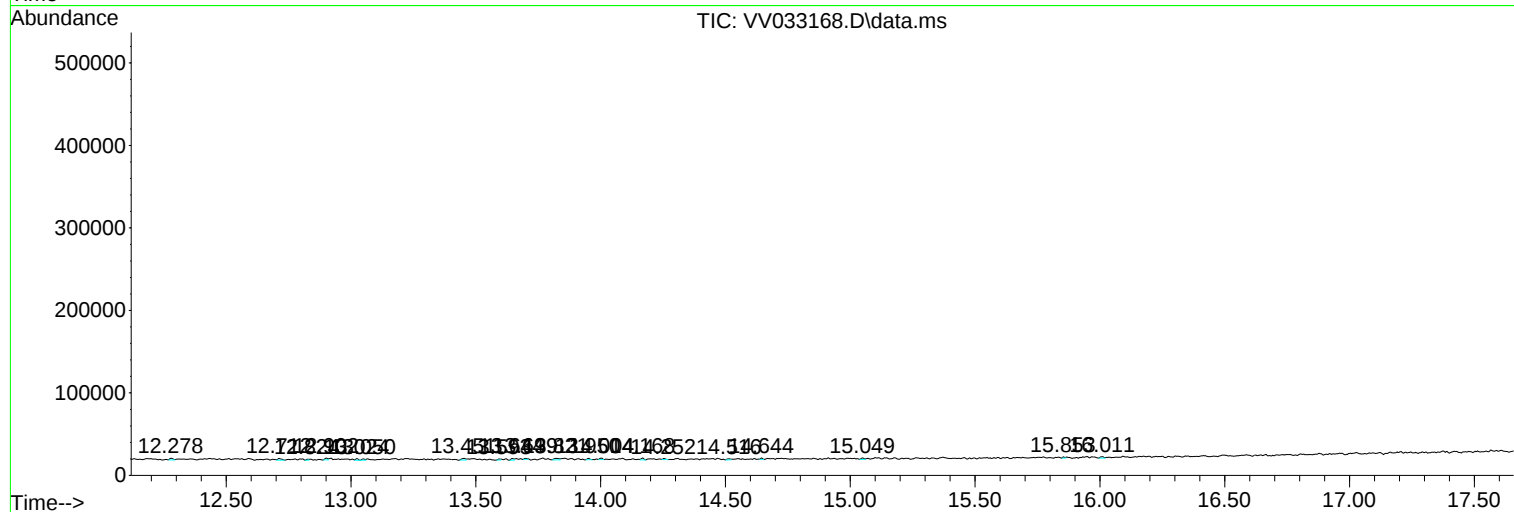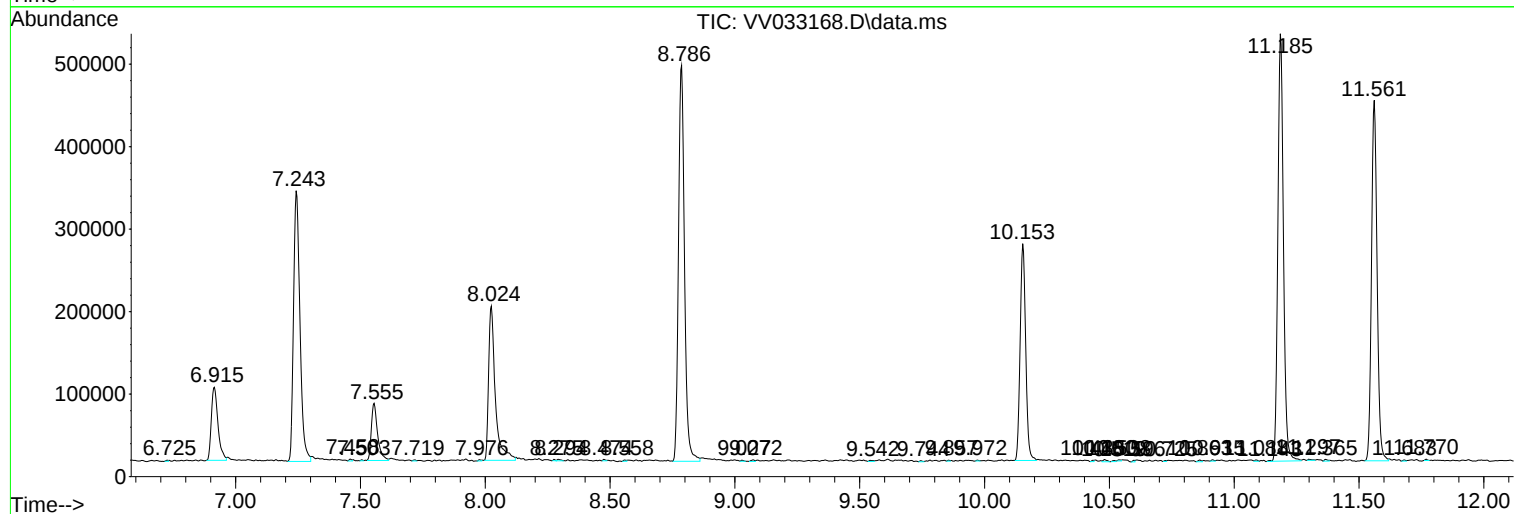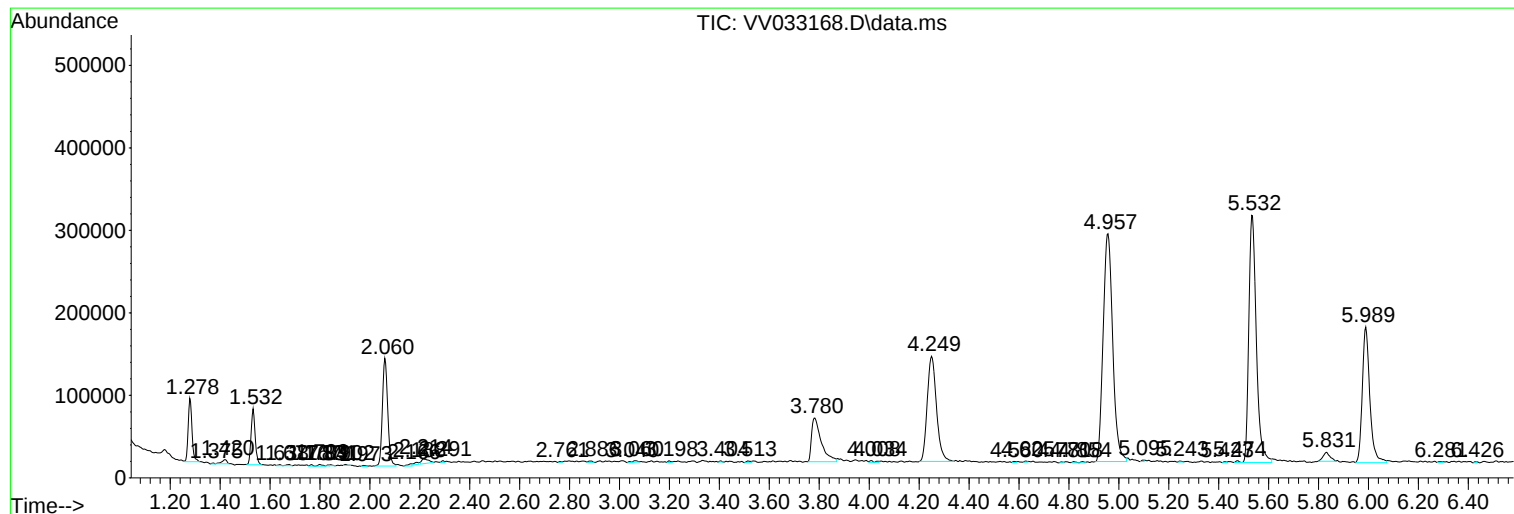

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033168.D
Acq On : 07 Dec 2023 23:56
Operator : SY/MD
Sample : 05689-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G88

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033168.D
Acq On : 07 Dec 2023 23:56
Operator : SY/MD
Sample : 05689-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G88

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------