

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033169.D
 Acq On : 08 Dec 2023 00:19
 Operator : SY/MD
 Sample : 05689-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G89

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VV033169.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	87	rVB	77902	83122	10.60%	1.239%
2	1.362	96	100	103	rBV	1352	1082	0.14%	0.016%
3	1.417	109	117	124	rBV2	4897	7926	1.01%	0.118%
4	1.484	133	138	143	rBV2	1476	1729	0.22%	0.026%
5	1.532	144	153	164	rVV	62206	74883	9.55%	1.116%
6	1.667	192	195	198	rVB2	1317	835	0.11%	0.012%
7	1.690	198	202	206	rVB2	1036	803	0.10%	0.012%
8	1.761	220	224	232	rVB3	1376	2105	0.27%	0.031%
9	1.847	247	251	255	rVB	2324	1995	0.25%	0.030%
10	2.060	304	317	332	rBV	133449	200779	25.61%	2.994%
11	2.163	342	349	351	rBV4	2219	2434	0.31%	0.036%
12	2.179	351	354	357	rBV2	878	776	0.10%	0.012%
13	2.217	358	366	381	rBV2	10493	23298	2.97%	0.347%
14	2.671	502	507	510	rBV	1956	2239	0.29%	0.033%
15	2.706	515	518	521	rBV2	1684	1339	0.17%	0.020%
16	2.783	540	542	545	rBV	1118	752	0.10%	0.011%
17	2.838	556	559	562	rBV2	1144	836	0.11%	0.012%
18	2.889	572	575	578	rBV	1654	1373	0.18%	0.020%
19	3.060	626	628	632	rBV2	1268	862	0.11%	0.013%
20	3.233	678	682	684	rBV	1363	1025	0.13%	0.015%
21	3.294	698	701	704	rVB	2519	1500	0.19%	0.022%
22	3.593	790	794	796	rBV	1159	1071	0.14%	0.016%
23	3.703	825	828	831	rBV	2116	1768	0.23%	0.026%
24	3.780	844	852	876	rBV	58915	154756	19.74%	2.307%
25	4.166	966	972	976	rBV	2523	3100	0.40%	0.046%
26	4.249	983	998	1023	rBV2	131386	334988	42.73%	4.995%
27	4.388	1036	1041	1045	rBV2	1448	1776	0.23%	0.026%
28	4.436	1053	1056	1059	rVB2	1390	863	0.11%	0.013%
29	4.812	1167	1173	1177	rBV2	2131	2926	0.37%	0.044%
30	4.957	1202	1218	1244	rBV2	275830	740927	94.50%	11.047%
31	5.207	1290	1296	1300	rBV3	1749	2301	0.29%	0.034%
32	5.252	1307	1310	1311	rBV	1248	759	0.10%	0.011%
33	5.317	1327	1330	1332	rBV	1140	789	0.10%	0.012%
34	5.359	1341	1343	1347	rVB	1528	954	0.12%	0.014%
35	5.532	1386	1397	1422	rBV	295882	609441	77.73%	9.087%
36	5.680	1441	1443	1446	rBV	1419	777	0.10%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120723\
 Data File : VW033169.D
 Acq On : 08 Dec 2023 00:19
 Operator : SY/MD
 Sample : 05689-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G89

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	5.834	1476	1491	1512	rBV5	64756	147515	18.81%	2.199%
38	5.931	1519	1521	1525	rVB2	1425	818	0.10%	0.012%
39	5.989	1526	1539	1558	rBV2	164747	333373	42.52%	4.970%
40	6.272	1622	1627	1632	rVB	1525	1947	0.25%	0.029%
41	6.394	1661	1665	1671	rVB2	1414	1758	0.22%	0.026%
42	6.436	1675	1678	1681	rBV	1567	958	0.12%	0.014%
43	6.461	1683	1686	1688	rBV2	1249	787	0.10%	0.012%
44	6.535	1707	1709	1715	rVB2	1662	1175	0.15%	0.018%
45	6.568	1716	1719	1722	rVB	2043	1195	0.15%	0.018%
46	6.915	1817	1827	1847	rBV	89408	169290	21.59%	2.524%
47	7.002	1852	1854	1857	rBV2	1212	858	0.11%	0.013%
48	7.243	1918	1929	1950	rBV	325526	582040	74.24%	8.678%
49	7.555	2017	2026	2042	rBV2	66711	118102	15.06%	1.761%
50	7.873	2122	2125	2131	rBV	1645	1501	0.19%	0.022%
51	7.912	2134	2137	2143	rBB	2082	1993	0.25%	0.030%
52	8.024	2163	2172	2210	rBV	189170	367213	46.84%	5.475%
53	8.214	2227	2231	2235	rBV	2247	2264	0.29%	0.034%
54	8.330	2263	2267	2268	rBV2	2001	1296	0.17%	0.019%
55	8.622	2355	2358	2361	rBV	1372	798	0.10%	0.012%
56	8.667	2369	2372	2374	rBV	1680	1123	0.14%	0.017%
57	8.783	2397	2408	2428	rBV	464568	777142	99.12%	11.587%
58	8.944	2456	2458	2467	rVB2	1410	1391	0.18%	0.021%
59	9.008	2475	2478	2481	rBV	1618	1049	0.13%	0.016%
60	9.114	2509	2511	2514	rVB	1510	769	0.10%	0.011%
61	9.143	2517	2520	2523	rBV	1759	1281	0.16%	0.019%
62	10.066	2803	2807	2810	rBV	1537	1412	0.18%	0.021%
63	10.153	2823	2834	2853	rBV	263071	410670	52.38%	6.123%
64	10.587	2966	2969	2971	rBV2	1463	1006	0.13%	0.015%
65	10.796	3031	3034	3035	rBV	1352	760	0.10%	0.011%
66	10.895	3061	3065	3070	rBV	1464	1445	0.18%	0.022%
67	10.982	3088	3092	3099	rVV2	1298	1598	0.20%	0.024%
68	11.034	3104	3108	3110	rBV	2175	1763	0.22%	0.026%
69	11.185	3145	3155	3176	rBV	504778	784037	100.00%	11.690%
70	11.416	3224	3227	3233	rBV2	1080	811	0.10%	0.012%
71	11.445	3233	3236	3242	rBV	1417	1287	0.16%	0.019%
72	11.561	3260	3272	3291	rBV	426214	676822	86.33%	10.091%
73	11.960	3394	3396	3399	rVB	1388	769	0.10%	0.011%
74	12.281	3493	3496	3501	rBV2	1346	1182	0.15%	0.018%
75	12.336	3506	3513	3519	rBV	2686	3950	0.50%	0.059%
76	12.365	3519	3522	3527	rVB	1568	1585	0.20%	0.024%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033169.D
 Acq On : 08 Dec 2023 00:19
 Operator : SY/MD
 Sample : 05689-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G89

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	12.397	3527	3532	3534	rBV2	1359	1339	0.17%	0.020%
78	12.500	3560	3564	3567	rBV	2001	1745	0.22%	0.026%
79	12.599	3591	3595	3599	rVB	1994	1615	0.21%	0.024%
80	12.763	3641	3646	3650	rBV2	1228	1606	0.20%	0.024%
81	13.178	3771	3775	3778	rBV2	1543	1392	0.18%	0.021%
82	13.252	3795	3798	3804	rBV2	1345	1242	0.16%	0.019%
83	13.580	3898	3900	3903	rVB	2313	1243	0.16%	0.019%
84	13.603	3903	3907	3909	rBV2	1112	949	0.12%	0.014%
85	13.808	3969	3971	3974	rVB	1582	906	0.12%	0.014%
86	13.898	3996	3999	4003	rBV2	1307	964	0.12%	0.014%
87	14.236	4100	4104	4110	rBV2	1429	1447	0.18%	0.022%
88	14.432	4161	4165	4168	rBV	2028	1686	0.22%	0.025%
89	14.509	4186	4189	4193	rVB	1868	1174	0.15%	0.018%
90	14.532	4193	4196	4201	rVB2	1461	1231	0.16%	0.018%
91	14.558	4201	4204	4207	rBV	1647	1115	0.14%	0.017%
92	14.654	4232	4234	4238	rBV2	1086	841	0.11%	0.013%
93	14.824	4285	4287	4293	rBV3	1065	856	0.11%	0.013%
94	14.895	4307	4309	4312	rBV2	1407	869	0.11%	0.013%
95	15.024	4346	4349	4352	rBV3	1444	1391	0.18%	0.021%
96	15.078	4364	4366	4370	rVB	1596	973	0.12%	0.015%
97	15.127	4378	4381	4387	rBV	1223	1164	0.15%	0.017%
98	15.207	4400	4406	4411	rBV3	2362	3085	0.39%	0.046%
99	15.361	4452	4454	4458	rVB	1292	730	0.09%	0.011%
100	15.439	4475	4478	4485	rBV2	1803	1918	0.24%	0.029%




Sum of corrected areas: 6707103

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033169.D
Acq On : 08 Dec 2023 00:19
Operator : SY/MD
Sample : 05689-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G89

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

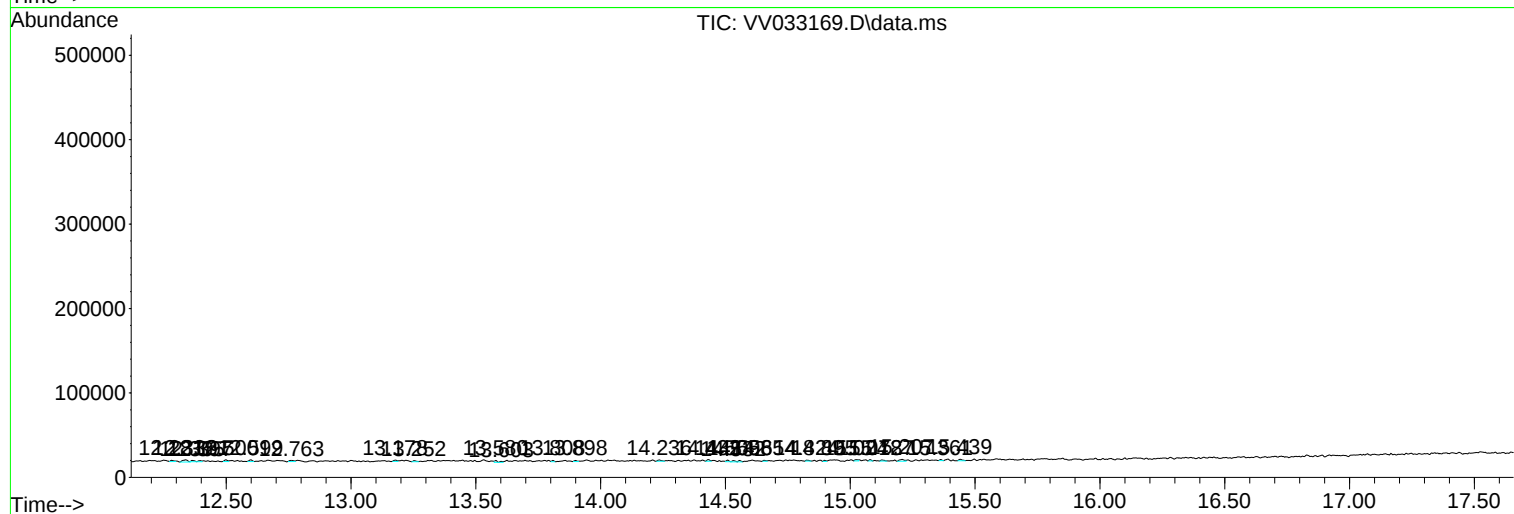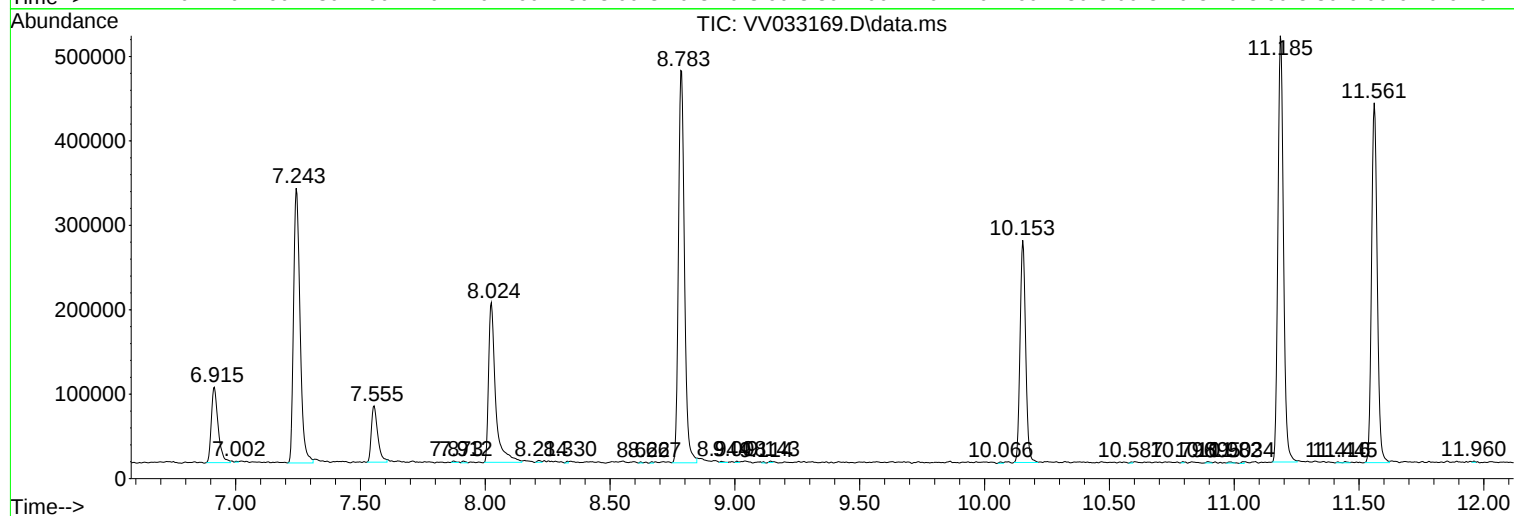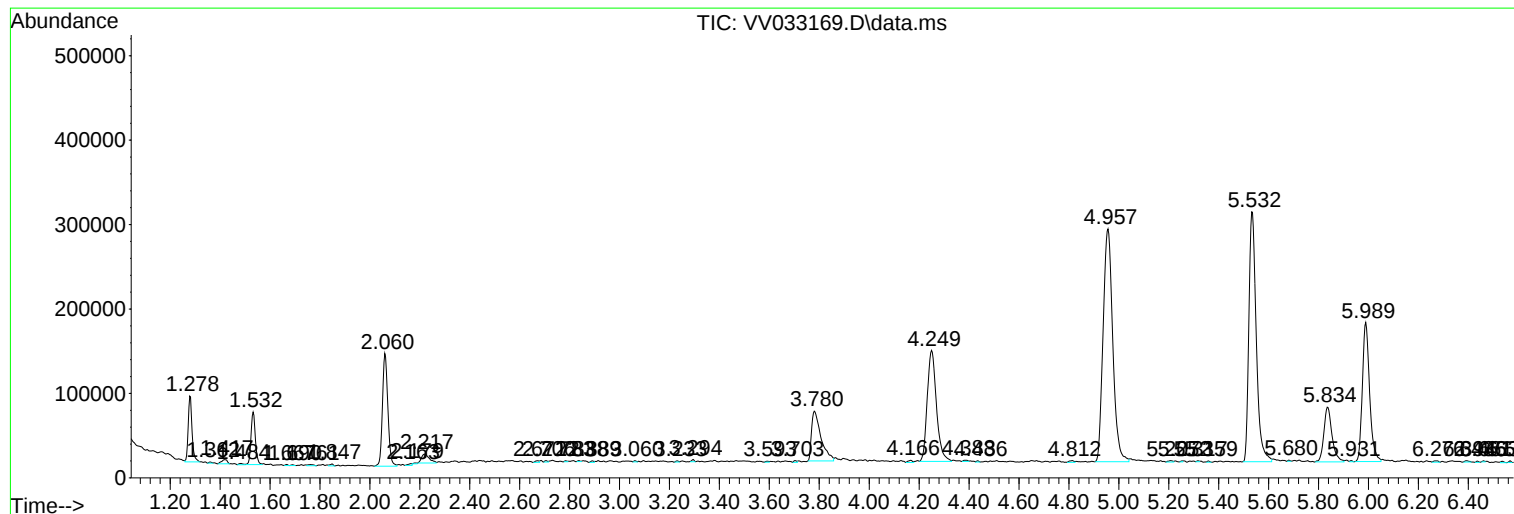

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033169.D
Acq On : 08 Dec 2023 00:19
Operator : SY/MD
Sample : 05689-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G89

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033169.D
Acq On : 08 Dec 2023 00:19
Operator : SY/MD
Sample : 05689-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G89

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------