

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033170.D
 Acq On : 08 Dec 2023 00:42
 Operator : SY/MD
 Sample : 05689-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G92

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M

Title : VOC Analysis

Signal : TIC: VV033170.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	87	rVB	78052	84377	10.58%	1.287%
2	1.420	112	118	124	rVB3	6235	7292	0.91%	0.111%
3	1.449	124	127	133	rVB2	1469	1214	0.15%	0.019%
4	1.532	145	153	169	rVB	65096	79521	9.97%	1.213%
5	1.613	174	178	180	rVB	1114	678	0.08%	0.010%
6	1.629	180	183	186	rBV3	913	688	0.09%	0.010%
7	1.648	186	189	192	rVB	1462	1013	0.13%	0.015%
8	1.671	192	196	197	rBV3	830	614	0.08%	0.009%
9	1.696	201	204	207	rBV2	835	520	0.07%	0.008%
10	1.722	207	212	213	rBV	1264	892	0.11%	0.014%
11	1.732	213	215	219	rVV3	1288	1036	0.13%	0.016%
12	1.777	223	229	233	rBV2	1367	1495	0.19%	0.023%
13	1.803	233	237	239	rVV2	804	577	0.07%	0.009%
14	1.825	239	244	248	rVV	1684	1533	0.19%	0.023%
15	1.848	248	251	255	rVV	807	615	0.08%	0.009%
16	1.880	258	261	266	rVB2	1424	1120	0.14%	0.017%
17	1.912	266	271	273	rBV2	729	907	0.11%	0.014%
18	1.925	273	275	278	rVB	1132	635	0.08%	0.010%
19	1.944	278	281	285	rBV	1009	701	0.09%	0.011%
20	1.979	289	292	296	rVB2	973	599	0.08%	0.009%
21	2.060	307	317	333	rVV	130328	193546	24.26%	2.953%
22	2.118	333	335	340	rVB4	2034	1112	0.14%	0.017%
23	2.159	340	348	349	rBV2	2326	2782	0.35%	0.042%
24	2.175	349	353	356	rBV2	1493	1542	0.19%	0.024%
25	2.217	357	366	377	rBV3	10440	20562	2.58%	0.314%
26	2.291	387	389	392	rBV	975	543	0.07%	0.008%
27	2.368	411	413	417	rBV	1662	1071	0.13%	0.016%
28	2.928	585	587	590	rBV	1203	707	0.09%	0.011%
29	3.439	744	746	751	rVB2	1771	1416	0.18%	0.022%
30	3.610	796	799	800	rBV	1209	747	0.09%	0.011%
31	3.780	844	852	878	rBV	58990	158742	19.90%	2.422%
32	4.134	959	962	966	rBV	1889	1672	0.21%	0.026%
33	4.191	978	980	983	rBV2	1171	763	0.10%	0.012%
34	4.249	983	998	1015	rBV	129759	328941	41.23%	5.018%
35	4.876	1190	1193	1196	rBV2	1179	860	0.11%	0.013%
36	4.957	1202	1218	1242	rBV3	275213	728012	91.24%	11.106%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120723\
 Data File : VW033170.D
 Acq On : 08 Dec 2023 00:42
 Operator : SY/MD
 Sample : 05689-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G92

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	5.085	1256	1258	1261	rBV	1737	876	0.11%	0.013%
38	5.468	1375	1377	1384	rVB	1779	1556	0.20%	0.024%
39	5.532	1386	1397	1420	rBV	302854	615634	77.16%	9.392%
40	5.831	1483	1490	1504	rVB6	10988	21229	2.66%	0.324%
41	5.989	1527	1539	1563	rBV	161207	334047	41.87%	5.096%
42	6.188	1595	1601	1604	rBV3	1917	2319	0.29%	0.035%
43	6.269	1623	1626	1628	rBV	1803	1310	0.16%	0.020%
44	6.349	1648	1651	1654	rVB2	1252	816	0.10%	0.012%
45	6.484	1690	1693	1695	rBV	1710	1092	0.14%	0.017%
46	6.912	1815	1826	1847	rBV	91047	174280	21.84%	2.659%
47	7.243	1918	1929	1957	rBV	326157	585709	73.41%	8.935%
48	7.442	1988	1991	1996	rBV	1437	1452	0.18%	0.022%
49	7.551	2017	2025	2042	rBV	67233	118694	14.88%	1.811%
50	7.706	2070	2073	2077	rVB	2020	1386	0.17%	0.021%
51	7.728	2078	2080	2084	rVB	1143	736	0.09%	0.011%
52	7.831	2109	2112	2114	rBV2	1356	906	0.11%	0.014%
53	7.934	2141	2144	2149	rBV	1433	1053	0.13%	0.016%
54	8.024	2163	2172	2200	rBV	186684	358519	44.93%	5.469%
55	8.786	2398	2409	2432	rBV	473493	782746	98.10%	11.941%
56	8.989	2469	2472	2476	rBV	1173	1002	0.13%	0.015%
57	9.098	2503	2506	2508	rBV	1552	979	0.12%	0.015%
58	9.378	2591	2593	2595	rBV2	987	576	0.07%	0.009%
59	9.407	2599	2602	2605	rBV	1695	1202	0.15%	0.018%
60	9.458	2615	2618	2619	rBV	931	581	0.07%	0.009%
61	9.879	2746	2749	2752	rBV	1381	797	0.10%	0.012%
62	9.931	2762	2765	2768	rBV2	1127	911	0.11%	0.014%
63	9.969	2773	2777	2781	rBV	1813	1920	0.24%	0.029%
64	10.153	2823	2834	2849	rBV	260821	404664	50.72%	6.173%
65	10.259	2865	2867	2870	rBV	996	529	0.07%	0.008%
66	10.326	2885	2888	2891	rVB2	2170	1393	0.17%	0.021%
67	10.584	2965	2968	2970	rBV	1170	697	0.09%	0.011%
68	10.838	3045	3047	3051	rBV	1156	810	0.10%	0.012%
69	11.063	3115	3117	3120	rBV2	1015	541	0.07%	0.008%
70	11.140	3138	3141	3143	rBV2	1153	751	0.09%	0.011%
71	11.185	3144	3155	3175	rVV	518896	797869	100.00%	12.172%
72	11.391	3216	3219	3223	rBV2	1363	1053	0.13%	0.016%
73	11.471	3241	3244	3250	rVB	1983	1876	0.24%	0.029%
74	11.503	3251	3254	3258	rBV	1139	1185	0.15%	0.018%
75	11.561	3261	3272	3293	rVV	428983	673778	84.45%	10.279%
76	12.034	3417	3419	3422	rBV	1039	685	0.09%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033170.D
 Acq On : 08 Dec 2023 00:42
 Operator : SY/MD
 Sample : 05689-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G92

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	12.137	3448	3451	3454	rVB	1712	1091	0.14%	0.017%
78	12.153	3454	3456	3462	rBV	1303	1223	0.15%	0.019%
79	12.326	3508	3510	3515	rVB	1918	1155	0.14%	0.018%
80	12.538	3573	3576	3580	rBV	1826	1482	0.19%	0.023%
81	12.915	3691	3693	3695	rBV	1041	565	0.07%	0.009%
82	13.226	3781	3790	3792	rBV	1679	2660	0.33%	0.041%
83	13.535	3884	3886	3892	rVB3	1027	860	0.11%	0.013%
84	13.564	3892	3895	3897	rBV	1234	708	0.09%	0.011%
85	13.625	3912	3914	3917	rBV	1176	987	0.12%	0.015%
86	13.735	3946	3948	3952	rBV2	1014	822	0.10%	0.013%
87	13.789	3959	3965	3967	rBV	1473	1817	0.23%	0.028%
88	13.905	3999	4001	4004	rBV	1003	634	0.08%	0.010%
89	14.082	4053	4056	4061	rBV	1277	1046	0.13%	0.016%
90	14.243	4103	4106	4111	rBV	1348	1227	0.15%	0.019%
91	14.374	4145	4147	4150	rVB	1278	707	0.09%	0.011%
92	14.390	4150	4152	4154	rBV	1027	592	0.07%	0.009%
93	14.407	4155	4157	4161	rVB	1688	1196	0.15%	0.018%
94	14.931	4317	4320	4321	rBV2	1801	1177	0.15%	0.018%
95	15.355	4450	4452	4455	rBV2	1401	870	0.11%	0.013%
96	15.480	4488	4491	4494	rVB2	1881	1284	0.16%	0.020%
97	15.702	4558	4560	4566	rVB3	1493	1108	0.14%	0.017%
98	15.844	4601	4604	4610	rVB	1719	1865	0.23%	0.028%
99	15.886	4614	4617	4622	rBV	1605	1687	0.21%	0.026%
100	16.162	4701	4703	4706	rBV2	1625	1174	0.15%	0.018%




Sum of corrected areas: 6555141

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033170.D
Acq On : 08 Dec 2023 00:42
Operator : SY/MD
Sample : 05689-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G92

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

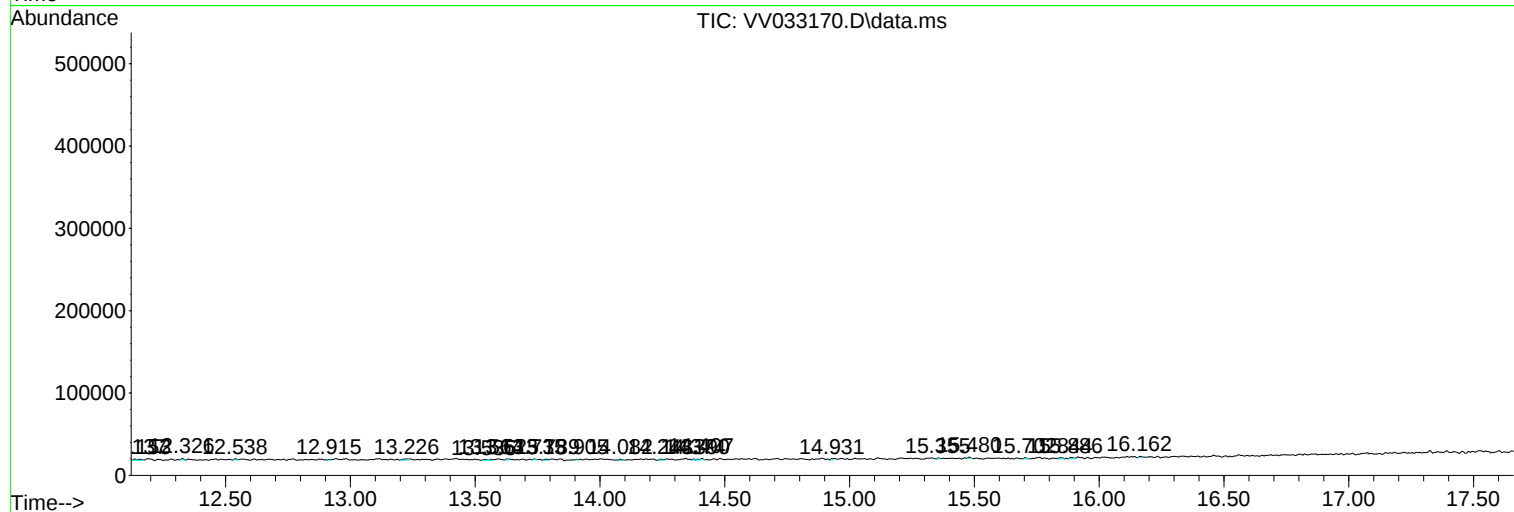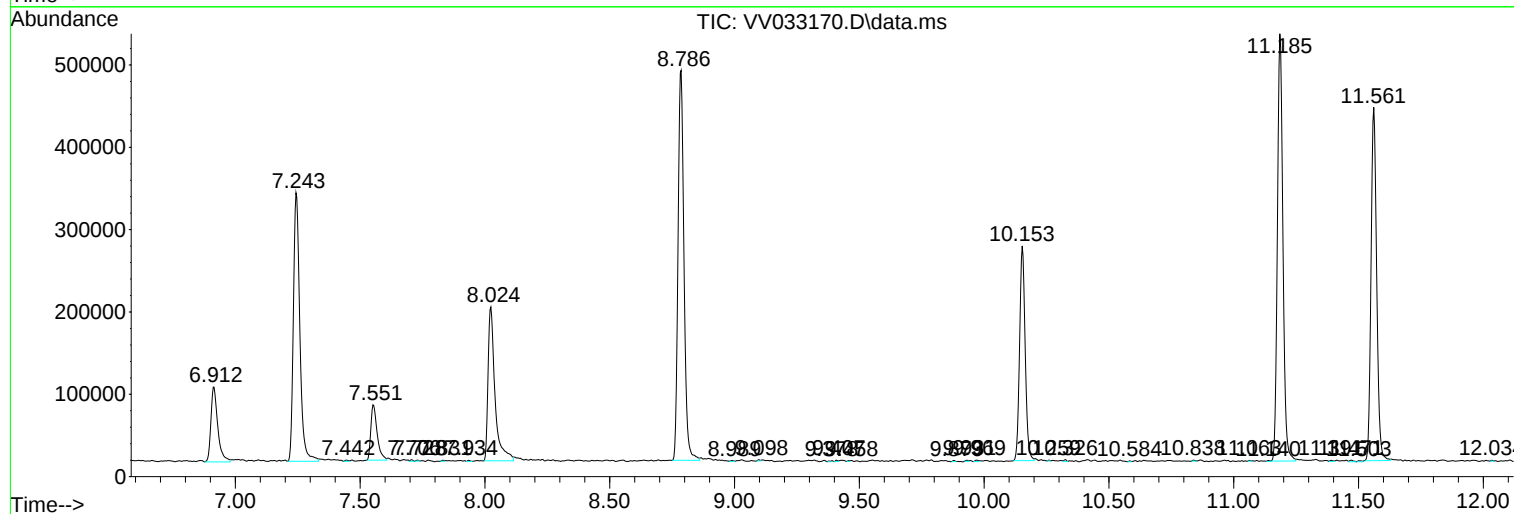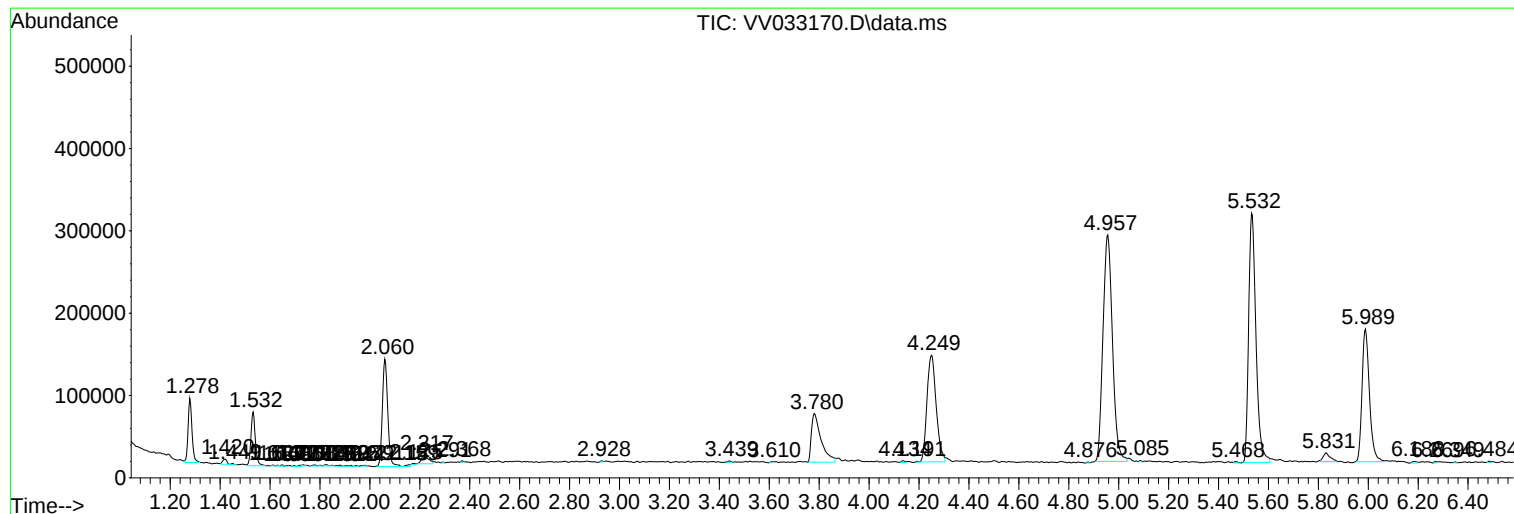

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033170.D
Acq On : 08 Dec 2023 00:42
Operator : SY/MD
Sample : 05689-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G92

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033170.D
Acq On : 08 Dec 2023 00:42
Operator : SY/MD
Sample : 05689-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G92

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc