

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033171.D
 Acq On : 08 Dec 2023 01:06
 Operator : SY/MD
 Sample : 05689-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G93

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M

Title : VOC Analysis

Signal : TIC: VV033171.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	84	rVB	74815	76884	9.64%	1.184%
2	1.417	111	117	125	rVB5	4808	7375	0.92%	0.114%
3	1.532	143	153	169	rVB	62762	77061	9.66%	1.187%
4	1.590	169	171	178	rVB2	1256	1229	0.15%	0.019%
5	1.629	178	183	188	rVB	1739	1864	0.23%	0.029%
6	1.683	193	200	203	rBV2	1599	1756	0.22%	0.027%
7	1.699	203	205	210	rBV	1062	986	0.12%	0.015%
8	1.764	221	225	228	rBV2	1175	1211	0.15%	0.019%
9	1.786	228	232	235	rVV2	1385	1286	0.16%	0.020%
10	1.825	239	244	248	rVV2	1109	1176	0.15%	0.018%
11	1.867	253	257	260	rBV2	895	679	0.09%	0.010%
12	1.889	260	264	269	rVB2	1349	1406	0.18%	0.022%
13	1.928	272	276	280	rVB4	1188	1061	0.13%	0.016%
14	1.979	287	292	295	rVB3	749	797	0.10%	0.012%
15	2.015	301	303	305	rBV	1155	701	0.09%	0.011%
16	2.060	305	317	331	rBV	127868	190014	23.83%	2.926%
17	2.137	336	341	343	rBV	1418	1094	0.14%	0.017%
18	2.162	343	349	352	rBV2	2395	2664	0.33%	0.041%
19	2.185	352	356	358	rBV	1338	1139	0.14%	0.018%
20	2.224	359	368	374	rBV2	9169	15710	1.97%	0.242%
21	2.355	406	409	412	rBV	1097	926	0.12%	0.014%
22	2.712	518	520	524	rVB	1492	926	0.12%	0.014%
23	2.806	544	549	552	rBV	1906	1933	0.24%	0.030%
24	3.021	613	616	618	rBV	1200	929	0.12%	0.014%
25	3.114	642	645	648	rBV	1250	758	0.10%	0.012%
26	3.394	729	732	734	rBV	1350	879	0.11%	0.014%
27	3.510	765	768	771	rBV	1789	1472	0.18%	0.023%
28	3.687	819	823	826	rBV	1690	1684	0.21%	0.026%
29	3.783	844	853	873	rBV2	51841	133007	16.68%	2.048%
30	4.249	984	998	1028	rBV	128051	333452	41.81%	5.135%
31	4.510	1076	1079	1081	rBV	1327	885	0.11%	0.014%
32	4.629	1113	1116	1119	rBV3	1138	871	0.11%	0.013%
33	4.773	1159	1161	1164	rBV	1346	898	0.11%	0.014%
34	4.789	1164	1166	1171	rVV	1312	1075	0.13%	0.017%
35	4.854	1182	1186	1188	rBV	1083	867	0.11%	0.013%
36	4.957	1202	1218	1243	rBV3	271745	732958	91.91%	11.288%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120723\
 Data File : VW033171.D
 Acq On : 08 Dec 2023 01:06
 Operator : SY/MD
 Sample : 05689-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G93

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	5.066	1250	1252	1257	rVB2	1823	1234	0.15%	0.019%
38	5.150	1275	1278	1283	rBV	2124	1923	0.24%	0.030%
39	5.313	1326	1329	1333	rBV	1630	1194	0.15%	0.018%
40	5.365	1342	1345	1347	rBV	1757	1163	0.15%	0.018%
41	5.481	1378	1381	1383	rBV	1060	841	0.11%	0.013%
42	5.535	1387	1398	1420	rBV	293057	608909	76.35%	9.377%
43	5.834	1480	1491	1509	rVB8	14615	35596	4.46%	0.548%
44	5.989	1527	1539	1558	rBV	157291	325912	40.87%	5.019%
45	6.143	1584	1587	1591	rVB2	2102	1531	0.19%	0.024%
46	6.387	1660	1663	1666	rBV	1058	939	0.12%	0.014%
47	6.860	1807	1810	1813	rVB	2133	1346	0.17%	0.021%
48	6.915	1813	1827	1845	rBV2	89148	174631	21.90%	2.689%
49	7.243	1918	1929	1950	rBV	321763	572987	71.85%	8.824%
50	7.452	1992	1994	1997	rBV	1198	796	0.10%	0.012%
51	7.555	2017	2026	2046	rBV	67088	119191	14.95%	1.836%
52	7.886	2127	2129	2133	rVB2	2544	1320	0.17%	0.020%
53	8.024	2163	2172	2197	rBV	176524	333791	41.85%	5.140%
54	8.223	2231	2234	2237	rBV2	2170	1630	0.20%	0.025%
55	8.419	2292	2295	2298	rBV2	1421	1252	0.16%	0.019%
56	8.439	2298	2301	2304	rVV2	1201	911	0.11%	0.014%
57	8.628	2357	2360	2363	rBV2	1480	1103	0.14%	0.017%
58	8.654	2365	2368	2370	rBV	1336	921	0.12%	0.014%
59	8.690	2376	2379	2384	rVB	1559	1314	0.16%	0.020%
60	8.786	2396	2409	2431	rBV	474650	785440	98.49%	12.096%
61	9.063	2491	2495	2498	rBV	2099	2090	0.26%	0.032%
62	9.194	2533	2536	2538	rBV	1262	905	0.11%	0.014%
63	9.259	2553	2556	2558	rBV	1504	1071	0.13%	0.016%
64	9.580	2652	2656	2661	rBV	1641	1766	0.22%	0.027%
65	9.876	2744	2748	2751	rBV	2036	1537	0.19%	0.024%
66	10.008	2786	2789	2791	rBV	1541	1049	0.13%	0.016%
67	10.153	2823	2834	2851	rBV	251184	397469	49.84%	6.121%
68	10.394	2907	2909	2912	rBV	1173	790	0.10%	0.012%
69	10.780	3024	3029	3036	rVB	1729	1847	0.23%	0.028%
70	10.812	3036	3039	3042	rBV	1542	1017	0.13%	0.016%
71	10.844	3046	3049	3052	rBV	1316	953	0.12%	0.015%
72	10.892	3060	3064	3071	rBV	1384	1753	0.22%	0.027%
73	11.185	3145	3155	3175	rBV	514087	797498	100.00%	12.281%
74	11.316	3193	3196	3198	rBV	1577	1171	0.15%	0.018%
75	11.561	3261	3272	3293	rBV	428478	671089	84.15%	10.335%
76	11.783	3335	3341	3346	rBV2	1853	2449	0.31%	0.038%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033171.D
 Acq On : 08 Dec 2023 01:06
 Operator : SY/MD
 Sample : 05689-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G93

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	12.181	3462	3465	3467	rBV	989	725	0.09%	0.011%
78	12.304	3499	3503	3505	rBV	1493	1399	0.18%	0.022%
79	12.541	3575	3577	3580	rBV	1319	707	0.09%	0.011%
80	12.638	3605	3607	3611	rVB	1977	1245	0.16%	0.019%
81	12.728	3631	3635	3637	rBV3	1517	1307	0.16%	0.020%
82	12.767	3645	3647	3651	rBV3	929	811	0.10%	0.012%
83	12.927	3695	3697	3699	rBV	1205	679	0.09%	0.010%
84	13.037	3728	3731	3733	rBV	1350	989	0.12%	0.015%
85	13.066	3737	3740	3743	rBV	2361	1883	0.24%	0.029%
86	13.136	3760	3762	3767	rVB	1751	1447	0.18%	0.022%
87	13.175	3767	3774	3777	rBV2	1519	1823	0.23%	0.028%
88	13.339	3822	3825	3827	rBV2	1318	973	0.12%	0.015%
89	13.529	3879	3884	3888	rBV2	2210	2205	0.28%	0.034%
90	13.982	4022	4025	4029	rBV	1765	1721	0.22%	0.027%
91	14.033	4038	4041	4044	rBV2	1139	853	0.11%	0.013%
92	14.088	4055	4058	4062	rBV	1202	986	0.12%	0.015%
93	14.316	4124	4129	4132	rBV2	2039	2225	0.28%	0.034%
94	14.467	4173	4176	4179	rBV	1308	877	0.11%	0.014%
95	14.570	4201	4208	4212	rBV	2607	4149	0.52%	0.064%
96	14.950	4322	4326	4330	rVB2	1361	1145	0.14%	0.018%
97	15.040	4352	4354	4356	rBV3	1224	767	0.10%	0.012%
98	15.133	4380	4383	4384	rBV	1312	796	0.10%	0.012%
99	15.580	4518	4522	4528	rVB	2289	2833	0.36%	0.044%
100	15.918	4624	4627	4629	rBV	1474	1020	0.13%	0.016%




Sum of corrected areas: 6493507

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033171.D
Acq On : 08 Dec 2023 01:06
Operator : SY/MD
Sample : 05689-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G93

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

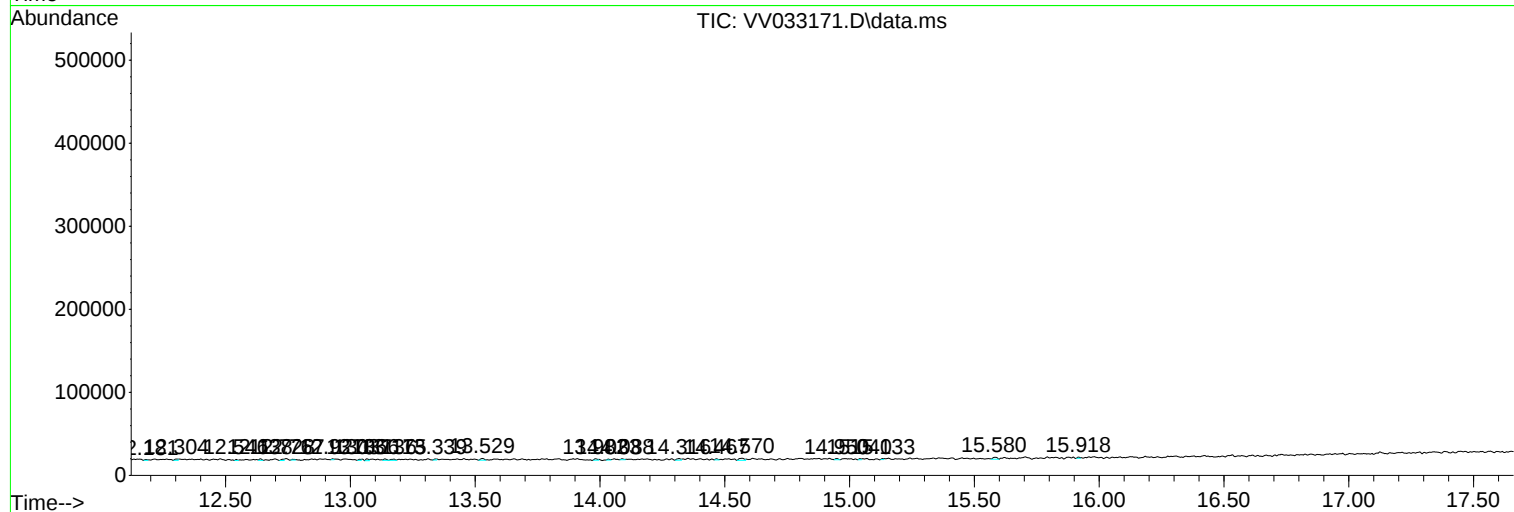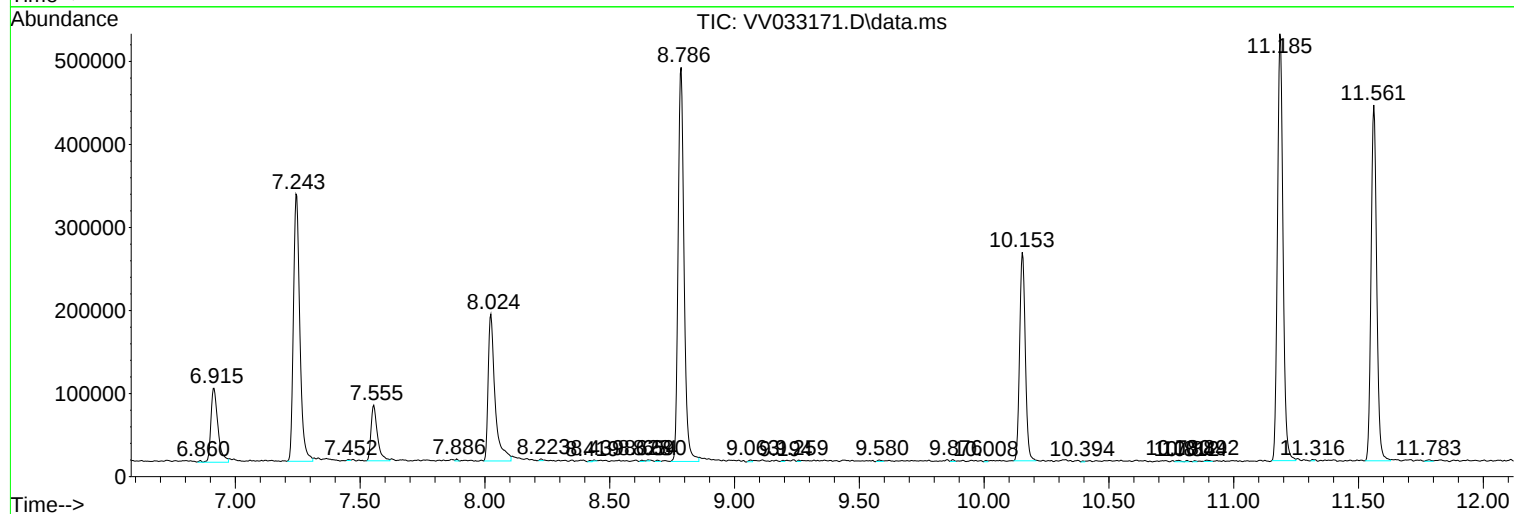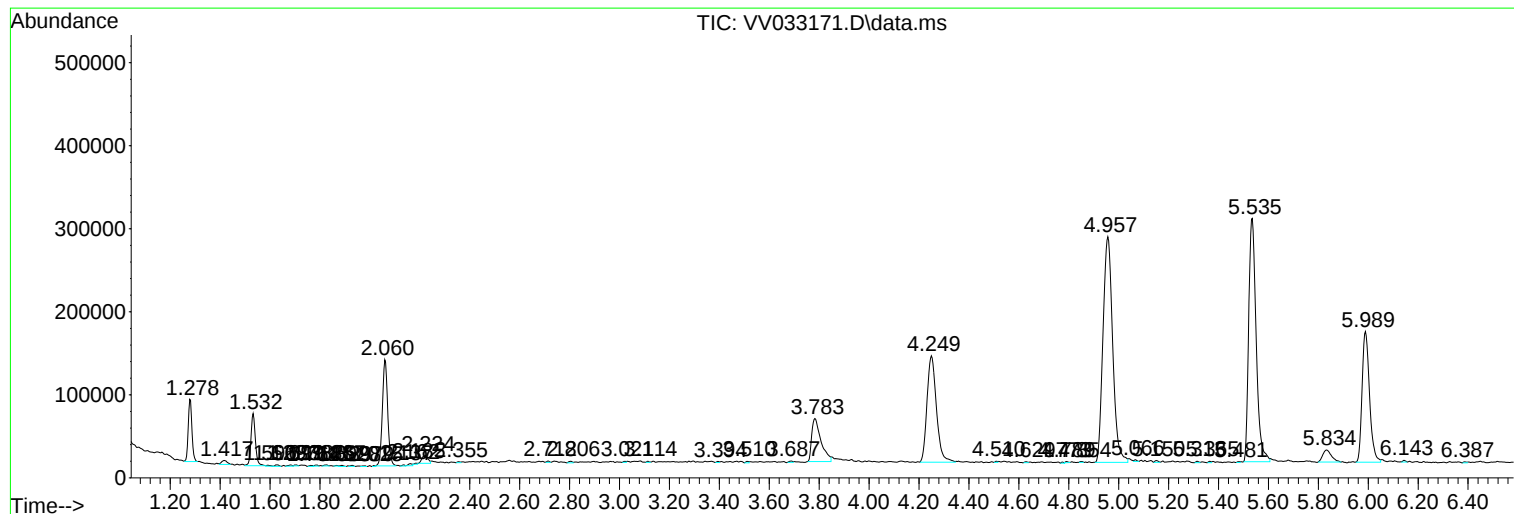

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033171.D
Acq On : 08 Dec 2023 01:06
Operator : SY/MD
Sample : 05689-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G93

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033171.D
Acq On : 08 Dec 2023 01:06
Operator : SY/MD
Sample : 05689-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G93

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------