

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033172.D
 Acq On : 08 Dec 2023 01:29
 Operator : SY/MD
 Sample : 05689-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G98

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M

Title : VOC Analysis

Signal : TIC: VV033172.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	86	rVB	77052	84064	10.97%	1.305%
2	1.339	91	93	97	rVB	1631	1088	0.14%	0.017%
3	1.417	111	117	129	rVB2	6761	10152	1.32%	0.158%
4	1.532	144	153	168	rVB	62517	76428	9.97%	1.186%
5	1.590	169	171	175	rVB	1006	679	0.09%	0.011%
6	1.626	179	182	187	rBV3	762	572	0.07%	0.009%
7	1.654	187	191	193	rBV2	409	346	0.05%	0.005%
8	1.671	194	196	200	rVB2	1048	673	0.09%	0.010%
9	1.690	200	202	203	rBV	711	345	0.05%	0.005%
10	1.700	203	205	209	rVB2	657	386	0.05%	0.006%
11	1.725	209	213	216	rBV3	949	674	0.09%	0.010%
12	1.741	216	218	223	rVB	1225	773	0.10%	0.012%
13	1.770	223	227	231	rBV	1204	1104	0.14%	0.017%
14	1.793	231	234	238	rBV	705	505	0.07%	0.008%
15	1.835	241	247	253	rBV2	1960	3024	0.39%	0.047%
16	1.860	253	255	256	rBV	663	296	0.04%	0.005%
17	1.966	285	288	299	rBV2	1677	2094	0.27%	0.032%
18	2.060	303	317	330	rBV	128203	188704	24.62%	2.929%
19	2.150	339	345	347	rBV	1494	1660	0.22%	0.026%
20	2.188	347	357	360	rVV	2235	4052	0.53%	0.063%
21	2.224	360	368	379	rVV3	8509	16952	2.21%	0.263%
22	2.355	405	409	410	rBV2	1604	1161	0.15%	0.018%
23	2.429	429	432	433	rBV	1198	703	0.09%	0.011%
24	2.555	468	471	473	rBV3	2080	1661	0.22%	0.026%
25	2.626	490	493	496	rBV2	1048	795	0.10%	0.012%
26	2.722	520	523	525	rBV	1277	1042	0.14%	0.016%
27	3.089	634	637	640	rBV	1311	822	0.11%	0.013%
28	3.275	690	695	698	rBV	3478	3156	0.41%	0.049%
29	3.407	734	736	739	rBV	1063	586	0.08%	0.009%
30	3.442	744	747	749	rBV	1605	918	0.12%	0.014%
31	3.490	759	762	766	rVB	1323	900	0.12%	0.014%
32	3.661	812	815	817	rBV	1550	1006	0.13%	0.016%
33	3.780	841	852	885	rBV2	76183	235377	30.71%	3.653%
34	4.047	932	935	939	rVB	1487	1229	0.16%	0.019%
35	4.249	984	998	1026	rVB	124642	317844	41.47%	4.933%
36	4.519	1079	1082	1085	rBV2	1415	1009	0.13%	0.016%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033172.D
 Acq On : 08 Dec 2023 01:29
 Operator : SY/MD
 Sample : 05689-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G98

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	4.645	1119	1121	1124	rVB	1198	689	0.09%	0.011%
38	4.696	1135	1137	1139	rBV3	912	555	0.07%	0.009%
39	4.783	1161	1164	1166	rBV	1291	848	0.11%	0.013%
40	4.857	1184	1187	1190	rBV2	1045	858	0.11%	0.013%
41	4.957	1202	1218	1239	rBV3	267756	717589	93.62%	11.137%
42	5.124	1267	1270	1273	rBV	1379	818	0.11%	0.013%
43	5.413	1357	1360	1362	rBV	1119	687	0.09%	0.011%
44	5.535	1386	1398	1427	rBV	283047	592670	77.32%	9.198%
45	5.828	1481	1489	1500	rBV5	14504	27531	3.59%	0.427%
46	5.937	1521	1523	1524	rBV	807	383	0.05%	0.006%
47	5.989	1527	1539	1560	rVV	157472	331438	43.24%	5.144%
48	6.104	1573	1575	1580	rVB	1413	1101	0.14%	0.017%
49	6.211	1605	1608	1614	rVB	1522	1086	0.14%	0.017%
50	6.465	1683	1687	1690	rBV2	1517	1492	0.19%	0.023%
51	6.809	1791	1794	1799	rBV	1005	998	0.13%	0.015%
52	6.915	1817	1827	1852	rBV	88362	169382	22.10%	2.629%
53	7.127	1890	1893	1897	rVB	1514	1112	0.15%	0.017%
54	7.243	1919	1929	1949	rBV	320479	567057	73.98%	8.801%
55	7.555	2017	2026	2047	rBV	65311	117335	15.31%	1.821%
56	7.735	2078	2082	2086	rBV3	1151	1421	0.19%	0.022%
57	8.024	2163	2172	2190	rBV	175432	334446	43.63%	5.191%
58	8.786	2398	2409	2433	rBV	460008	755766	98.60%	11.730%
59	9.288	2562	2565	2570	rBV2	1444	1352	0.18%	0.021%
60	9.519	2633	2637	2642	rBV6	2356	2784	0.36%	0.043%
61	9.596	2657	2661	2664	rBV2	1154	951	0.12%	0.015%
62	9.789	2718	2721	2724	rBV	1430	917	0.12%	0.014%
63	9.857	2740	2742	2744	rBV	902	397	0.05%	0.006%
64	10.059	2801	2805	2809	rBV2	1357	1444	0.19%	0.022%
65	10.085	2810	2813	2816	rVV	1018	749	0.10%	0.012%
66	10.153	2823	2834	2851	rBV	245543	385899	50.35%	5.989%
67	10.323	2885	2887	2890	rBV3	934	578	0.08%	0.009%
68	10.387	2903	2907	2911	rBV3	1479	1453	0.19%	0.023%
69	10.497	2937	2941	2944	rBV	1891	1578	0.21%	0.024%
70	10.599	2970	2973	2976	rVB	1125	762	0.10%	0.012%
71	10.995	3092	3096	3099	rBV	1483	1285	0.17%	0.020%
72	11.185	3144	3155	3179	rBV	493516	766508	100.00%	11.896%
73	11.561	3261	3272	3290	rBV	420386	658284	85.88%	10.217%
74	11.677	3305	3308	3312	rBV	1637	1362	0.18%	0.021%
75	11.924	3382	3385	3388	rVB	1709	977	0.13%	0.015%
76	11.943	3388	3391	3396	rBV	1213	1343	0.18%	0.021%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033172.D
 Acq On : 08 Dec 2023 01:29
 Operator : SY/MD
 Sample : 05689-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G98

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	12.059	3424	3427	3428	rBV	1090	725	0.09%	0.011%
78	12.889	3683	3685	3687	rBV2	906	410	0.05%	0.006%
79	12.947	3699	3703	3705	rBV2	1208	1056	0.14%	0.016%
80	13.069	3738	3741	3747	rBV2	1299	1301	0.17%	0.020%
81	13.136	3760	3762	3764	rBV	836	486	0.06%	0.008%
82	13.178	3771	3775	3778	rBV	2139	1967	0.26%	0.031%
83	13.304	3811	3814	3817	rBV	1570	990	0.13%	0.015%
84	13.384	3837	3839	3841	rBV	1161	661	0.09%	0.010%
85	13.770	3956	3959	3965	rBV	1603	1599	0.21%	0.025%
86	13.799	3965	3968	3972	rVB	1337	976	0.13%	0.015%
87	13.898	3997	3999	4003	rBV	1145	1117	0.15%	0.017%
88	14.059	4045	4049	4052	rBV	1382	1383	0.18%	0.021%
89	14.143	4073	4075	4077	rBV	1176	658	0.09%	0.010%
90	14.185	4085	4088	4095	rBV	1528	1223	0.16%	0.019%
91	14.249	4105	4108	4114	rVB	1772	1703	0.22%	0.026%
92	14.294	4118	4122	4123	rBV	1256	872	0.11%	0.014%
93	14.326	4130	4132	4136	rVB	1725	1096	0.14%	0.017%
94	15.030	4348	4351	4353	rVB	1521	917	0.12%	0.014%
95	15.136	4382	4384	4388	rVB	1697	977	0.13%	0.015%
96	15.268	4421	4425	4430	rBV2	1566	1892	0.25%	0.029%
97	15.345	4447	4449	4454	rBV2	1288	709	0.09%	0.011%
98	15.413	4467	4470	4475	rBV3	1835	1471	0.19%	0.023%
99	15.529	4503	4506	4511	rBV2	1641	1520	0.20%	0.024%
100	16.049	4666	4668	4671	rVB2	1916	861	0.11%	0.013%




Sum of corrected areas: 6443235

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033172.D
Acq On : 08 Dec 2023 01:29
Operator : SY/MD
Sample : 05689-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G98

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

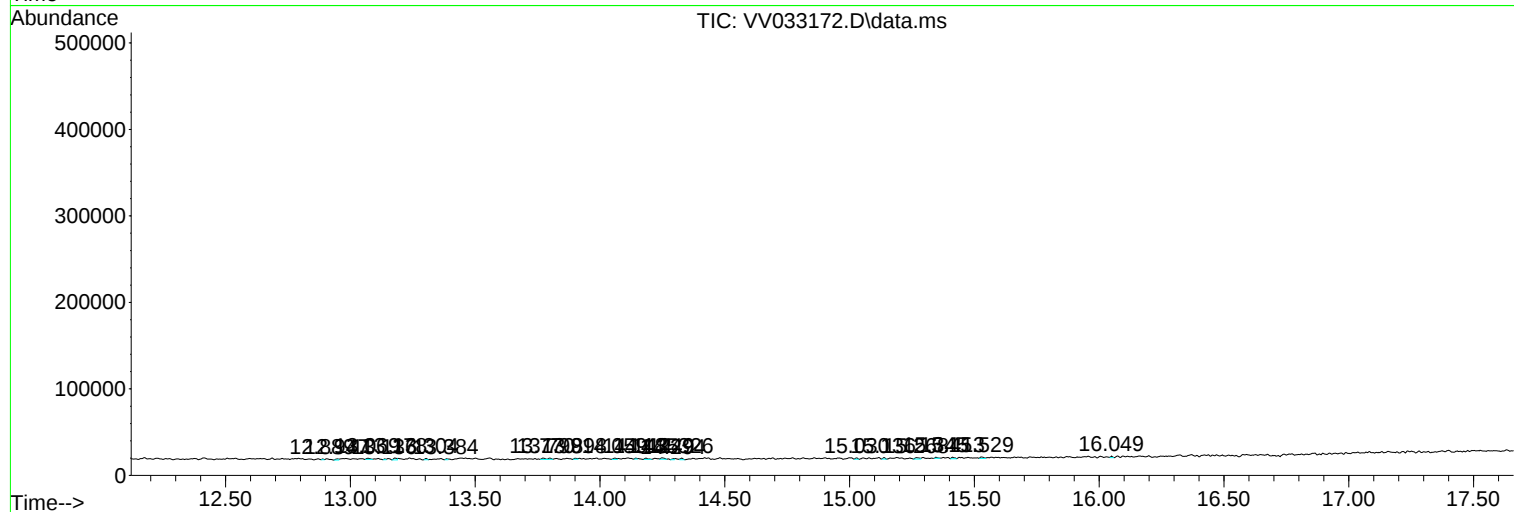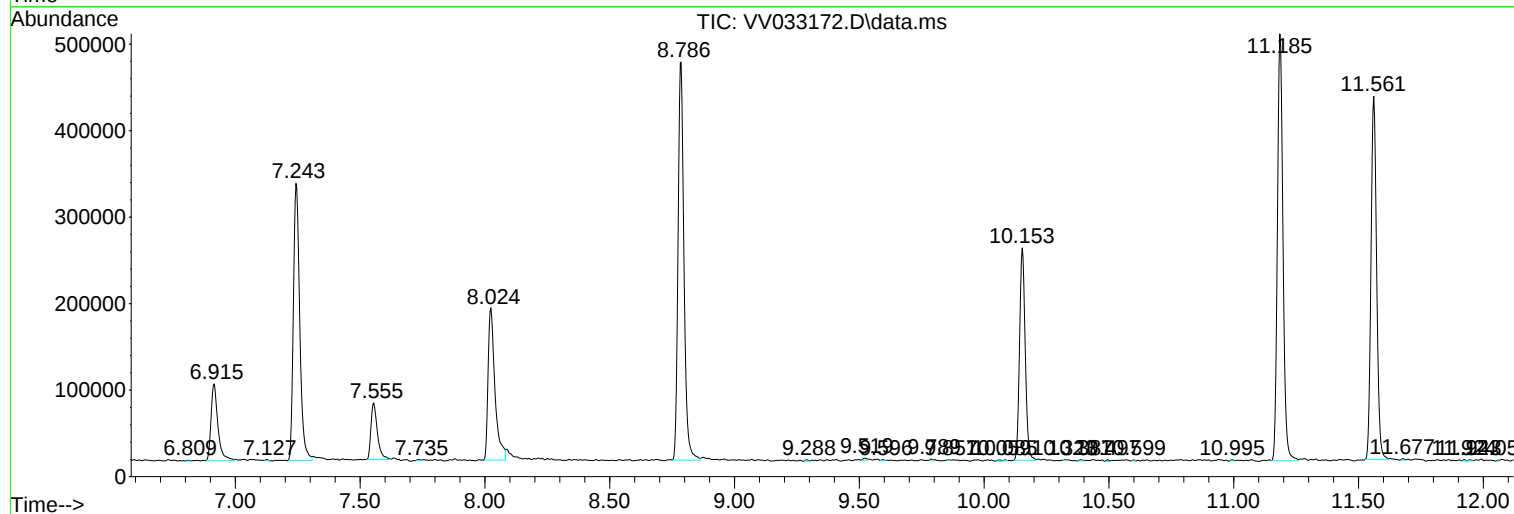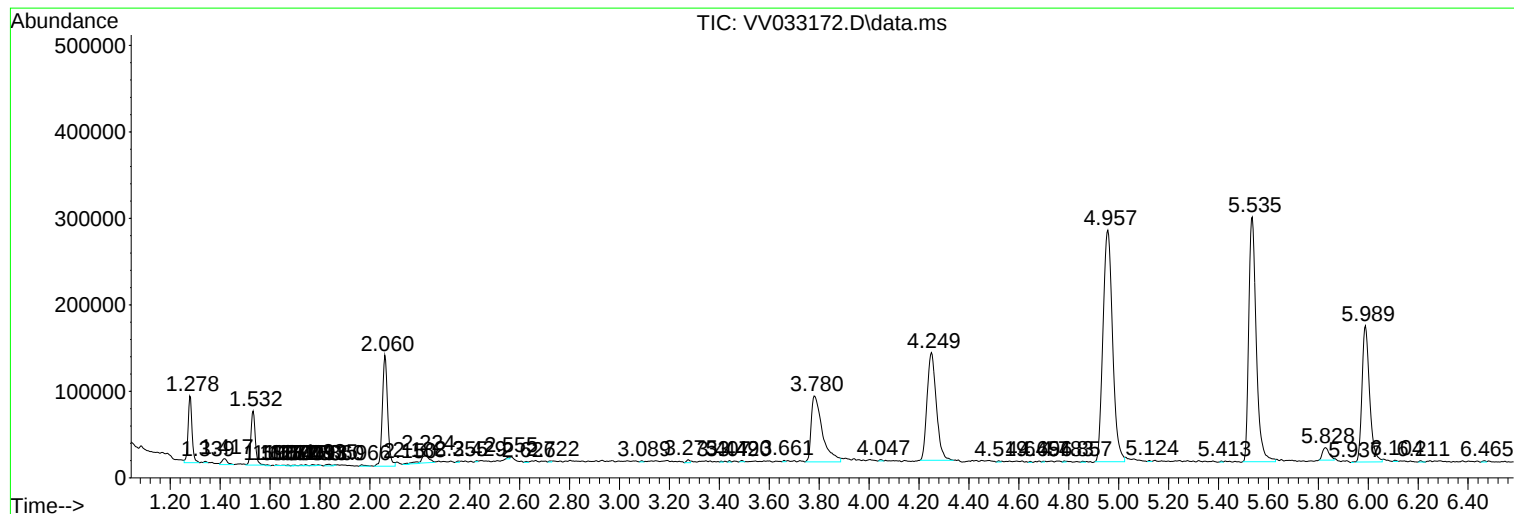

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033172.D
Acq On : 08 Dec 2023 01:29
Operator : SY/MD
Sample : 05689-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G98

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033172.D
Acq On : 08 Dec 2023 01:29
Operator : SY/MD
Sample : 05689-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G98

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc