

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033173.D
 Acq On : 08 Dec 2023 01:52
 Operator : SY/MD
 Sample : 05689-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GA1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VV033173.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	89	rVB	75290	82199	10.46%	1.239%
2	1.417	110	117	123	rVB3	4040	4429	0.56%	0.067%
3	1.532	144	153	164	rVB	60814	71780	9.13%	1.082%
4	1.581	164	168	171	rVB3	1403	1235	0.16%	0.019%
5	1.851	247	252	255	rBV2	999	949	0.12%	0.014%
6	1.941	277	280	284	rVB	1263	895	0.11%	0.013%
7	1.973	284	290	296	rBV6	2173	3617	0.46%	0.055%
8	2.021	299	305	307	rBV5	958	855	0.11%	0.013%
9	2.060	307	317	332	rBV2	127315	191373	24.34%	2.884%
10	2.118	332	335	341	rVB2	1987	1557	0.20%	0.023%
11	2.156	341	347	350	rBV	2087	2341	0.30%	0.035%
12	2.185	350	356	358	rBV2	2363	2495	0.32%	0.038%
13	2.217	359	366	379	rBV4	6149	12608	1.60%	0.190%
14	2.298	389	391	397	rVB	1566	1115	0.14%	0.017%
15	2.516	456	459	464	rBV2	1561	1553	0.20%	0.023%
16	2.748	528	531	535	rVB	1546	909	0.12%	0.014%
17	2.954	591	595	599	rVB	1560	1212	0.15%	0.018%
18	3.069	628	631	635	rBV	1118	1107	0.14%	0.017%
19	3.198	669	671	676	rVB	1452	1036	0.13%	0.016%
20	3.323	707	710	715	rBV2	1783	1979	0.25%	0.030%
21	3.577	786	789	795	rVB	1224	1069	0.14%	0.016%
22	3.610	795	799	803	rBV	1530	1442	0.18%	0.022%
23	3.786	844	854	879	rBV	49884	144002	18.32%	2.170%
24	3.944	900	903	905	rBV	1406	921	0.12%	0.014%
25	4.249	983	998	1018	rBV	125020	321561	40.90%	4.846%
26	4.439	1054	1057	1061	rVB	1628	1245	0.16%	0.019%
27	4.497	1072	1075	1079	rBV3	1424	1569	0.20%	0.024%
28	4.638	1116	1119	1125	rVB	1626	1332	0.17%	0.020%
29	4.690	1132	1135	1139	rBV	1594	1212	0.15%	0.018%
30	4.793	1163	1167	1170	rBV	2012	1381	0.18%	0.021%
31	4.809	1170	1172	1176	rBV	902	898	0.11%	0.014%
32	4.886	1193	1196	1199	rBV	1259	990	0.13%	0.015%
33	4.957	1203	1218	1243	rVV2	265798	712713	90.65%	10.740%
34	5.146	1275	1277	1285	rVB3	1749	1369	0.17%	0.021%
35	5.191	1289	1291	1294	rBV	1312	938	0.12%	0.014%
36	5.426	1362	1364	1369	rVB	1666	1253	0.16%	0.019%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033173.D
 Acq On : 08 Dec 2023 01:52
 Operator : SY/MD
 Sample : 05689-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GA1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	5.471	1375	1378	1381	rBV2	1647	1003	0.13%	0.015%
38	5.487	1381	1383	1385	rBV	1484	904	0.11%	0.014%
39	5.532	1387	1397	1419	rVV	295419	601631	76.52%	9.066%
40	5.693	1444	1447	1451	rBV	1636	1297	0.16%	0.020%
41	5.835	1478	1491	1516	rBV3	143212	302721	38.50%	4.562%
42	5.989	1528	1539	1566	rVB	157166	324050	41.22%	4.883%
43	6.458	1681	1685	1688	rBV	1542	1393	0.18%	0.021%
44	6.542	1707	1711	1713	rBV	1942	1528	0.19%	0.023%
45	6.619	1731	1735	1740	rBV2	966	1056	0.13%	0.016%
46	6.661	1744	1748	1750	rBV	1419	1256	0.16%	0.019%
47	6.915	1817	1827	1841	rBV2	88276	163151	20.75%	2.458%
48	7.108	1883	1887	1891	rBV3	1019	1140	0.15%	0.017%
49	7.146	1896	1899	1907	rVV3	1246	1530	0.19%	0.023%
50	7.243	1919	1929	1949	rBV	312690	552895	70.33%	8.331%
51	7.420	1981	1984	1986	rBV	1690	1264	0.16%	0.019%
52	7.494	2005	2007	2013	rVB	1413	1192	0.15%	0.018%
53	7.555	2017	2026	2045	rBV	66838	122182	15.54%	1.841%
54	7.722	2076	2078	2081	rBV3	1115	900	0.11%	0.014%
55	7.876	2116	2126	2130	rBV5	3588	6156	0.78%	0.093%
56	7.918	2135	2139	2143	rVB	1311	1117	0.14%	0.017%
57	8.024	2163	2172	2190	rBV	164177	302595	38.49%	4.560%
58	8.359	2273	2276	2280	rBV2	1721	1188	0.15%	0.018%
59	8.381	2280	2283	2288	rVV2	1314	1216	0.15%	0.018%
60	8.596	2347	2350	2353	rVB	1834	1171	0.15%	0.018%
61	8.616	2353	2356	2358	rBV	1787	1335	0.17%	0.020%
62	8.786	2398	2409	2434	rBV	468946	768257	97.72%	11.577%
63	9.227	2539	2546	2550	rBV	2335	3087	0.39%	0.047%
64	9.857	2739	2742	2747	rBV	1180	1037	0.13%	0.016%
65	9.899	2751	2755	2758	rBV	1465	1116	0.14%	0.017%
66	9.918	2758	2761	2764	rVB	1240	847	0.11%	0.013%
67	9.940	2764	2768	2772	rBV	1509	1328	0.17%	0.020%
68	10.075	2808	2810	2815	rBV	990	837	0.11%	0.013%
69	10.153	2824	2834	2857	rVB	246165	390715	49.70%	5.888%
70	10.317	2879	2885	2887	rBV	2421	2724	0.35%	0.041%
71	10.465	2928	2931	2935	rBV	1283	854	0.11%	0.013%
72	10.609	2970	2976	2979	rBV2	1838	2392	0.30%	0.036%
73	10.638	2983	2985	2990	rVB2	1838	1463	0.19%	0.022%
74	11.018	3099	3103	3108	rBV	1255	1791	0.23%	0.027%
75	11.088	3122	3125	3129	rBV	1927	1645	0.21%	0.025%
76	11.185	3144	3155	3174	rBV	510971	786192	100.00%	11.847%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033173.D
 Acq On : 08 Dec 2023 01:52
 Operator : SY/MD
 Sample : 05689-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GA1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	11.403	3221	3223	3226	rVB	1564	843	0.11%	0.013%
78	11.561	3261	3272	3294	rBV	424440	661017	84.08%	9.961%
79	12.111	3439	3443	3444	rBV	1232	1043	0.13%	0.016%
80	12.178	3460	3464	3468	rBV	1957	2038	0.26%	0.031%
81	12.645	3606	3609	3615	rVV2	1468	1939	0.25%	0.029%
82	12.673	3616	3618	3623	rVV	1601	1416	0.18%	0.021%
83	12.886	3680	3684	3687	rBV	1781	1644	0.21%	0.025%
84	13.088	3744	3747	3750	rBV	1425	1083	0.14%	0.016%
85	13.104	3750	3752	3757	rVV	1177	928	0.12%	0.014%
86	13.352	3827	3829	3833	rVB	1479	922	0.12%	0.014%
87	13.551	3887	3891	3894	rBV	1540	1260	0.16%	0.019%
88	13.728	3938	3946	3949	rBV	1934	2861	0.36%	0.043%
89	13.770	3954	3959	3964	rVV	1756	2220	0.28%	0.033%
90	13.934	4008	4010	4013	rBV	1341	979	0.12%	0.015%
91	14.294	4120	4122	4130	rVB2	1857	1871	0.24%	0.028%
92	14.632	4224	4227	4229	rBV3	1111	854	0.11%	0.013%
93	15.001	4339	4342	4350	rVB3	1583	1579	0.20%	0.024%
94	15.201	4401	4404	4409	rVB4	1604	1469	0.19%	0.022%
95	15.683	4552	4554	4556	rBV	1712	1083	0.14%	0.016%
96	15.773	4577	4582	4585	rBV	2429	2577	0.33%	0.039%
97	15.860	4606	4609	4611	rBV2	1424	924	0.12%	0.014%
98	15.943	4629	4635	4638	rBV	3076	3344	0.43%	0.050%
99	16.088	4677	4680	4683	rBV4	1768	1405	0.18%	0.021%
100	16.278	4737	4739	4742	rBV	2313	1649	0.21%	0.025%




Sum of corrected areas: 6636243

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033173.D
Acq On : 08 Dec 2023 01:52
Operator : SY/MD
Sample : 05689-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GA1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

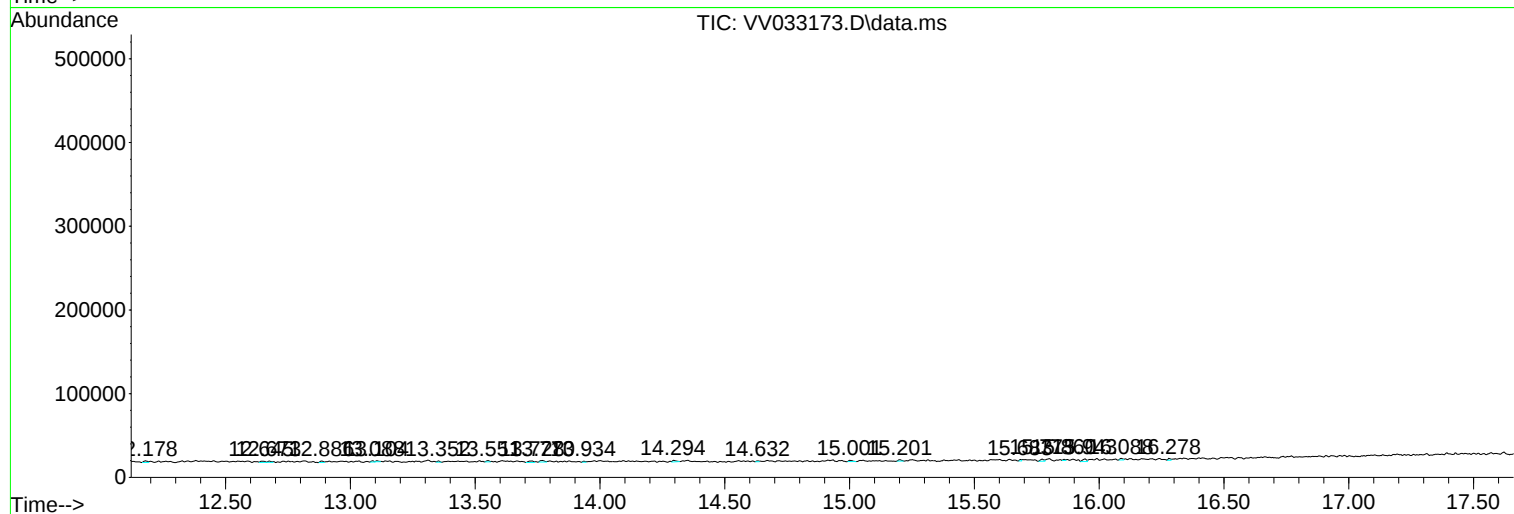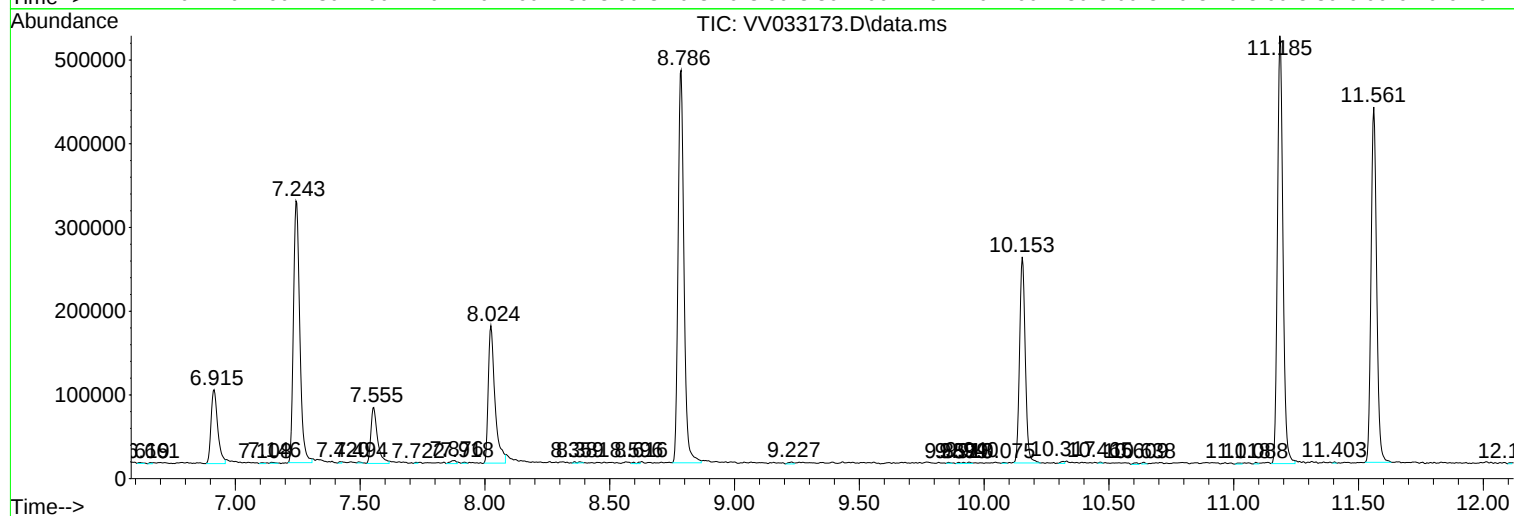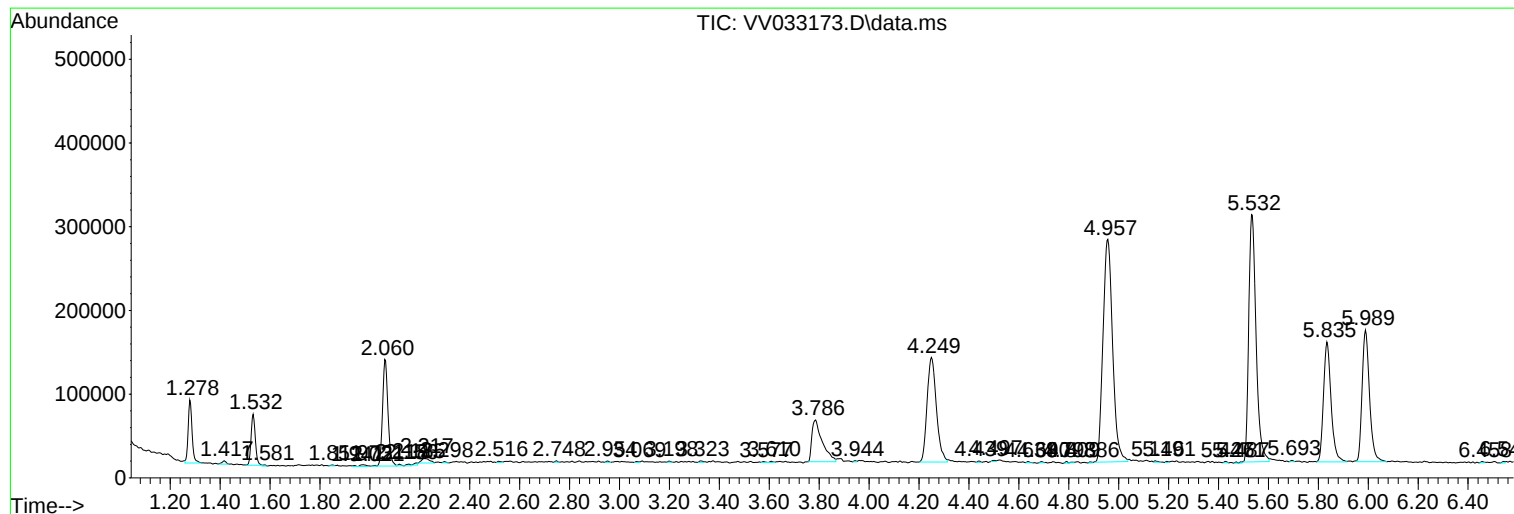

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033173.D
Acq On : 08 Dec 2023 01:52
Operator : SY/MD
Sample : 05689-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GA1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033173.D
Acq On : 08 Dec 2023 01:52
Operator : SY/MD
Sample : 05689-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GA1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc