

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033174.D
 Acq On : 08 Dec 2023 02:15
 Operator : SY/MD
 Sample : 05689-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GA2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VV033174.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	83	rVB	73131	75308	10.03%	1.224%
2	1.413	109	116	128	rVB4	5336	7879	1.05%	0.128%
3	1.462	128	131	136	rVB3	1693	1508	0.20%	0.025%
4	1.532	142	153	164	rBV	61085	73782	9.83%	1.200%
5	1.719	209	211	216	rVV2	916	964	0.13%	0.016%
6	1.780	228	230	236	rBV2	961	806	0.11%	0.013%
7	1.809	236	239	246	rVB2	1528	1343	0.18%	0.022%
8	1.844	246	250	253	rBV2	1129	897	0.12%	0.015%
9	1.889	258	264	267	rBV2	823	780	0.10%	0.013%
10	1.992	292	296	299	rVB	1201	872	0.12%	0.014%
11	2.015	299	303	307	rBV2	1314	1030	0.14%	0.017%
12	2.060	307	317	334	rVB	118286	172866	23.03%	2.811%
13	2.192	340	358	359	rBV	3953	6674	0.89%	0.109%
14	2.220	361	367	374	rBV	5052	7117	0.95%	0.116%
15	2.269	380	382	386	rBV	983	815	0.11%	0.013%
16	2.291	386	389	395	rVV	1620	1754	0.23%	0.029%
17	2.513	455	458	462	rBV	1650	1445	0.19%	0.023%
18	2.764	533	536	538	rBV	1389	1041	0.14%	0.017%
19	3.124	645	648	650	rBV	1602	928	0.12%	0.015%
20	3.391	726	731	737	rBV3	1193	1367	0.18%	0.022%
21	3.632	803	806	807	rBV	1569	907	0.12%	0.015%
22	3.780	844	852	870	rBV	51129	128178	17.07%	2.084%
23	4.011	921	924	930	rBV	1306	1366	0.18%	0.022%
24	4.249	983	998	1029	rBV	129467	334590	44.57%	5.440%
25	4.362	1030	1033	1036	rVV	1403	797	0.11%	0.013%
26	4.529	1082	1085	1088	rVB	1363	830	0.11%	0.013%
27	4.661	1124	1126	1133	rVB2	1001	853	0.11%	0.014%
28	4.802	1163	1170	1172	rBV	2156	2744	0.37%	0.045%
29	4.847	1180	1184	1188	rBV	1481	1663	0.22%	0.027%
30	4.889	1194	1197	1199	rBV	1615	1128	0.15%	0.018%
31	4.957	1202	1218	1241	rBV2	261718	697909	92.96%	11.347%
32	5.195	1288	1292	1295	rBV	1544	1183	0.16%	0.019%
33	5.362	1341	1344	1347	rBV2	1333	1328	0.18%	0.022%
34	5.535	1385	1398	1427	rBV	279237	586939	78.18%	9.543%
35	5.728	1455	1458	1462	rBV3	1135	983	0.13%	0.016%
36	5.828	1480	1489	1507	rVB4	11690	23552	3.14%	0.383%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033174.D
 Acq On : 08 Dec 2023 02:15
 Operator : SY/MD
 Sample : 05689-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GA2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	5.899	1507	1511	1520	rVB	2053	2383	0.32%	0.039%
38	5.989	1526	1539	1559	rBV	151916	314888	41.94%	5.120%
39	6.072	1563	1565	1568	rBV	1749	975	0.13%	0.016%
40	6.133	1582	1584	1587	rVB	1408	815	0.11%	0.013%
41	6.179	1595	1598	1601	rBV4	1019	852	0.11%	0.014%
42	6.648	1741	1744	1750	rBV2	1418	1322	0.18%	0.021%
43	6.741	1771	1773	1780	rVB	1497	1364	0.18%	0.022%
44	6.786	1784	1787	1790	rBV	933	774	0.10%	0.013%
45	6.912	1817	1826	1845	rBV2	84712	157196	20.94%	2.556%
46	7.079	1876	1878	1883	rBV	1441	1055	0.14%	0.017%
47	7.243	1919	1929	1946	rBV	299719	524407	69.85%	8.526%
48	7.555	2017	2026	2042	rBV	63689	113673	15.14%	1.848%
49	7.741	2081	2084	2086	rBV	1548	904	0.12%	0.015%
50	7.796	2098	2101	2106	rBV	1102	962	0.13%	0.016%
51	7.870	2116	2124	2125	rBV3	2246	2627	0.35%	0.043%
52	8.024	2163	2172	2206	rBV	172290	334083	44.50%	5.432%
53	8.297	2254	2257	2261	rBV2	1198	1105	0.15%	0.018%
54	8.323	2262	2265	2269	rVB	2357	1515	0.20%	0.025%
55	8.510	2321	2323	2329	rVB	1977	1473	0.20%	0.024%
56	8.632	2358	2361	2364	rBV	1232	1123	0.15%	0.018%
57	8.786	2398	2409	2426	rBV	440862	721890	96.15%	11.737%
58	8.940	2454	2457	2462	rBV2	1268	1076	0.14%	0.017%
59	9.127	2511	2515	2517	rBV3	1482	1289	0.17%	0.021%
60	9.391	2595	2597	2601	rVB	1403	824	0.11%	0.013%
61	9.439	2609	2612	2615	rBV2	1466	1089	0.15%	0.018%
62	9.461	2616	2619	2624	rVV2	1464	1285	0.17%	0.021%
63	9.635	2670	2673	2674	rBV	1231	731	0.10%	0.012%
64	9.966	2767	2776	2778	rBV4	2275	2991	0.40%	0.049%
65	10.063	2798	2806	2809	rBV	2167	2754	0.37%	0.045%
66	10.153	2823	2834	2853	rBV	247805	391487	52.15%	6.365%
67	10.320	2882	2886	2890	rBV4	2643	2730	0.36%	0.044%
68	10.622	2977	2980	2982	rBV	1148	807	0.11%	0.013%
69	10.770	3022	3026	3029	rBV2	1393	1198	0.16%	0.019%
70	10.805	3034	3037	3044	rVB2	1616	1894	0.25%	0.031%
71	10.847	3045	3050	3053	rBV	1277	1203	0.16%	0.020%
72	10.886	3059	3062	3065	rBV	1270	750	0.10%	0.012%
73	10.982	3087	3092	3093	rBV	1404	1279	0.17%	0.021%
74	11.185	3144	3155	3177	rBV	488700	750765	100.00%	12.206%
75	11.561	3261	3272	3295	rBV	402763	627024	83.52%	10.195%
76	11.915	3379	3382	3385	rVB	1594	1081	0.14%	0.018%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033174.D
 Acq On : 08 Dec 2023 02:15
 Operator : SY/MD
 Sample : 05689-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GA2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	12.108	3439	3442	3446	rVB	1924	1500	0.20%	0.024%
78	12.564	3581	3584	3587	rVB	1425	900	0.12%	0.015%
79	12.735	3634	3637	3642	rBV	1528	1407	0.19%	0.023%
80	12.776	3647	3650	3653	rVB	2011	1353	0.18%	0.022%
81	12.898	3686	3688	3691	rVB	1419	720	0.10%	0.012%
82	13.014	3721	3724	3727	rBV	1250	978	0.13%	0.016%
83	13.034	3728	3730	3735	rVB	1909	1377	0.18%	0.022%
84	13.114	3752	3755	3758	rVB	1772	1084	0.14%	0.018%
85	13.262	3798	3801	3805	rVB	1513	1178	0.16%	0.019%
86	13.371	3832	3835	3838	rBV	1318	823	0.11%	0.013%
87	13.715	3939	3942	3945	rBV2	1272	1020	0.14%	0.017%
88	13.921	4002	4006	4009	rBV	1529	1365	0.18%	0.022%
89	13.995	4025	4029	4032	rBV2	1448	1388	0.18%	0.023%
90	14.307	4123	4126	4129	rVB	1885	1164	0.16%	0.019%
91	14.458	4171	4173	4177	rVB	1806	1019	0.14%	0.017%
92	14.689	4240	4245	4246	rBV2	1389	1254	0.17%	0.020%
93	15.024	4346	4349	4352	rVB2	1403	856	0.11%	0.014%
94	15.062	4358	4361	4363	rBV	1461	764	0.10%	0.012%
95	15.390	4461	4463	4465	rBV	1138	752	0.10%	0.012%
96	15.445	4477	4480	4483	rBV	1536	1056	0.14%	0.017%
97	15.840	4600	4603	4607	rBV	1645	1483	0.20%	0.024%
98	16.004	4652	4654	4658	rVB2	2687	1711	0.23%	0.028%
99	16.313	4747	4750	4752	rBV2	1540	1006	0.13%	0.016%
100	17.136	5002	5006	5009	rBV	3133	2661	0.35%	0.043%




Sum of corrected areas: 6150588

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033174.D
Acq On : 08 Dec 2023 02:15
Operator : SY/MD
Sample : 05689-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GA2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

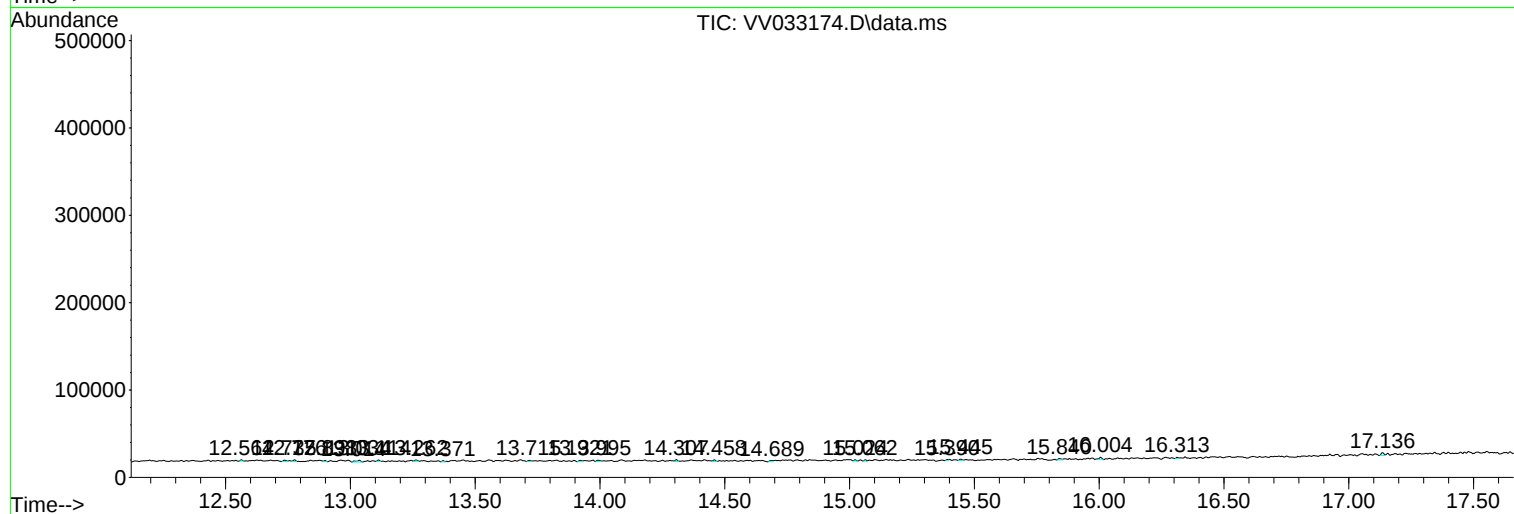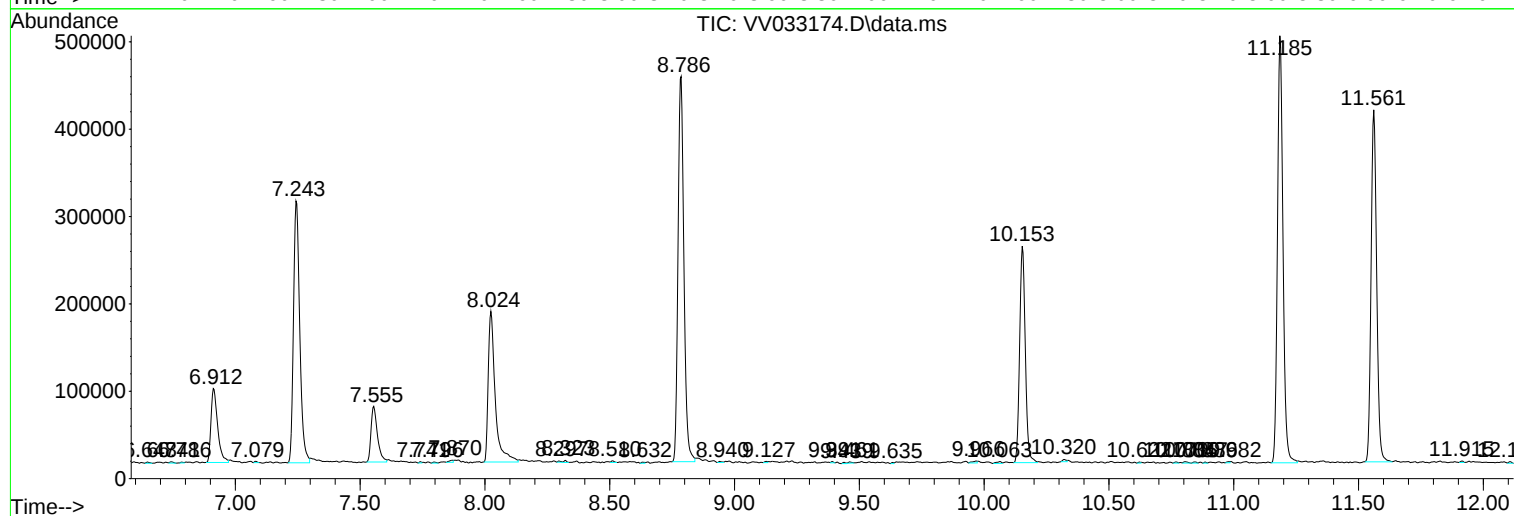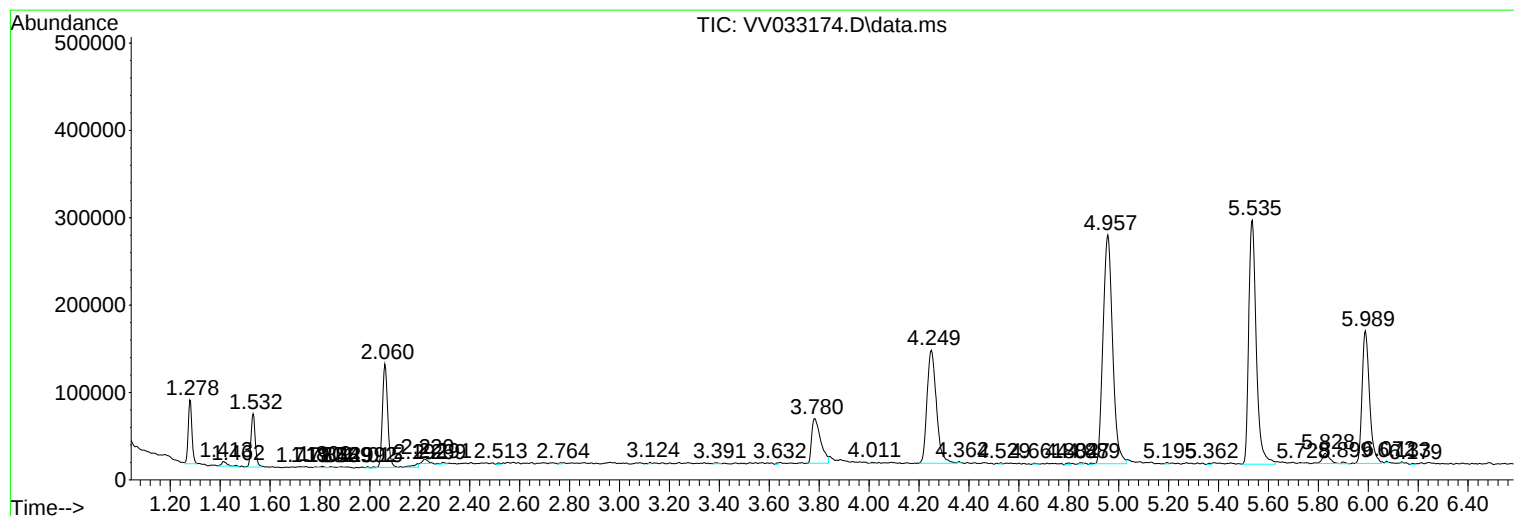

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033174.D
Acq On : 08 Dec 2023 02:15
Operator : SY/MD
Sample : 05689-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GA2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033174.D
Acq On : 08 Dec 2023 02:15
Operator : SY/MD
Sample : 05689-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GA2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------