
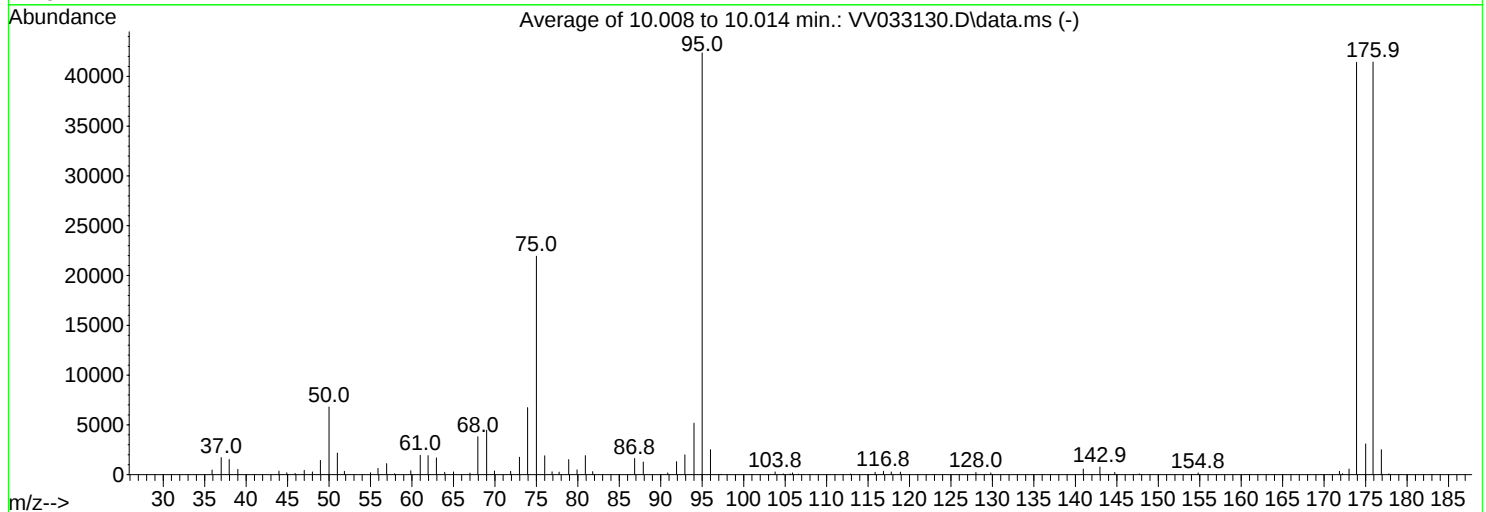


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033130.D
Acq On : 07 Dec 2023 08:25
Operator : SY/MD
Sample : BFB242
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB242

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Title : VOC Analysis
Last Update : Fri Dec 08 04:15:58 2023

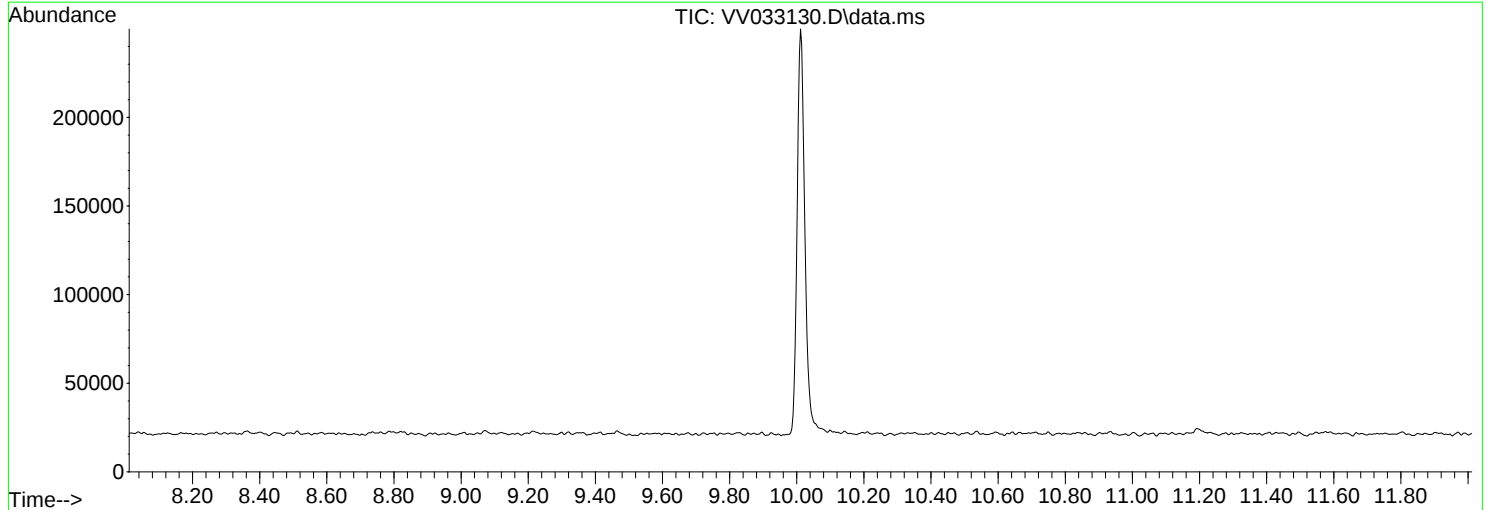

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2779

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.1	6801	PASS
75	95	30	80	51.8	21936	PASS
95	95	100	100	100.0	42365	PASS
96	95	5	9	5.9	2504	PASS
173	174	0.00	2	1.4	571	PASS
174	95	50	120	97.8	41416	PASS
175	174	5	9	7.4	3080	PASS
176	174	95	105	100.1	41440	PASS
177	176	5	10	6.1	2512	PASS

m/z	Abundance
39.10	182.0
39.90	20928.0

Instrument :
MSVOA_V
ClientSampleId :
BFB242

m/z	Abundance
35.90	460.0
37.00	1628.0
38.00	1464.0
39.00	780.0
39.90	20880.0
43.90	348.0
44.90	180.0
45.90	114.0
47.00	415.0
48.00	283.0
48.90	1480.0
50.00	6513.0
51.00	2224.0
51.80	326.0
55.00	168.0
55.90	635.0
57.00	1150.0
57.90	164.0
59.80	380.0
61.00	1943.0
62.00	1854.0
62.90	1759.0
63.90	241.0
65.00	196.0
67.00	179.0
68.00	3758.0
69.00	4458.0
70.00	385.0
71.90	333.0
72.90	1792.0
73.90	6612.0
75.00	21568.0
76.00	2075.0
76.90	293.0
77.80	250.0
78.90	1590.0
79.90	409.0
80.90	1925.0
81.80	319.0
86.90	1627.0
87.90	1306.0
91.00	189.0
91.90	1205.0
92.90	1864.0
94.00	5032.0
95.00	41608.0
96.00	2404.0
97.00	102.0
103.80	242.0
104.80	123.0
105.90	296.0
115.90	237.0
116.90	354.0
117.70	274.0
118.90	248.0
128.00	176.0
129.80	148.0
141.00	578.0
142.90	656.0
144.80	217.0
154.80	183.0
171.90	334.0
173.00	538.0
173.90	39856.0
175.00	2883.0
175.90	38944.0
176.90	2481.0
177.80	127.0

Instrument :
MSVOA_V
ClientSampleId :
BFB242

m/z	Abundance
35.90	494.0
37.00	1797.0
38.00	1588.0
39.00	721.0
39.90	20608.0
44.00	373.0
44.90	195.0
45.90	131.0
47.00	422.0
48.00	280.0
48.90	1468.0
50.00	7101.0
51.00	2225.0
51.80	373.0
55.00	192.0
55.90	649.0
57.00	1144.0
57.90	125.0
59.90	405.0
61.00	1998.0
61.90	1974.0
63.00	1742.0
63.90	237.0
65.00	300.0
67.00	185.0
67.90	3869.0
69.00	4658.0
69.90	382.0
71.90	367.0
72.90	1784.0
74.00	6836.0
75.00	22752.0
76.00	1925.0
76.90	301.0
77.70	277.0
78.90	1567.0
79.90	502.0
80.90	2026.0
81.80	296.0
86.80	1710.0
87.90	1291.0
90.80	168.0
91.90	1341.0
92.90	2049.0
94.00	5385.0
95.00	43856.0
96.00	2581.0
97.30	101.0
103.80	303.0
104.80	104.0
105.90	254.0
106.60	113.0
112.90	103.0
115.90	261.0
116.80	353.0
117.80	285.0
118.90	282.0
128.00	257.0
129.10	103.0
129.80	179.0
140.90	554.0
143.00	819.0
144.70	238.0
147.70	108.0
154.80	179.0
171.80	345.0
173.00	573.0
173.90	42936.0
175.00	3173.0
175.90	42880.0
176.90	2582.0
177.80	111.0

Instrument :
MSVOA_V
ClientSampleId :
BFB242

m/z	Abundance
35.90	432.0
37.00	1712.0
37.90	1512.0
39.00	647.0
39.90	20464.0
43.90	357.0
44.90	222.0
45.90	128.0
47.00	464.0
48.00	259.0
49.00	1352.0
50.00	6788.0
51.00	2062.0
51.90	310.0
55.00	220.0
55.90	600.0
56.90	1015.0
59.90	421.0
61.00	1909.0
62.00	1925.0
63.00	1568.0
64.00	226.0
65.00	333.0
67.00	141.0
67.90	3811.0
69.00	4310.0
69.90	348.0
71.90	298.0
73.00	1664.0
74.00	6735.0
75.00	21488.0
76.00	1712.0
76.90	289.0
77.70	240.0
78.90	1369.0
79.90	523.0
80.90	1807.0
81.80	313.0
86.80	1549.0
87.90	1209.0
90.80	180.0
91.90	1379.0
92.90	2079.0
94.00	5127.0
95.00	41632.0
96.00	2528.0
103.80	282.0
105.60	228.0
106.60	103.0
112.90	113.0
115.80	233.0
116.80	329.0
117.90	277.0
118.90	258.0
128.00	263.0
129.80	188.0
140.90	560.0
143.00	828.0
143.70	114.0
144.70	244.0
147.70	141.0
154.80	173.0
171.80	337.0
172.20	298.0
173.00	601.0
173.90	41456.0
175.00	3185.0
175.90	42496.0
176.90	2474.0

Instrument :
MSVOA_V
ClientSampleId :
BFB242