

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120821\
 Data File : VW023850.D
 Acq On : 08 Dec 2021 20:31
 Operator : SY/MD
 Sample : M4889-26
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CS0

Quant Time: Dec 09 00:35:38 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Dec 02 02:08:23 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	106459	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	107251	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	51384	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	39985	4.575	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	91.600%
7) Chloroethane-d5	1.568	69	33729	4.910	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	98.200%
11) 1,1-Dichloroethene-d2	2.108	63	54328	3.527	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	70.600%
20) 2-Butanone-d5	3.915	46	46301	44.070	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	88.140%
24) Chloroform-d	4.349	84	78023	5.127	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.600%
26) 1,2-Dichloroethane-d4	5.034	65	37691	5.302	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	106.000%
32) Benzene-d6	5.053	84	145519	4.981	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.600%
36) 1,2-Dichloropropane-d6	6.069	67	44013	5.374	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	107.400%
41) Toluene-d8	7.317	98	126733	4.643	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.800%
43) trans-1,3-Dichloroprop...	7.625	79	17861	5.410	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	108.200%
46) 2-Hexanone-d5	8.092	63	71101	64.819	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	129.640%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	31433	5.333	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	106.600%
66) 1,2-Dichlorobenzene-d4	11.625	152	52051	5.730	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	114.600%
Target Compounds					Qvalue	
42) Toluene	7.400	91	2300	0.069	ug/L	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120821\
Data File : VV023850.D
Acq On : 08 Dec 2021 20:31
Operator : SY/MD
Sample : M4889-26
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CS0


Quant Time: Dec 09 00:35:38 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Dec 02 02:08:23 2021
Response via : Initial Calibration

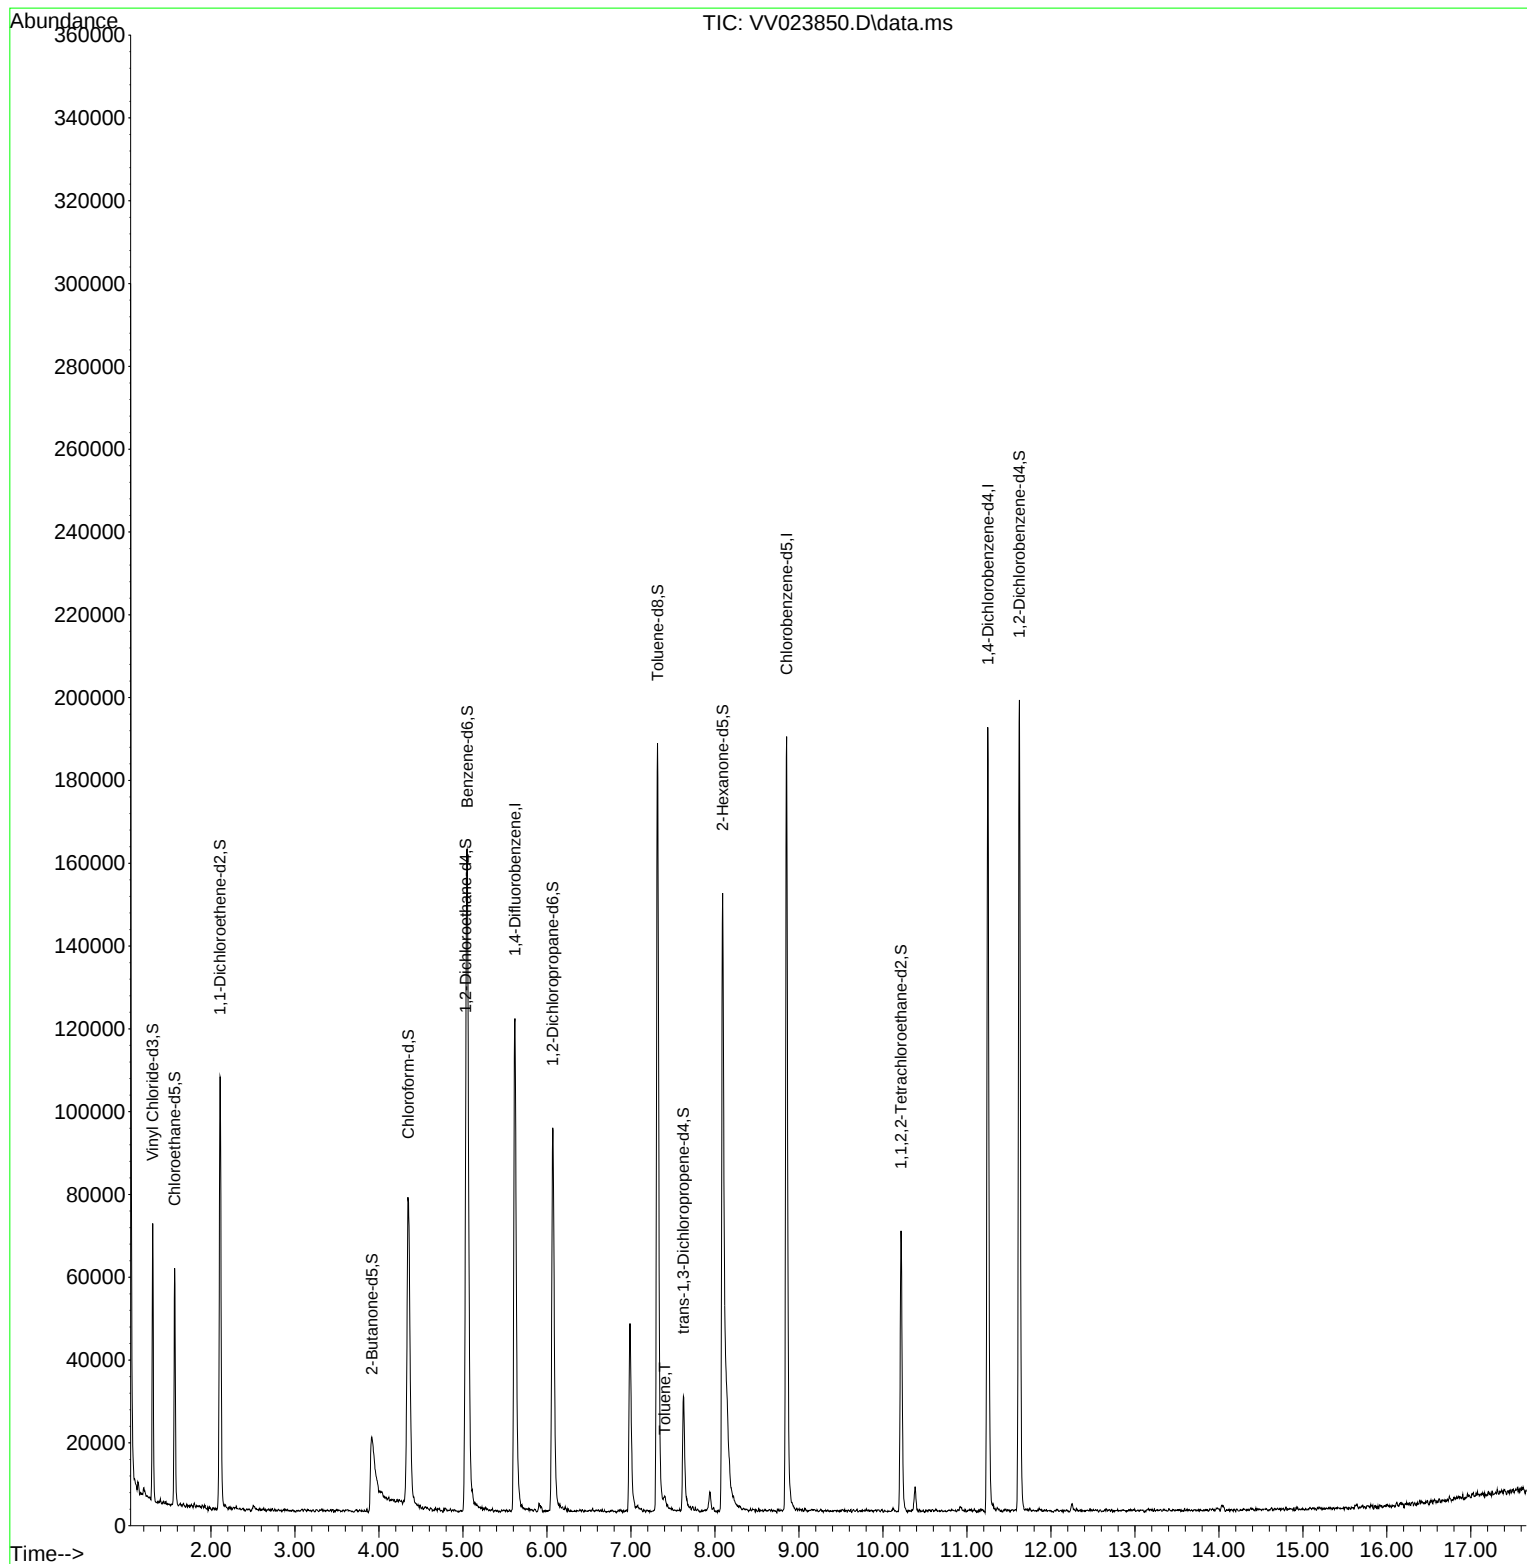

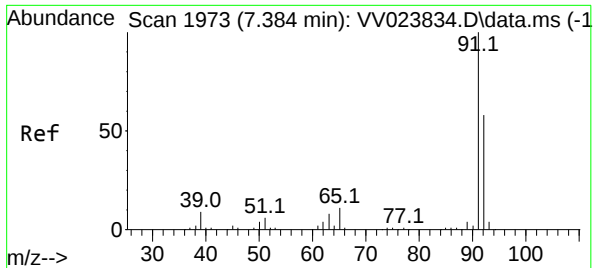

#42
 Toluene
 Concen: 0.069 ug/L
 RT: 7.400 min Scan# 1978
 Delta R.T. 0.016 min
 Lab File: VV023850.D
 Acq: 08 Dec 2021 20:31

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CS0

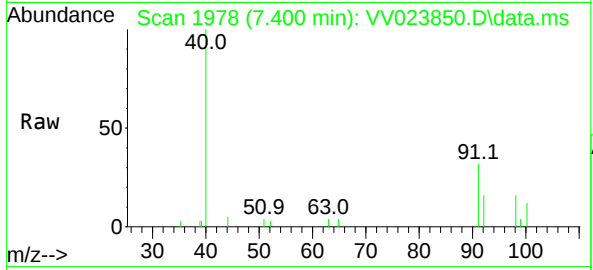

Tgt Ion: 91 Resp: 2300

Ion	Ratio	Lower	Upper
91	100		
92	48.5	41.5	77.1

