

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120821\
 Data File : VV023836.D
 Acq On : 08 Dec 2021 12:40
 Operator : SY/MD
 Sample : M4879-16
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV023836.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	94	rVB	72807	72286	16.98%	2.067%
2	1.568	156	164	177	rVB	57214	64290	15.10%	1.838%
3	2.108	320	332	349	rBV	109387	158222	37.16%	4.524%
4	2.507	447	456	470	rBV2	14126	23297	5.47%	0.666%
5	3.912	882	893	911	rBV2	17092	61742	14.50%	1.765%
6	4.346	1013	1028	1051	rVB2	75038	190485	44.74%	5.446%
7	5.043	1230	1245	1277	rBV2	165888	425790	100.00%	12.173%
8	5.613	1410	1422	1452	rBV	135915	279342	65.61%	7.986%
9	5.908	1503	1514	1525	rBV4	2566	4302	1.01%	0.123%
10	6.066	1550	1563	1590	rBV	93482	195875	46.00%	5.600%
11	6.985	1837	1849	1876	rBV2	49851	97064	22.80%	2.775%
12	7.313	1940	1951	1969	rBV	201413	353721	83.07%	10.113%
13	7.397	1972	1977	1988	rVB6	3074	5383	1.26%	0.154%
14	7.625	2038	2048	2071	rBV2	28339	55069	12.93%	1.574%
15	8.092	2182	2193	2233	rBV	152940	376298	88.38%	10.758%
16	8.850	2418	2429	2452	rBV	207554	344296	80.86%	9.844%
17	10.214	2842	2853	2871	rBV	66924	110959	26.06%	3.172%
18	11.249	3164	3175	3200	rBV	221964	345968	81.25%	9.891%
19	11.622	3279	3291	3309	rBV	210802	333303	78.28%	9.529%




Sum of corrected areas: 3497692

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120821\
Data File : VV023836.D
Acq On : 08 Dec 2021 12:40
Operator : SY/MD
Sample : M4879-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

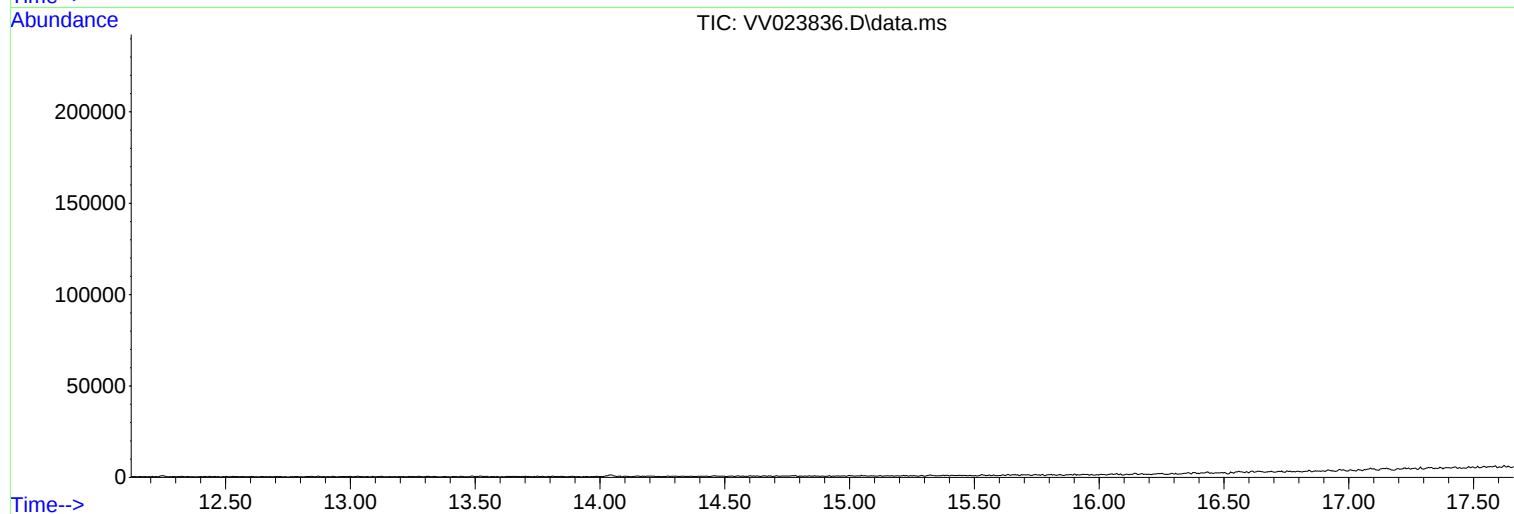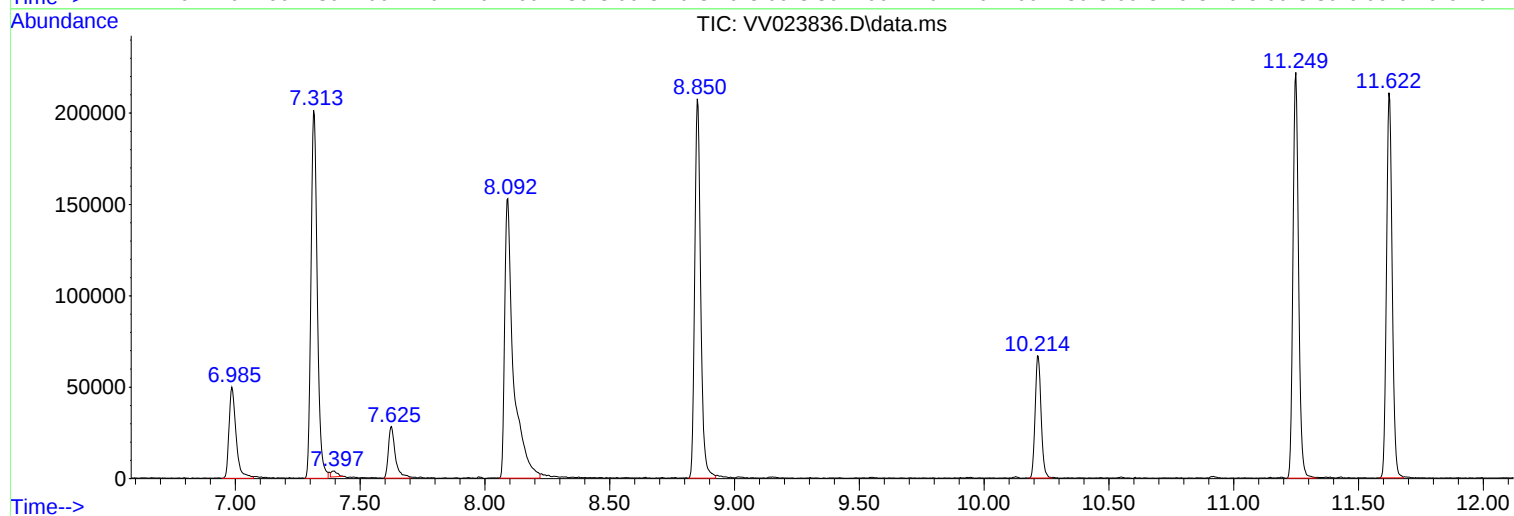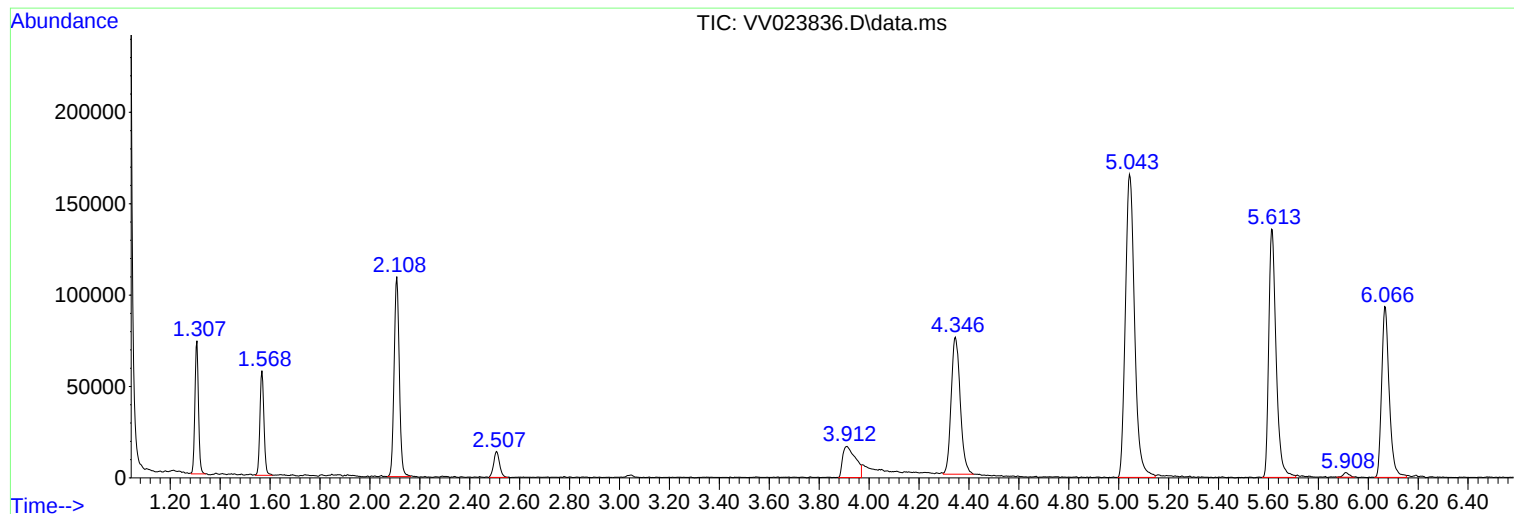

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120821\
Data File : VV023836.D
Acq On : 08 Dec 2021 12:40
Operator : SY/MD
Sample : M4879-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120821\
Data File : VV023836.D
Acq On : 08 Dec 2021 12:40
Operator : SY/MD
Sample : M4879-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc