

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120821\
 Data File : VV023838.D
 Acq On : 08 Dec 2021 15:46
 Operator : SY/MD
 Sample : M4889-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CN1

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.1 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV023838.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	98	rVB	74194	73180	16.96%	2.083%
2	1.568	156	164	178	rVB	58998	65410	15.16%	1.862%
3	2.108	321	332	344	rBV	112061	160780	37.26%	4.577%
4	3.912	883	893	911	rBV	16833	59362	13.76%	1.690%
5	4.349	1013	1029	1053	rVB2	80262	195806	45.37%	5.575%
6	5.050	1230	1247	1269	rBV2	171019	431529	100.00%	12.285%
7	5.616	1412	1423	1449	rBV	131319	272473	63.14%	7.757%
8	6.069	1551	1564	1585	rBV2	97231	205644	47.65%	5.855%
9	6.989	1840	1850	1868	rBV2	50351	93227	21.60%	2.654%
10	7.317	1940	1952	1973	rBV	203497	366085	84.83%	10.422%
11	7.397	1973	1977	1985	rVB4	3909	4861	1.13%	0.138%
12	7.625	2039	2048	2066	rBV2	28254	54024	12.52%	1.538%
13	7.937	2134	2145	2155	rBV3	3456	6945	1.61%	0.198%
14	8.092	2182	2193	2231	rBV	157808	390691	90.54%	11.123%
15	8.854	2419	2430	2454	rBV	199961	336130	77.89%	9.569%
16	10.217	2843	2854	2866	rBV	72377	116466	26.99%	3.316%
17	10.381	2898	2905	2914	rBV4	3340	4864	1.13%	0.138%
18	11.249	3164	3175	3193	rBV	212942	330874	76.67%	9.420%
19	11.625	3280	3292	3312	rBV	212648	339038	78.57%	9.652%
20	14.046	4035	4045	4050	rVB4	3692	5132	1.19%	0.146%




Sum of corrected areas: 3512521

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120821\
Data File : VV023838.D
Acq On : 08 Dec 2021 15:46
Operator : SY/MD
Sample : M4889-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CN1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

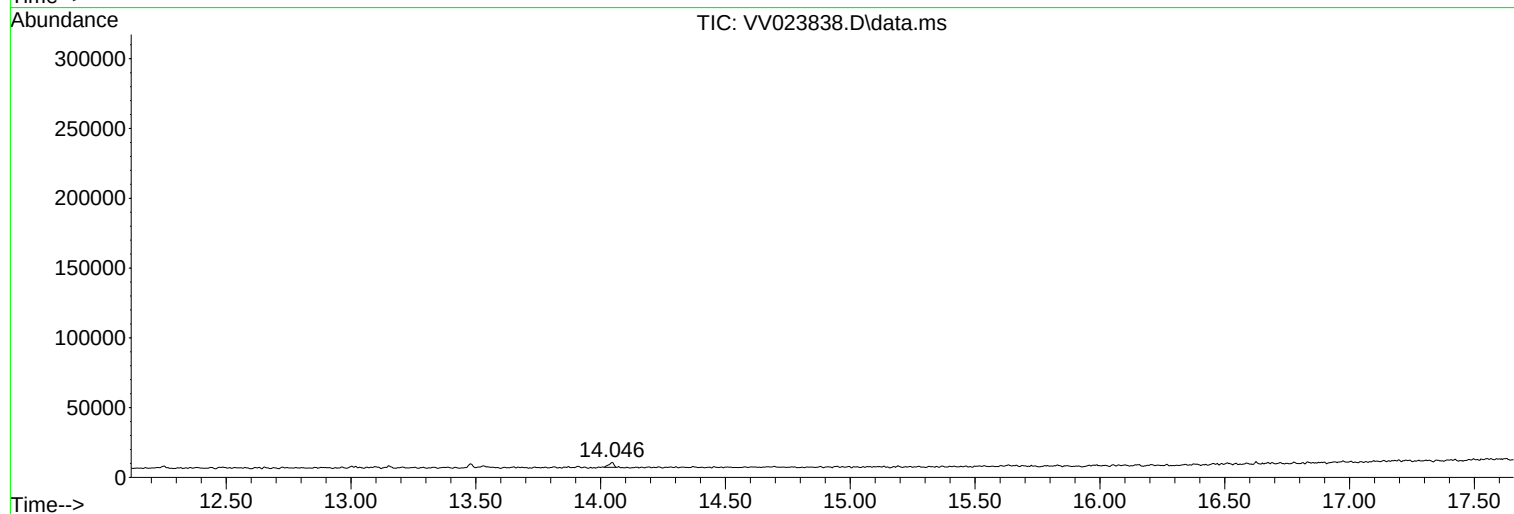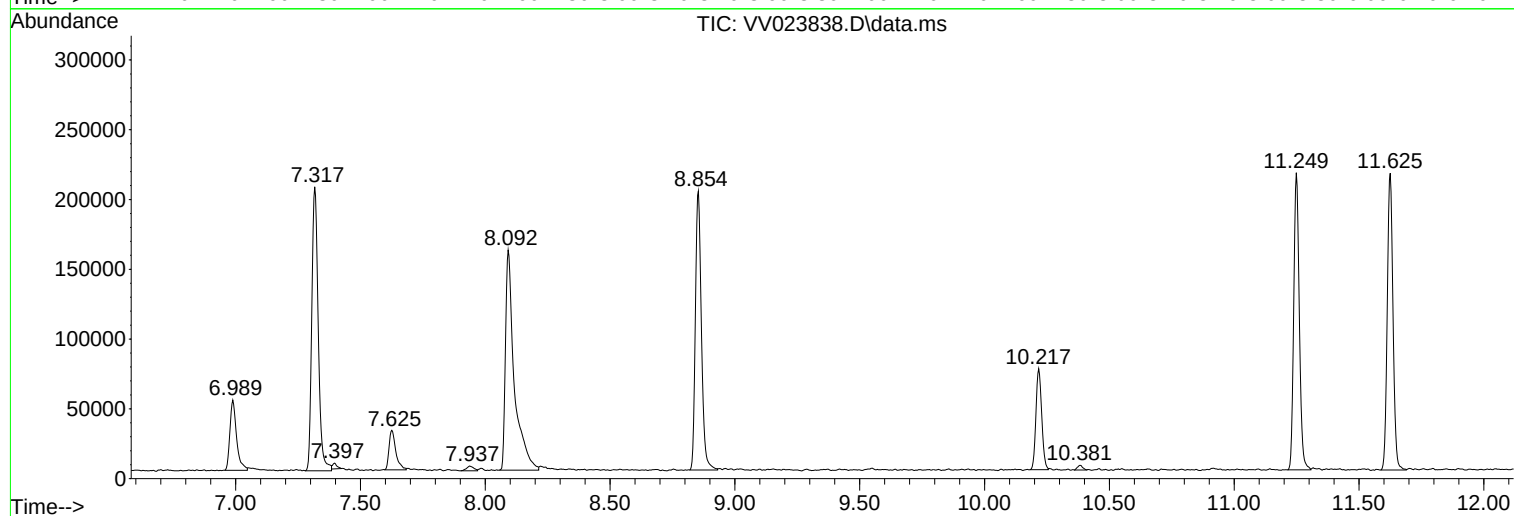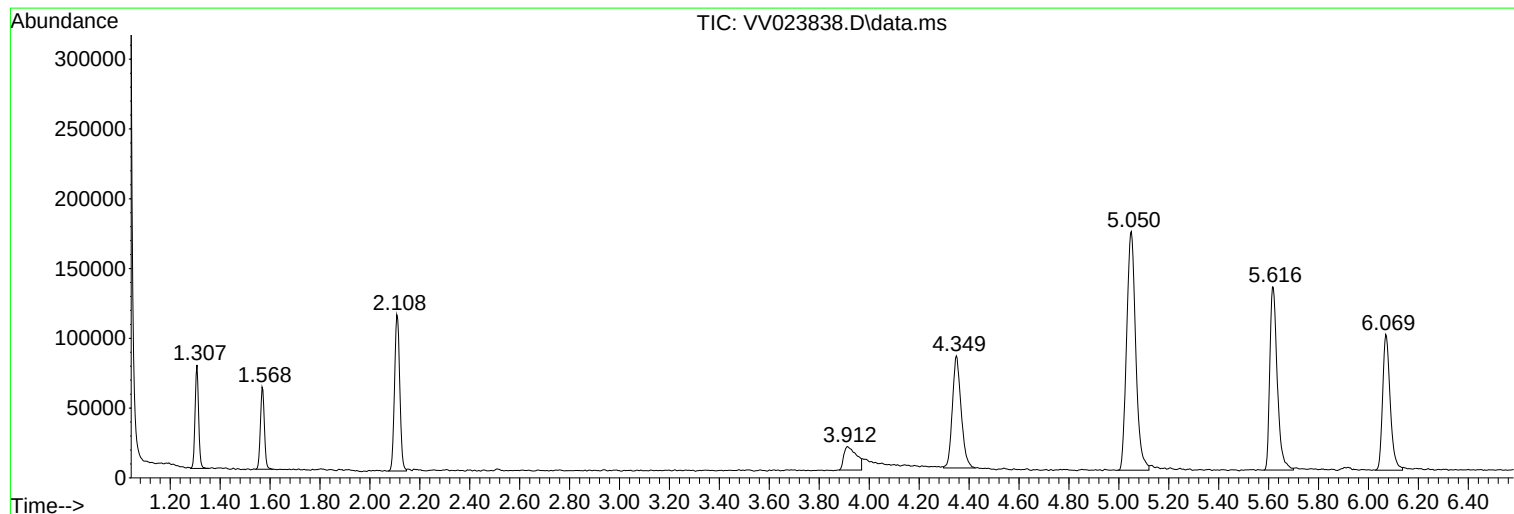

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120821\
Data File : VV023838.D
Acq On : 08 Dec 2021 15:46
Operator : SY/MD
Sample : M4889-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CN1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120821\
Data File : VV023838.D
Acq On : 08 Dec 2021 15:46
Operator : SY/MD
Sample : M4889-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CN1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
