

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120821\
 Data File : VV023840.D
 Acq On : 08 Dec 2021 16:33
 Operator : SY/MD
 Sample : M4889-16
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CN7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023840.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.198	44	49	58	rVB	13545	12939	3.28%	0.400%
2	1.304	74	82	92	rVB	68474	67822	17.18%	2.099%
3	1.564	156	163	179	rVB	54668	61516	15.58%	1.903%
4	2.105	318	331	345	rBV	104272	150842	38.20%	4.668%
5	3.912	882	893	913	rBV3	17617	70773	17.92%	2.190%
6	4.349	1014	1029	1051	rVB	72616	182320	46.17%	5.642%
7	5.047	1230	1246	1272	rBV2	155538	394848	100.00%	12.218%
8	5.616	1411	1423	1448	rBV	119913	244462	61.91%	7.564%
9	6.069	1552	1564	1591	rVB	86982	181137	45.88%	5.605%
10	6.989	1839	1850	1865	rBV2	44408	85167	21.57%	2.635%
11	7.317	1941	1952	1971	rBV	184399	329378	83.42%	10.192%
12	7.400	1975	1978	1991	rVB4	3674	5181	1.31%	0.160%
13	7.625	2039	2048	2064	rBV	27203	48348	12.24%	1.496%
14	7.937	2135	2145	2155	rBV2	4532	8204	2.08%	0.254%
15	8.092	2181	2193	2231	rBV2	149755	364597	92.34%	11.282%
16	8.854	2418	2430	2452	rVV	179337	299781	75.92%	9.276%
17	10.217	2835	2854	2867	rBV	66590	108466	27.47%	3.356%
18	10.384	2895	2906	2919	rBV4	5294	8854	2.24%	0.274%
19	11.249	3164	3175	3195	rBV	188372	296767	75.16%	9.183%
20	11.625	3281	3292	3307	rBV	193780	306191	77.55%	9.474%
21	14.040	4033	4043	4052	rBV2	2614	4154	1.05%	0.129%




Sum of corrected areas: 3231747

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120821\
Data File : VV023840.D
Acq On : 08 Dec 2021 16:33
Operator : SY/MD
Sample : M4889-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CN7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

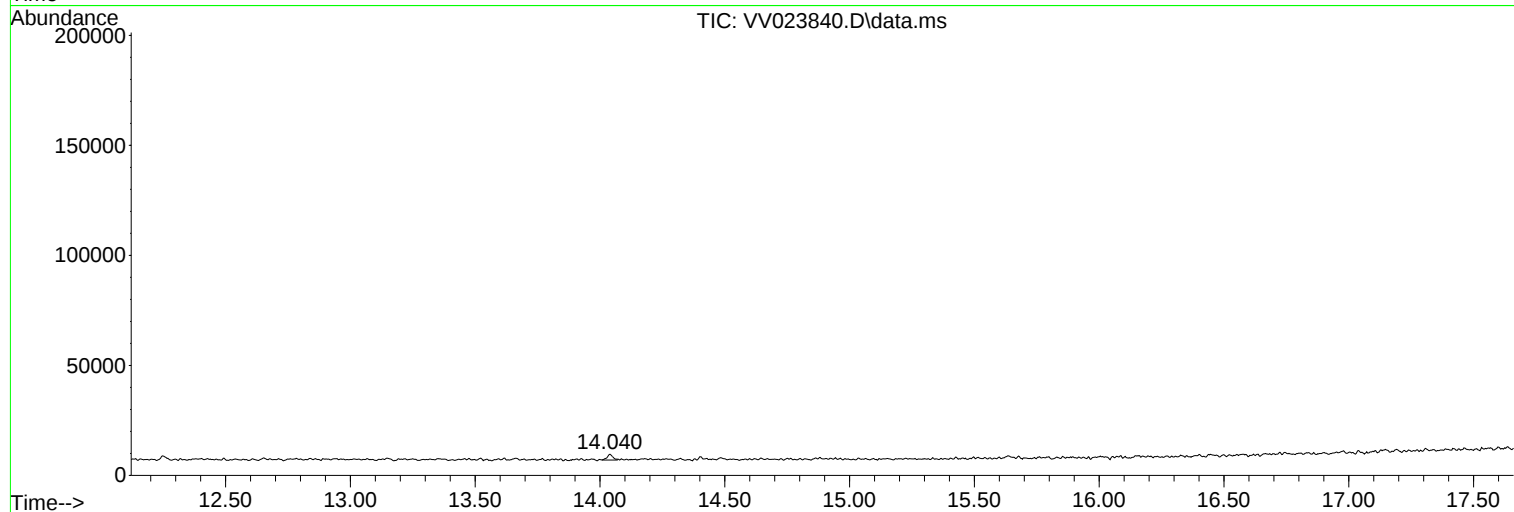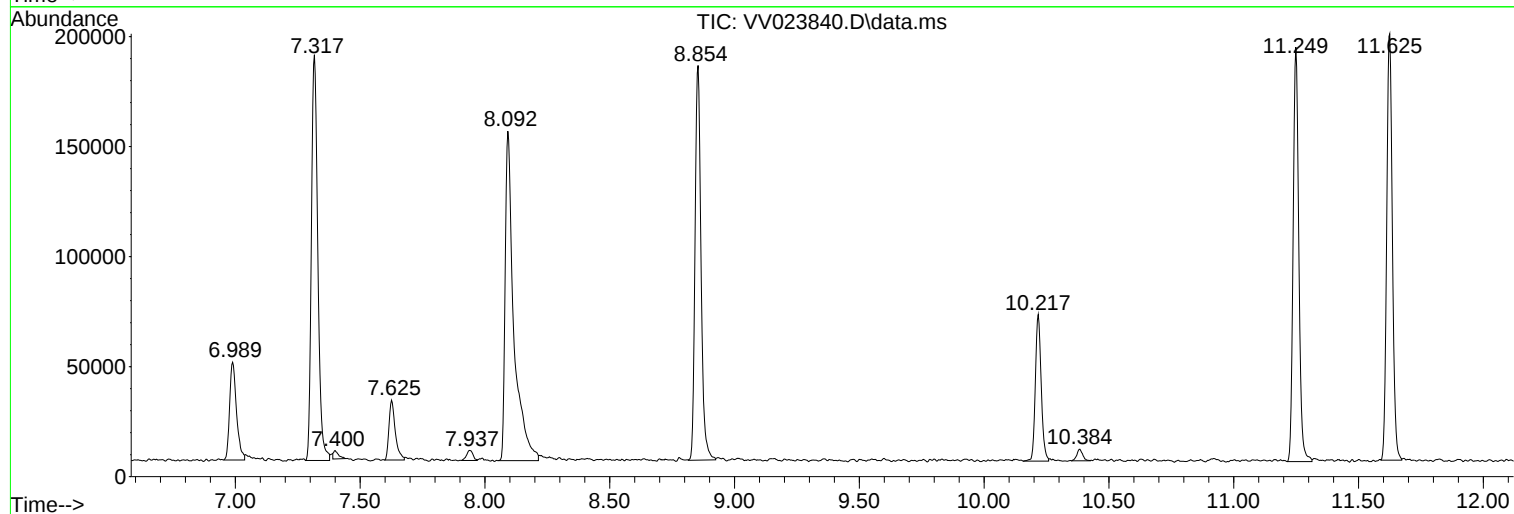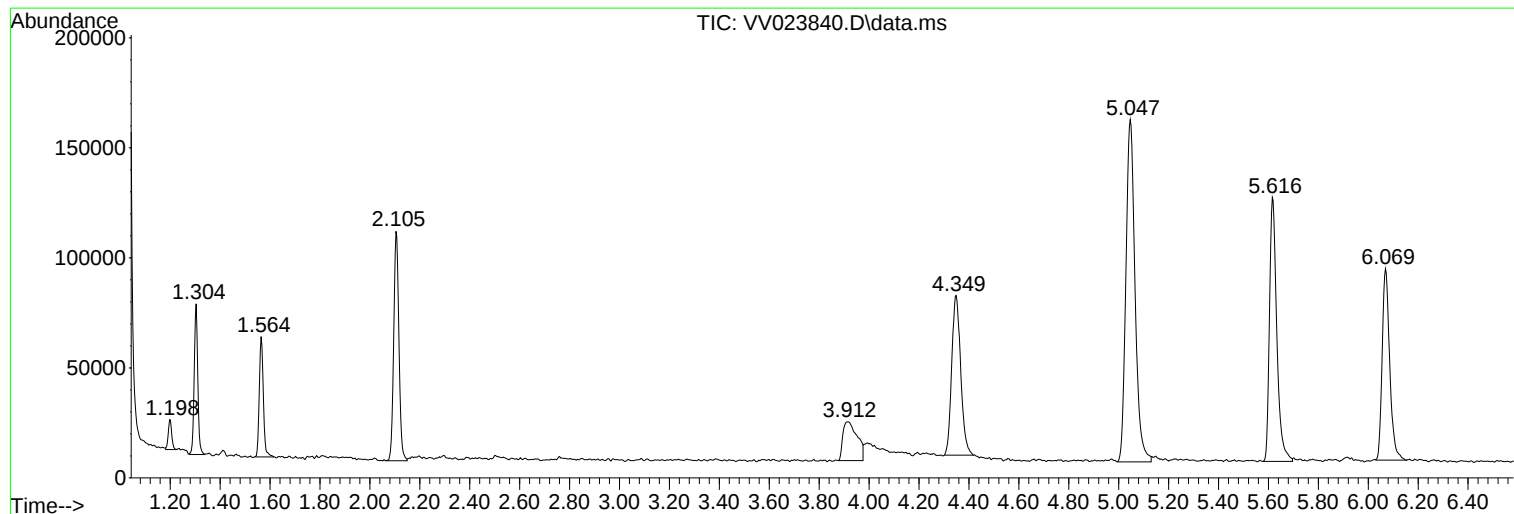

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120821\
Data File : VV023840.D
Acq On : 08 Dec 2021 16:33
Operator : SY/MD
Sample : M4889-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CN7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120821\
Data File : VV023840.D
Acq On : 08 Dec 2021 16:33
Operator : SY/MD
Sample : M4889-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CN7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
