

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120821\
 Data File : VV023841.D
 Acq On : 08 Dec 2021 16:57
 Operator : SY/MD
 Sample : M4889-17
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CP0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023841.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.201	46	50	60	rVB5	3879	4873	1.18%	0.145%
2	1.307	74	83	91	rBV	67836	68390	16.51%	2.031%
3	1.568	156	164	177	rBV	55736	63639	15.36%	1.890%
4	2.108	322	332	346	rBV	108292	156085	37.68%	4.635%
5	3.924	886	897	901	rBV2	17346	32323	7.80%	0.960%
6	4.355	1013	1031	1058	rVB2	75152	193309	46.66%	5.741%
7	5.050	1231	1247	1276	rBV2	162974	414252	100.00%	12.302%
8	5.619	1411	1424	1447	rBV	130635	268243	64.75%	7.966%
9	6.072	1549	1565	1586	rBV2	91633	195395	47.17%	5.803%
10	6.989	1839	1850	1872	rBV2	47127	91717	22.14%	2.724%
11	7.317	1940	1952	1972	rBV	189511	341778	82.50%	10.150%
12	7.625	2038	2048	2068	rBV2	27681	52033	12.56%	1.545%
13	7.940	2136	2146	2155	rVB4	4979	9268	2.24%	0.275%
14	8.095	2181	2194	2223	rBV	176058	375767	90.71%	11.160%
15	8.854	2419	2430	2450	rBV	195541	329916	79.64%	9.798%
16	10.217	2844	2854	2871	rVB2	69048	112195	27.08%	3.332%
17	10.381	2897	2905	2913	rBV2	6060	9174	2.21%	0.272%
18	11.249	3161	3175	3193	rBV	205874	322520	77.86%	9.578%
19	11.625	3280	3292	3311	rVB	202354	320063	77.26%	9.505%
20	14.043	4032	4044	4052	rBV4	3036	6297	1.52%	0.187%




Sum of corrected areas: 3367237

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120821\
Data File : VV023841.D
Acq On : 08 Dec 2021 16:57
Operator : SY/MD
Sample : M4889-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CP0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

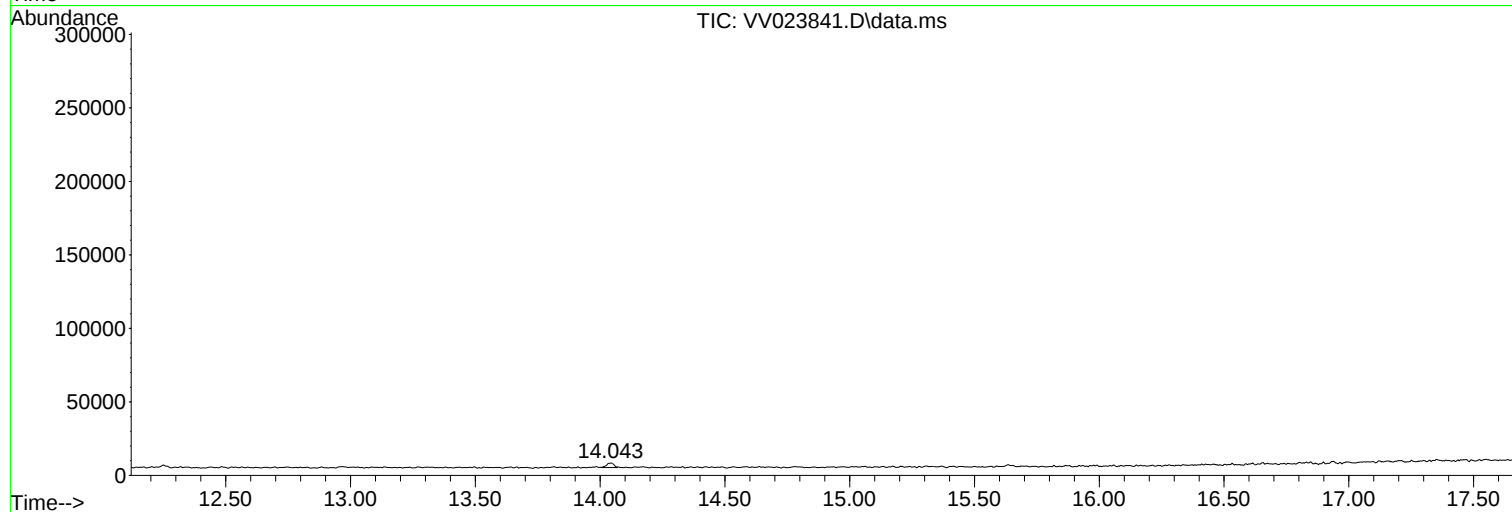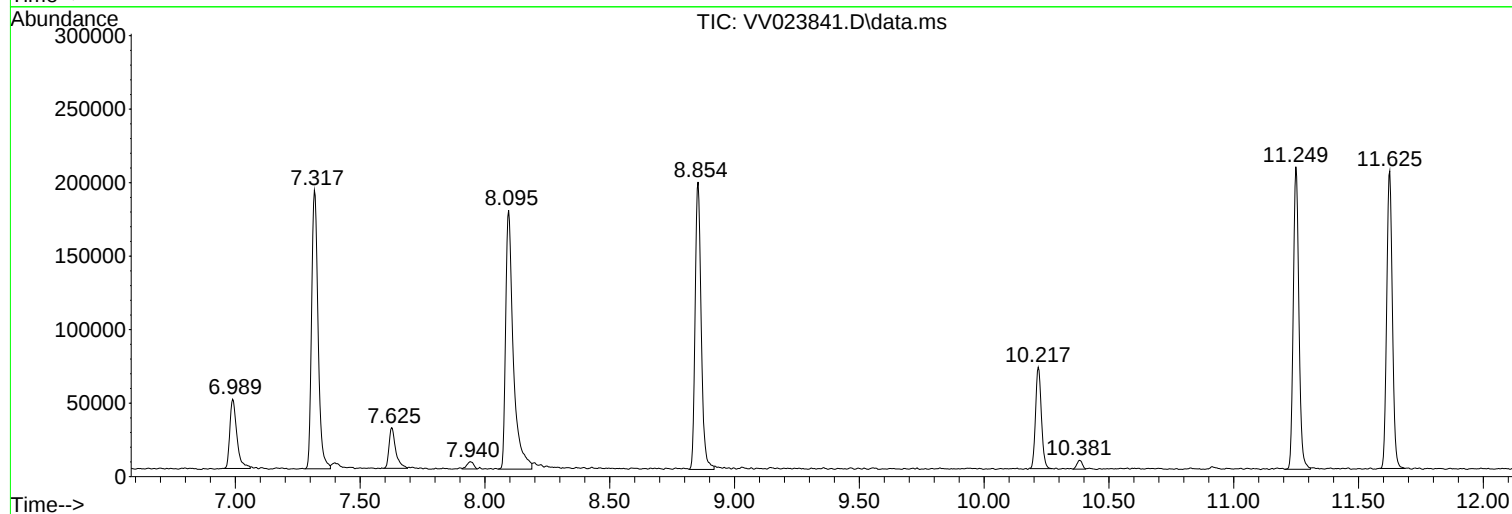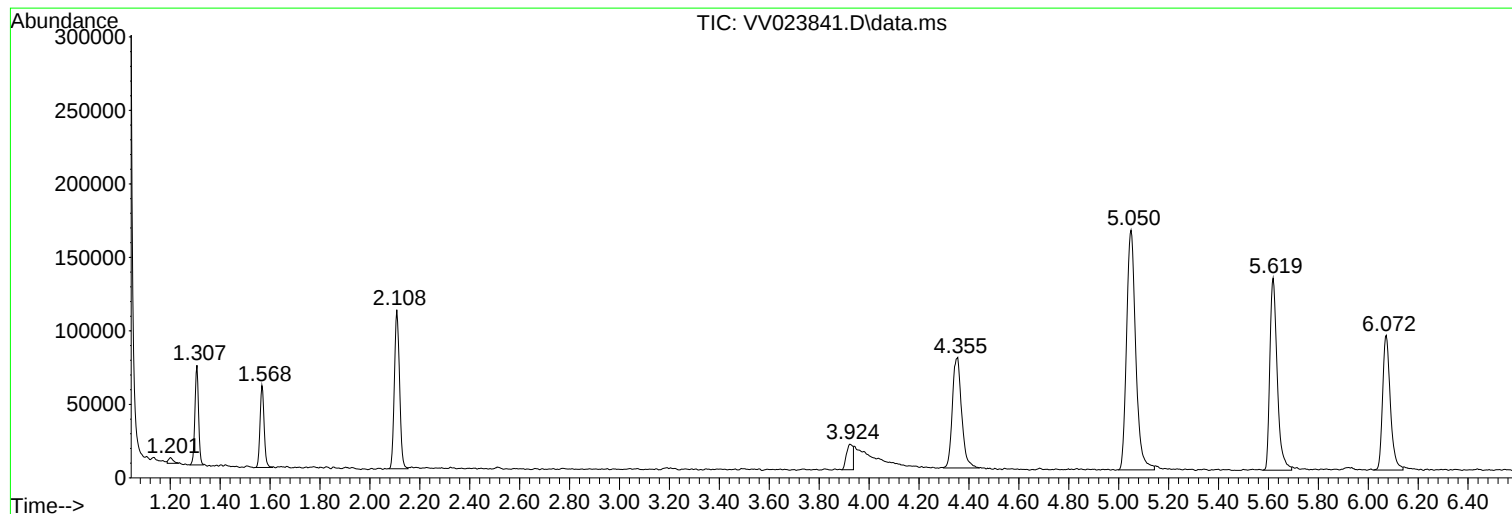

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120821\
Data File : VV023841.D
Acq On : 08 Dec 2021 16:57
Operator : SY/MD
Sample : M4889-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CP0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120821\
Data File : VV023841.D
Acq On : 08 Dec 2021 16:57
Operator : SY/MD
Sample : M4889-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CP0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc