

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120821\
 Data File : VV023842.D
 Acq On : 08 Dec 2021 17:21
 Operator : SY/MD
 Sample : M4889-18
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CP3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023842.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.201	45	50	57	rVB3	6164	6702	1.61%	0.192%
2	1.307	76	83	98	rVB	71384	74191	17.87%	2.125%
3	1.571	157	165	178	rVB	57411	66142	15.93%	1.894%
4	2.111	320	333	350	rBV	107464	158195	38.11%	4.531%
5	3.899	879	889	931	rBV	38070	153538	36.99%	4.398%
6	4.352	1013	1030	1051	rBV	77619	195051	46.99%	5.587%
7	5.050	1227	1247	1272	rBV2	165952	415083	100.00%	11.889%
8	5.619	1412	1424	1443	rBV	128615	261694	63.05%	7.495%
9	6.069	1552	1564	1585	rBV	92577	193971	46.73%	5.556%
10	6.989	1838	1850	1866	rBV2	48802	90135	21.71%	2.582%
11	7.317	1937	1952	1971	rBV	198732	348102	83.86%	9.970%
12	7.400	1971	1978	1987	rVB5	2624	4825	1.16%	0.138%
13	7.625	2039	2048	2065	rBV3	27950	52478	12.64%	1.503%
14	7.940	2139	2146	2154	rVB5	7171	11778	2.84%	0.337%
15	8.092	2183	2193	2217	rBV	204501	370304	89.21%	10.606%
16	8.854	2419	2430	2451	rBV	190759	324955	78.29%	9.307%
17	10.217	2841	2854	2866	rBV2	67647	109692	26.43%	3.142%
18	10.384	2897	2906	2917	rVB3	9501	14957	3.60%	0.428%
19	11.249	3162	3175	3191	rBV	204258	315545	76.02%	9.038%
20	11.622	3280	3291	3310	rBV	209153	324121	78.09%	9.283%




Sum of corrected areas: 3491459

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120821\
Data File : VV023842.D
Acq On : 08 Dec 2021 17:21
Operator : SY/MD
Sample : M4889-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CP3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

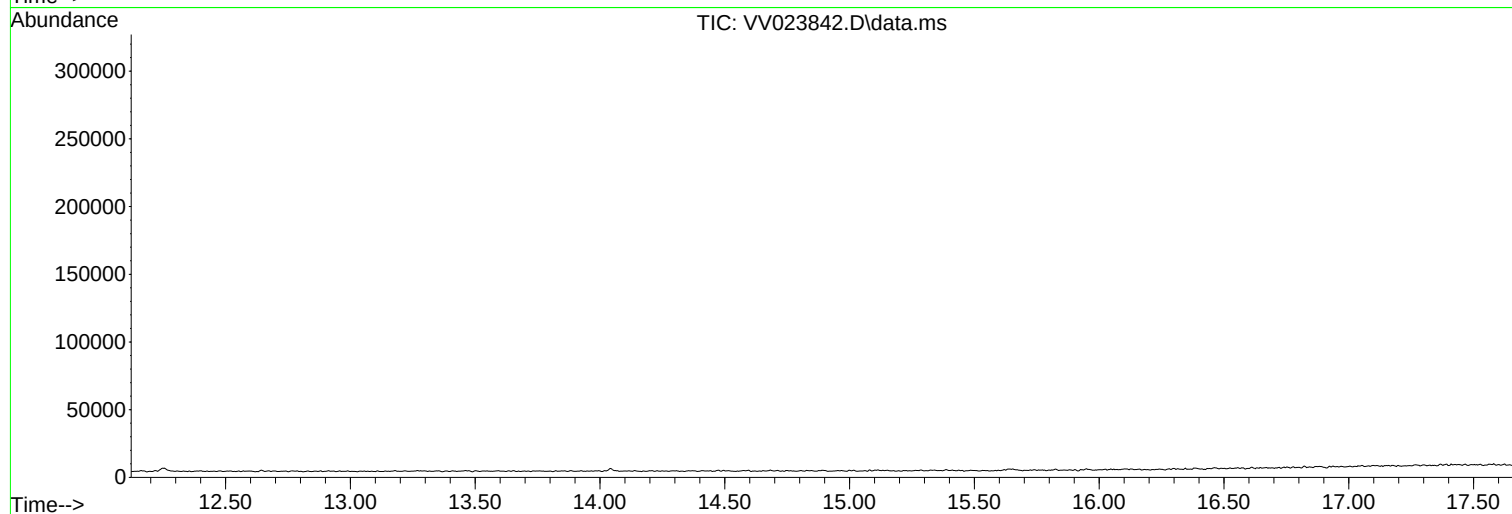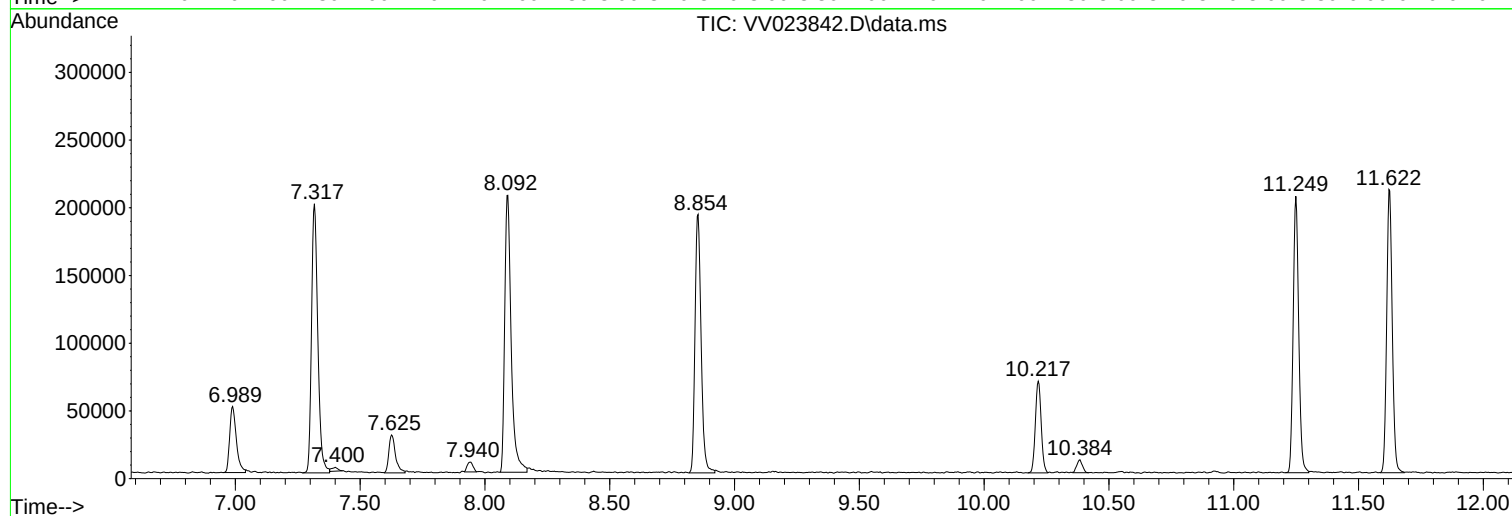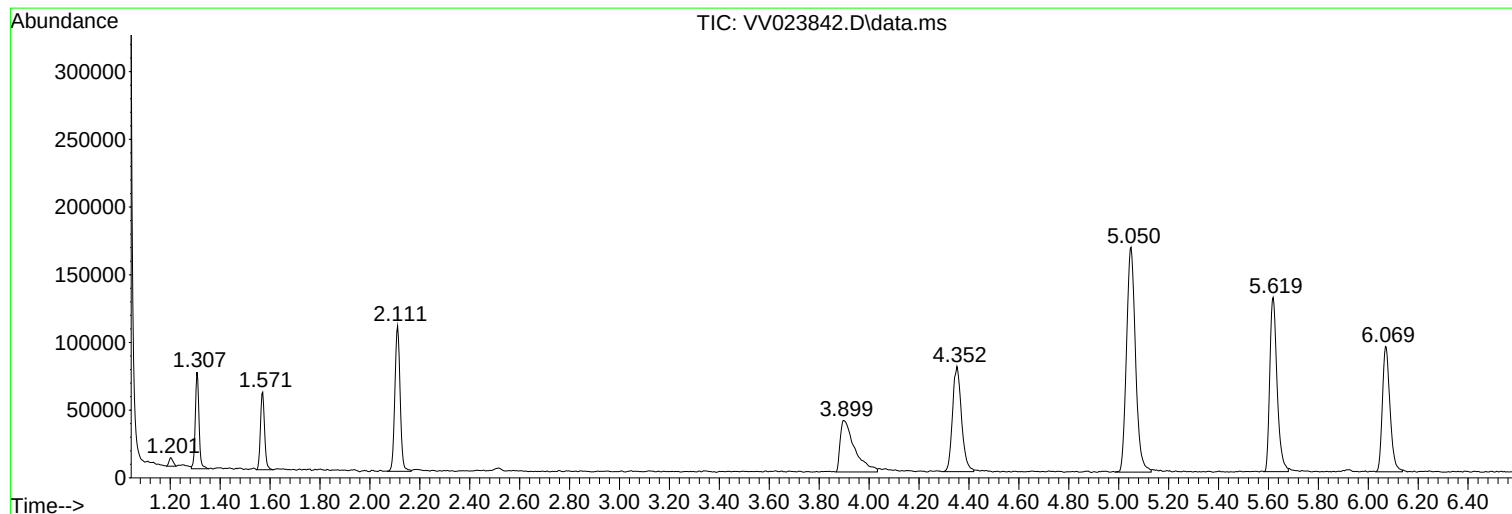

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120821\
Data File : VV023842.D
Acq On : 08 Dec 2021 17:21
Operator : SY/MD
Sample : M4889-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CP3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120821\
Data File : VV023842.D
Acq On : 08 Dec 2021 17:21
Operator : SY/MD
Sample : M4889-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CP3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc