

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120821\
 Data File : VV023843.D
 Acq On : 08 Dec 2021 17:44
 Operator : SY/MD
 Sample : M4889-19
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CP6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023843.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	97	rVB	70557	70512	17.30%	2.131%
2	1.568	157	164	178	rBV	57673	65563	16.08%	1.982%
3	2.108	322	332	349	rBV	105612	155508	38.15%	4.700%
4	3.912	884	893	896	rBV2	17449	29724	7.29%	0.898%
5	4.349	1014	1029	1052	rVB2	78224	191408	46.95%	5.785%
6	5.050	1232	1247	1270	rBV2	162262	407666	100.00%	12.322%
7	5.619	1410	1424	1448	rBV	124375	255276	62.62%	7.716%
8	5.915	1508	1516	1529	rVB8	2465	4804	1.18%	0.145%
9	6.069	1552	1564	1583	rBV	92618	191543	46.99%	5.789%
10	6.989	1836	1850	1872	rBV2	46990	92234	22.62%	2.788%
11	7.317	1941	1952	1971	rBV	191272	344075	84.40%	10.400%
12	7.625	2039	2048	2076	rVB	27720	51838	12.72%	1.567%
13	7.940	2135	2146	2154	rBV3	4246	7790	1.91%	0.235%
14	8.091	2183	2193	2226	rBV	159875	373568	91.64%	11.291%
15	8.853	2418	2430	2451	rBV	187430	314818	77.22%	9.515%
16	10.217	2843	2854	2868	rBV	68452	112646	27.63%	3.405%
17	10.381	2898	2905	2918	rVB3	5806	10308	2.53%	0.312%
18	11.249	3164	3175	3190	rBV	201575	305022	74.82%	9.219%
19	11.625	3279	3292	3313	rVB	200227	319852	78.46%	9.667%
20	12.249	3477	3486	3496	rVB4	2198	4408	1.08%	0.133%




Sum of corrected areas: 3308563

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120821\
Data File : VV023843.D
Acq On : 08 Dec 2021 17:44
Operator : SY/MD
Sample : M4889-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CP6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

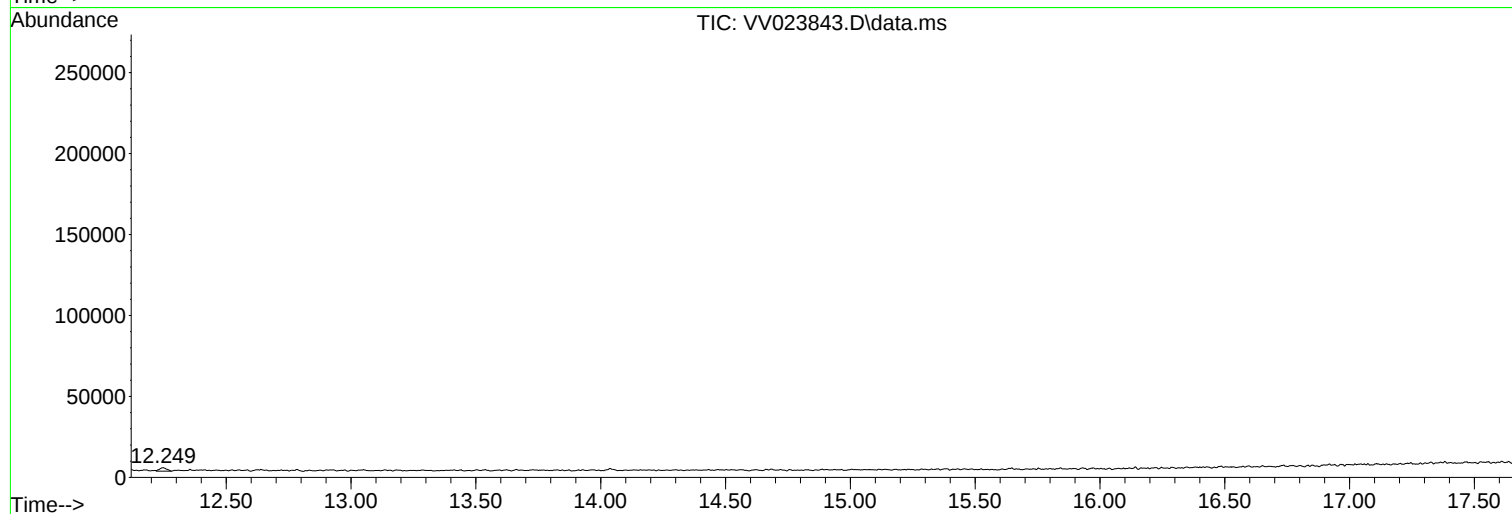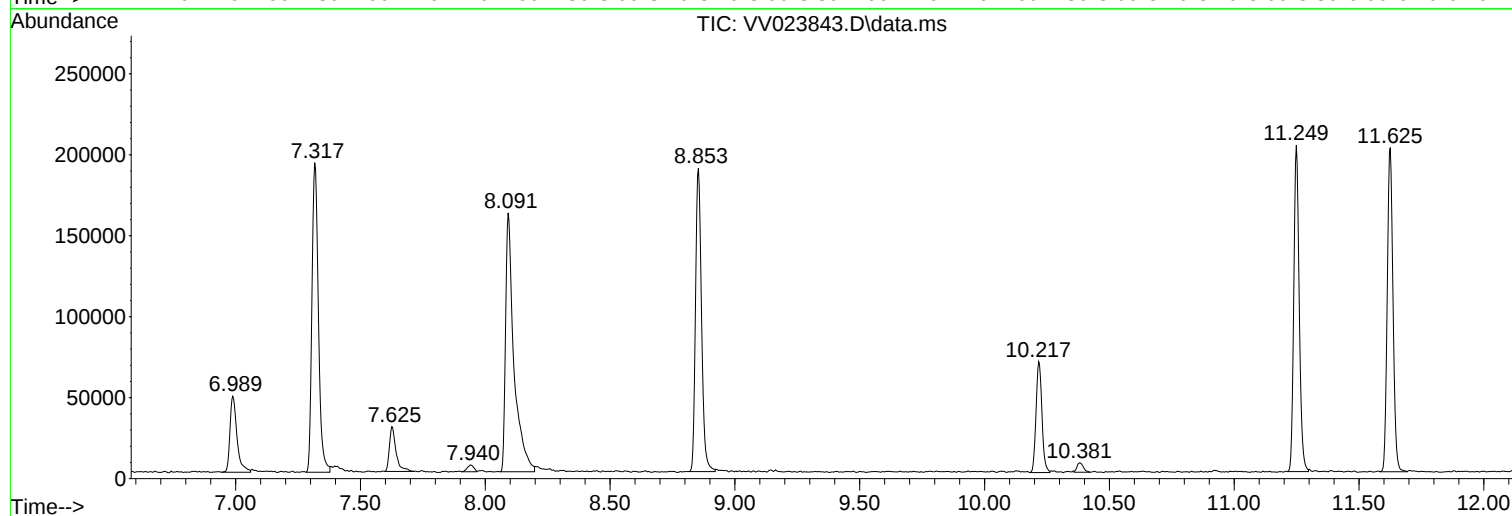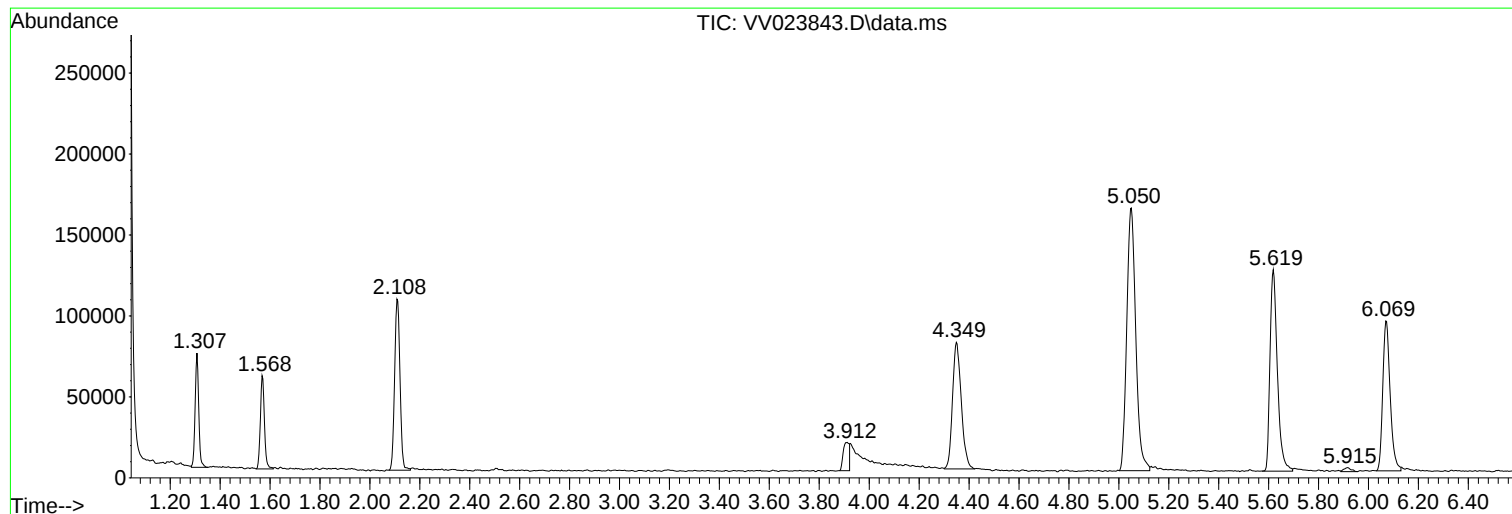

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120821\
Data File : VV023843.D
Acq On : 08 Dec 2021 17:44
Operator : SY/MD
Sample : M4889-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CP6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120821\
Data File : VV023843.D
Acq On : 08 Dec 2021 17:44
Operator : SY/MD
Sample : M4889-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CP6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc