

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120821\
 Data File : VV023845.D
 Acq On : 08 Dec 2021 18:32
 Operator : SY/MD
 Sample : M4889-21
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CQ2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023845.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.201	45	50	56	rBV	11047	10385	2.55%	0.307%
2	1.307	76	83	97	rVB	72594	73426	18.02%	2.173%
3	1.568	156	164	173	rBV	56796	64557	15.84%	1.911%
4	2.108	322	332	345	rBV	105068	153035	37.55%	4.530%
5	2.513	449	458	470	rVB6	2553	4636	1.14%	0.137%
6	3.912	882	893	925	rBV	17459	82912	20.35%	2.454%
7	4.349	1014	1029	1054	rVB	77480	191107	46.90%	5.656%
8	5.047	1231	1246	1274	rBV3	161440	407507	100.00%	12.061%
9	5.619	1413	1424	1448	rBV	124661	259399	63.66%	7.678%
10	6.069	1550	1564	1582	rBV2	90291	188958	46.37%	5.593%
11	6.989	1840	1850	1869	rBV	46459	88693	21.76%	2.625%
12	7.317	1941	1952	1970	rBV	191358	335529	82.34%	9.931%
13	7.629	2039	2049	2067	rBV2	26635	50602	12.42%	1.498%
14	7.940	2132	2146	2156	rBV3	5585	10288	2.52%	0.305%
15	8.092	2182	2193	2232	rBV	158763	383574	94.13%	11.353%
16	8.854	2419	2430	2451	rBV	193125	322599	79.16%	9.548%
17	10.217	2843	2854	2871	rBV2	68078	111338	27.32%	3.295%
18	10.381	2895	2905	2917	rVB4	6630	10643	2.61%	0.315%
19	11.249	3164	3175	3198	rBV	200230	310704	76.25%	9.196%
20	11.625	3280	3292	3308	rBV	197586	318700	78.21%	9.433%




Sum of corrected areas: 3378592

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120821\
Data File : VV023845.D
Acq On : 08 Dec 2021 18:32
Operator : SY/MD
Sample : M4889-21
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CQ2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

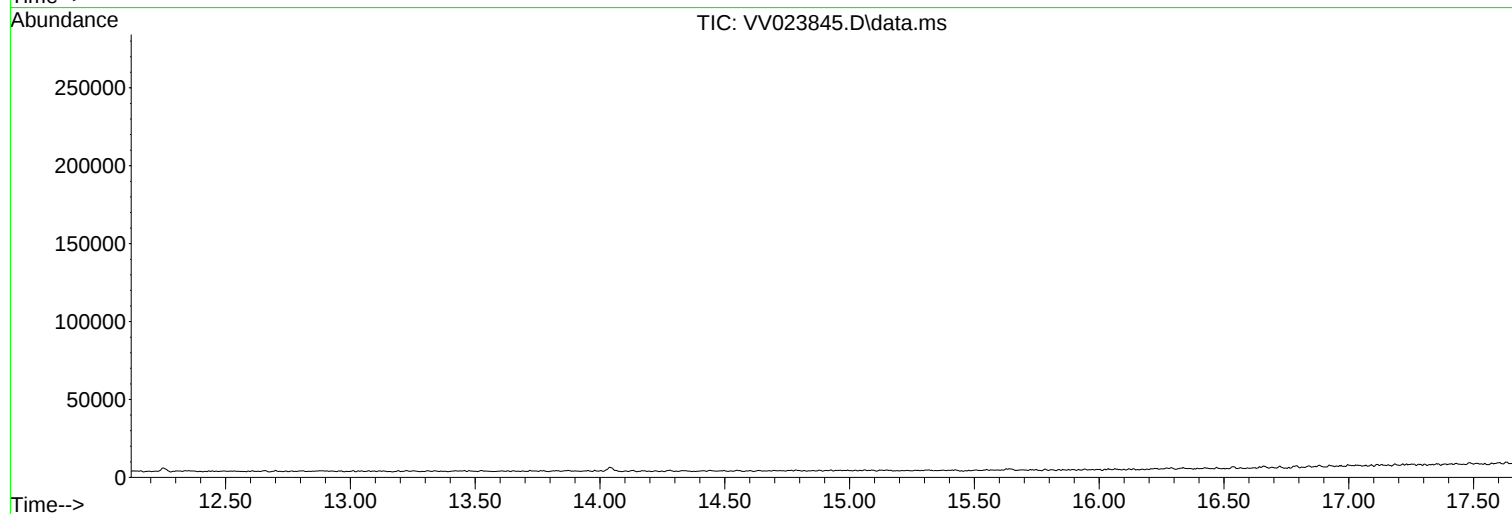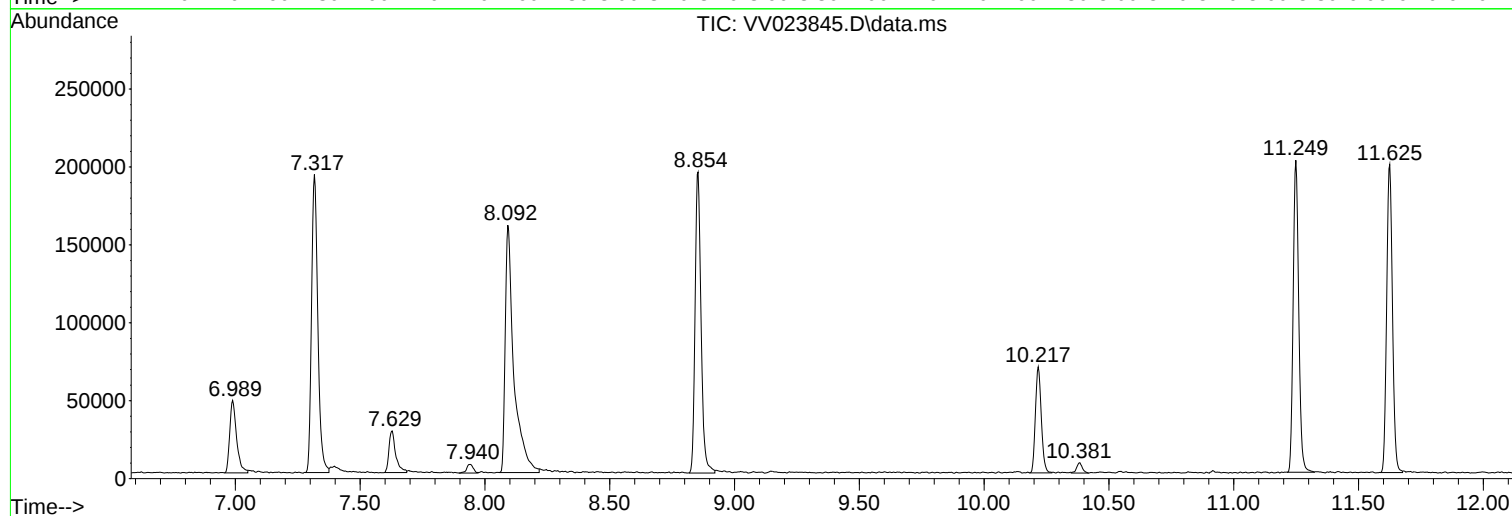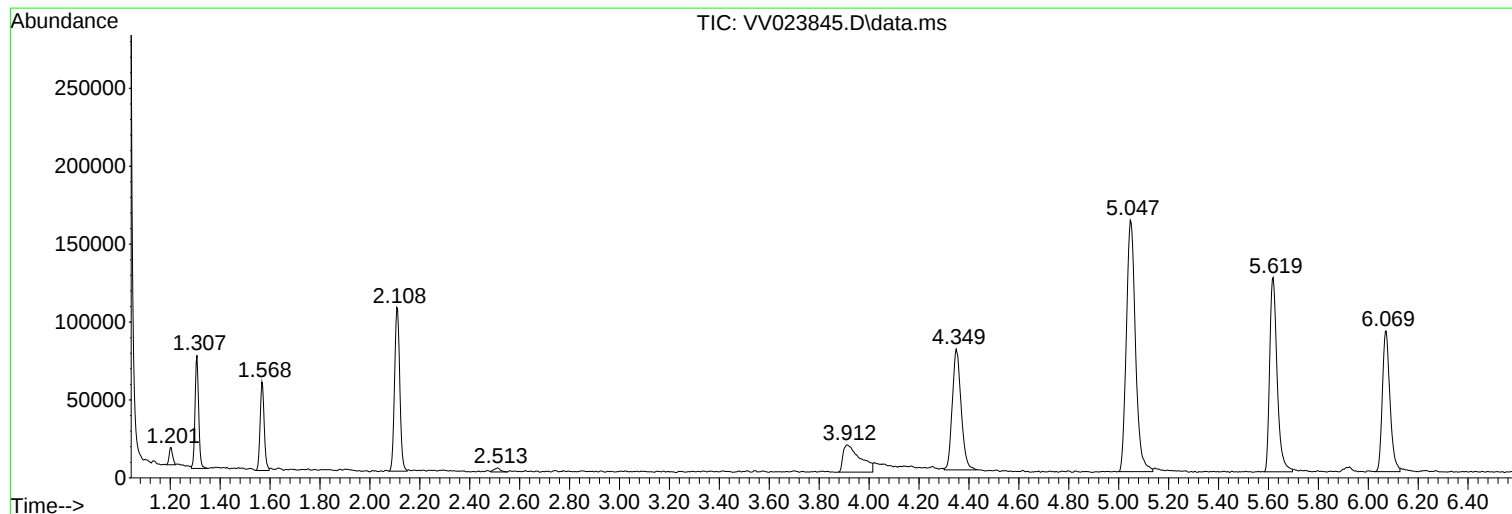

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120821\
Data File : VV023845.D
Acq On : 08 Dec 2021 18:32
Operator : SY/MD
Sample : M4889-21
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CQ2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120821\
Data File : VV023845.D
Acq On : 08 Dec 2021 18:32
Operator : SY/MD
Sample : M4889-21
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CQ2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc