

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120821\
 Data File : VV023846.D
 Acq On : 08 Dec 2021 18:56
 Operator : SY/MD
 Sample : M4889-22
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CQ5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV023846.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	93	rVB	65119	68749	16.84%	2.054%
2	1.568	154	164	174	rBV	55689	62733	15.37%	1.874%
3	2.108	322	332	343	rBV	105998	152721	37.41%	4.563%
4	3.921	881	896	922	rBV3	19482	91156	22.33%	2.723%
5	4.349	1012	1029	1056	rVB2	74515	198200	48.55%	5.922%
6	5.050	1228	1247	1266	rBV2	163405	408238	100.00%	12.197%
7	5.619	1410	1424	1447	rBV	119425	250308	61.31%	7.478%
8	6.069	1550	1564	1591	rBV	92675	197106	48.28%	5.889%
9	6.989	1839	1850	1868	rBV2	46749	89342	21.88%	2.669%
10	7.317	1940	1952	1969	rBV	188621	332603	81.47%	9.937%
11	7.394	1973	1976	1984	rVB6	2751	4116	1.01%	0.123%
12	7.625	2036	2048	2064	rBV2	27277	51949	12.73%	1.552%
13	7.937	2136	2145	2157	rBV2	5055	9849	2.41%	0.294%
14	8.092	2182	2193	2231	rBV	153542	377391	92.44%	11.275%
15	8.854	2418	2430	2461	rBV	184025	310906	76.16%	9.289%
16	10.214	2844	2853	2870	rBV	67318	110297	27.02%	3.295%
17	10.384	2896	2906	2914	rVB5	5961	9708	2.38%	0.290%
18	11.249	3164	3175	3198	rBV	190749	301227	73.79%	9.000%
19	11.625	3280	3292	3311	rBV	195654	316081	77.43%	9.444%
20	14.040	4034	4043	4050	rBV3	2502	4356	1.07%	0.130%




Sum of corrected areas: 3347036

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120821\
Data File : VV023846.D
Acq On : 08 Dec 2021 18:56
Operator : SY/MD
Sample : M4889-22
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CQ5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

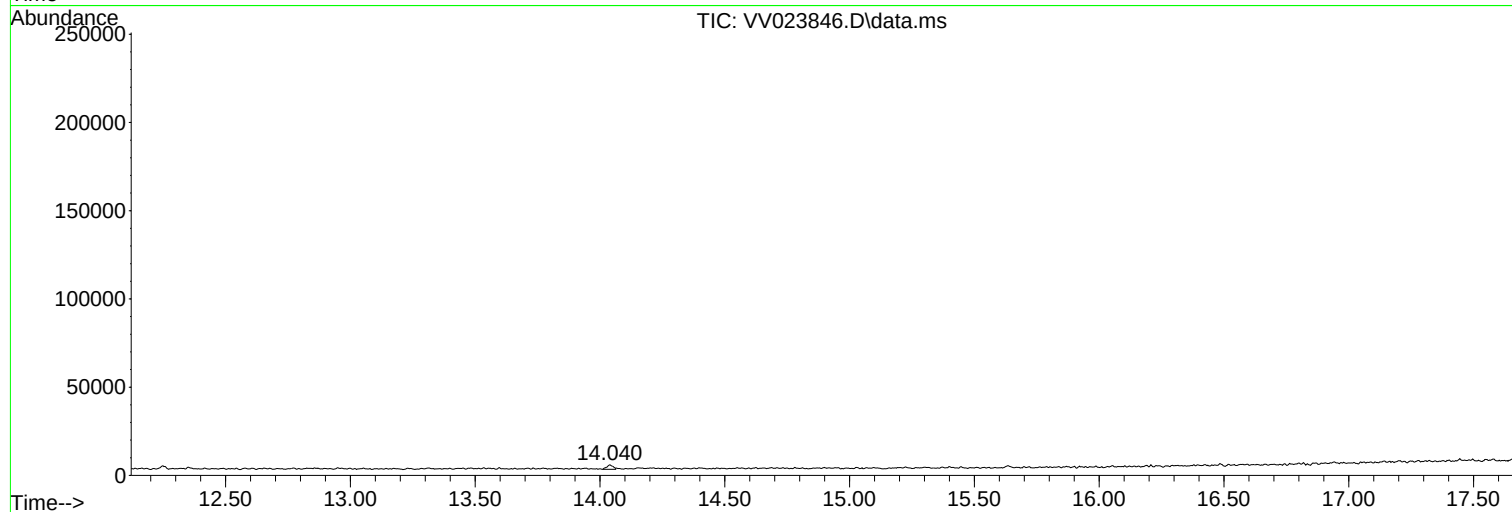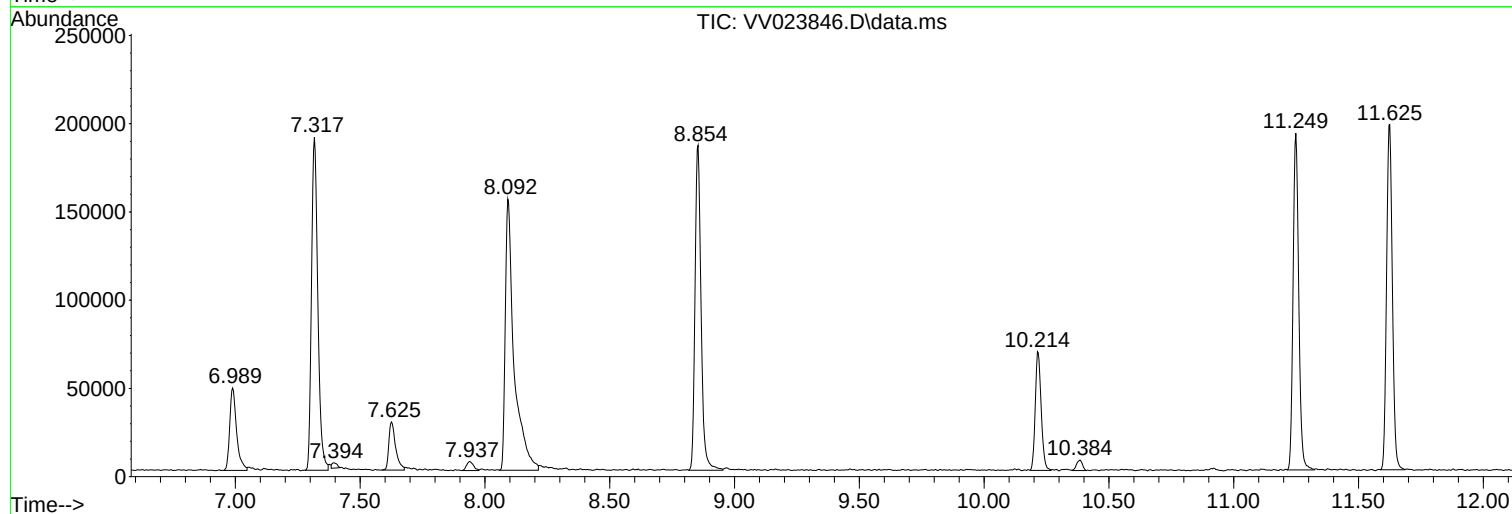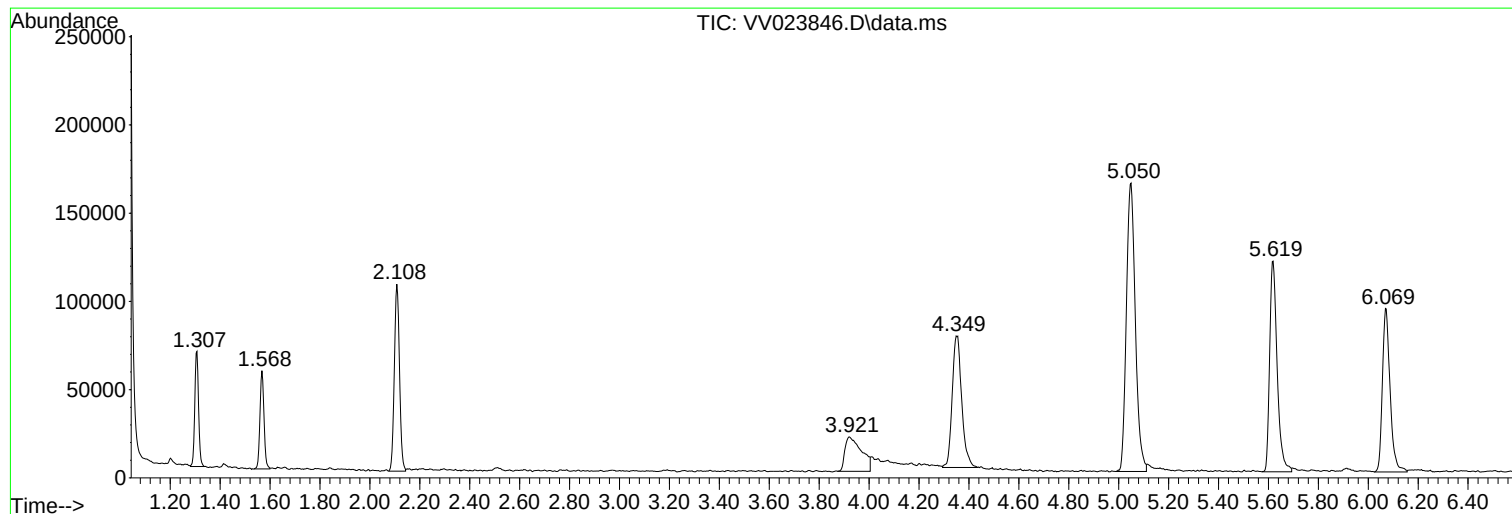

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120821\
Data File : VV023846.D
Acq On : 08 Dec 2021 18:56
Operator : SY/MD
Sample : M4889-22
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CQ5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120821\
Data File : VV023846.D
Acq On : 08 Dec 2021 18:56
Operator : SY/MD
Sample : M4889-22
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CQ5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc