

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120821\
 Data File : VV023847.D
 Acq On : 08 Dec 2021 19:20
 Operator : SY/MD
 Sample : M4889-23
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CQ8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV023847.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	92	rVB	66275	68509	16.75%	2.034%
2	1.568	155	164	174	rBV	53732	60716	14.85%	1.802%
3	2.108	322	332	350	rBV	105315	155283	37.97%	4.610%
4	3.915	882	894	916	rBV2	19051	74176	18.14%	2.202%
5	4.346	1014	1028	1051	rBV	76221	198042	48.43%	5.879%
6	4.831	1165	1179	1195	rVB4	12986	30851	7.54%	0.916%
7	5.050	1227	1247	1269	rBV2	161695	408930	100.00%	12.139%
8	5.619	1412	1424	1444	rBV	124049	250512	61.26%	7.437%
9	6.072	1552	1565	1587	rBV2	91075	190389	46.56%	5.652%
10	6.989	1840	1850	1868	rBV2	46488	87190	21.32%	2.588%
11	7.317	1939	1952	1972	rBV	192559	338585	82.80%	10.051%
12	7.397	1972	1977	1989	rVB6	3558	6948	1.70%	0.206%
13	7.625	2040	2048	2062	rBV2	27962	50375	12.32%	1.495%
14	7.940	2133	2146	2155	rBV3	5315	9756	2.39%	0.290%
15	8.091	2180	2193	2240	rBV	154302	378690	92.61%	11.242%
16	8.853	2418	2430	2445	rBV	190771	314844	76.99%	9.346%
17	10.217	2841	2854	2872	rBV	67406	111721	27.32%	3.317%
18	10.384	2894	2906	2914	rBV3	8040	11605	2.84%	0.345%
19	11.249	3161	3175	3192	rBV	197485	306167	74.87%	9.089%
20	11.625	3280	3292	3311	rBV	198516	315312	77.11%	9.360%




Sum of corrected areas: 3368601

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120821\
Data File : VV023847.D
Acq On : 08 Dec 2021 19:20
Operator : SY/MD
Sample : M4889-23
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CQ8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

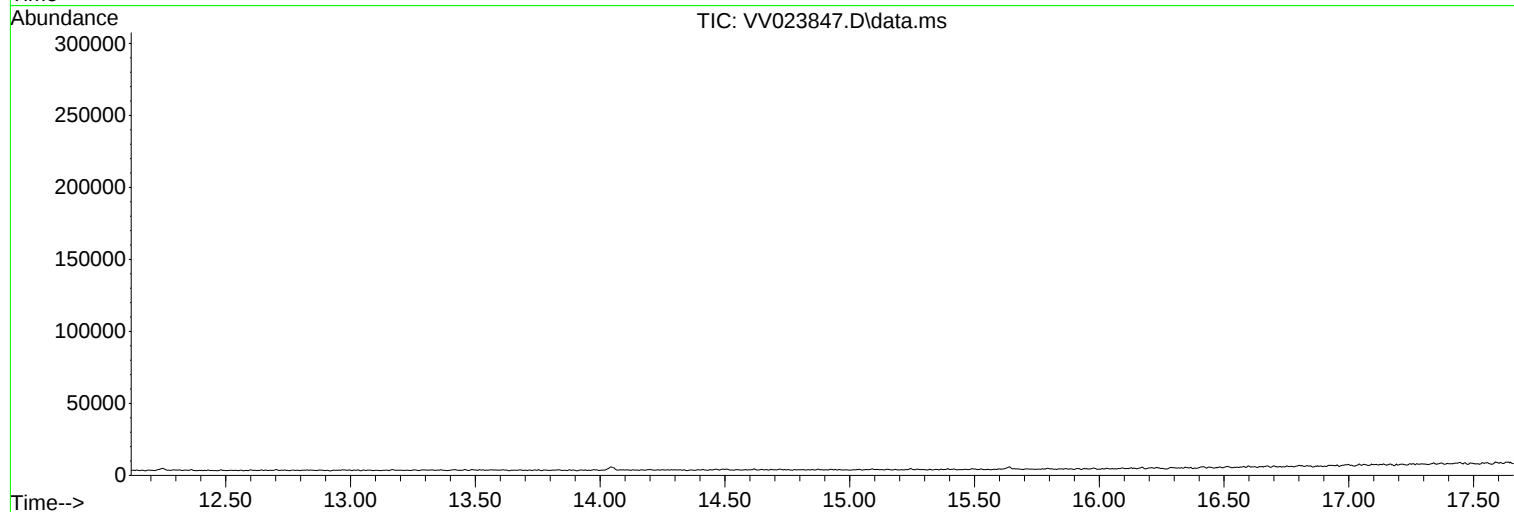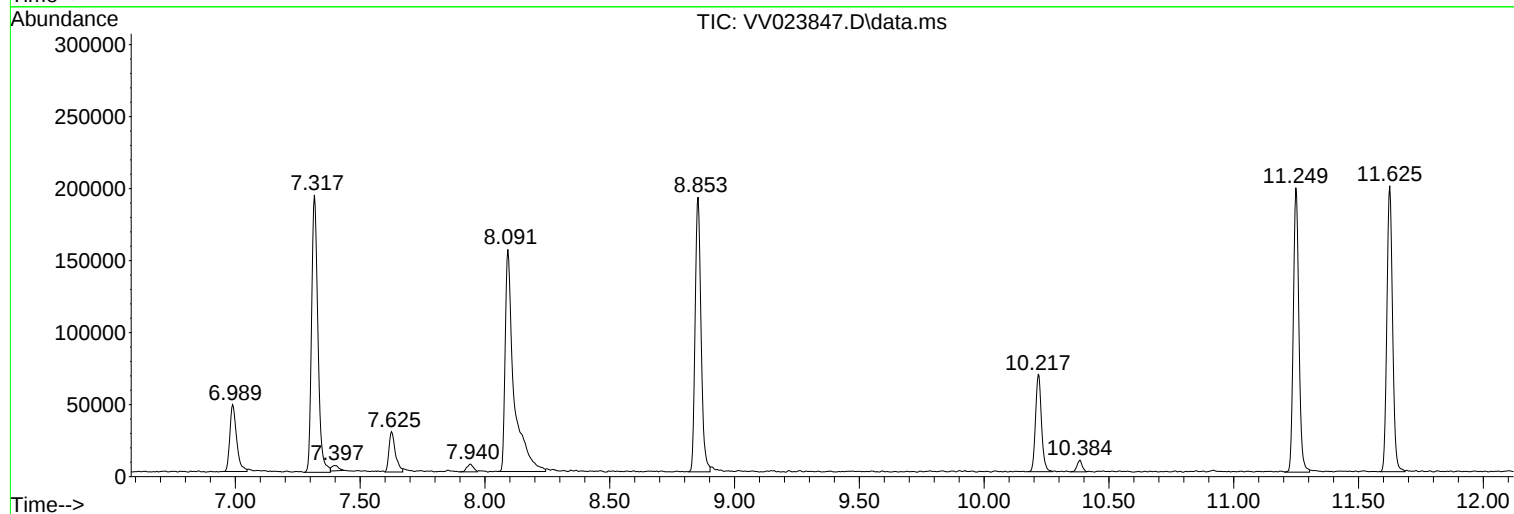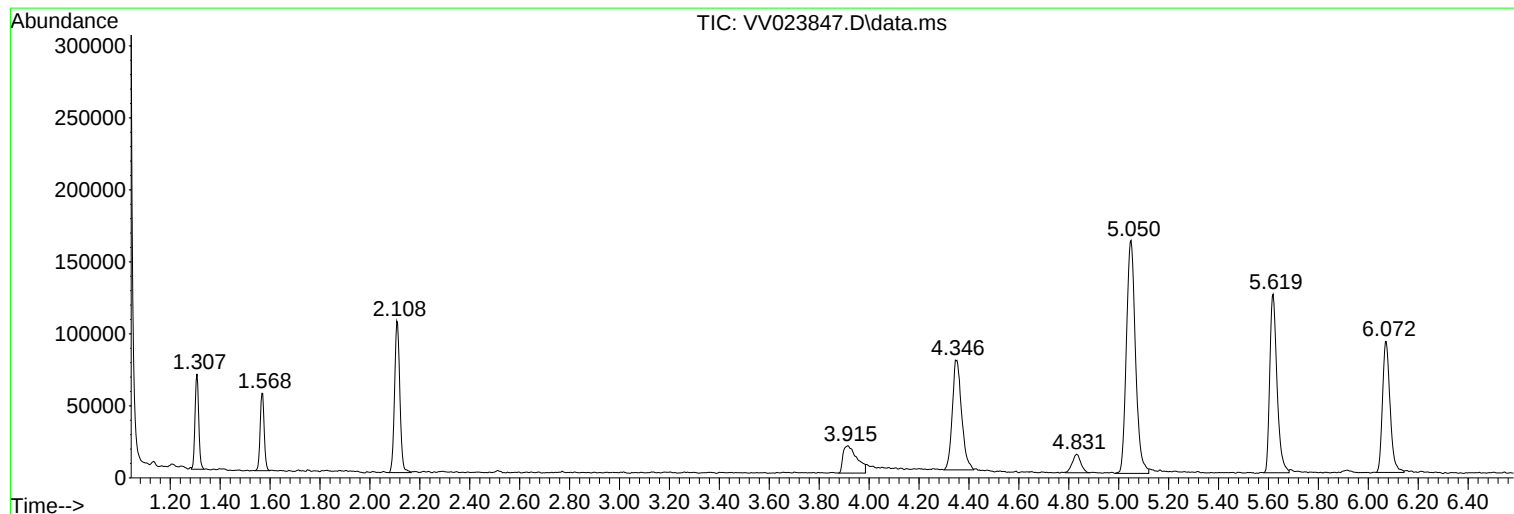

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120821\
Data File : VV023847.D
Acq On : 08 Dec 2021 19:20
Operator : SY/MD
Sample : M4889-23
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CQ8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120821\
Data File : VV023847.D
Acq On : 08 Dec 2021 19:20
Operator : SY/MD
Sample : M4889-23
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CQ8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
