
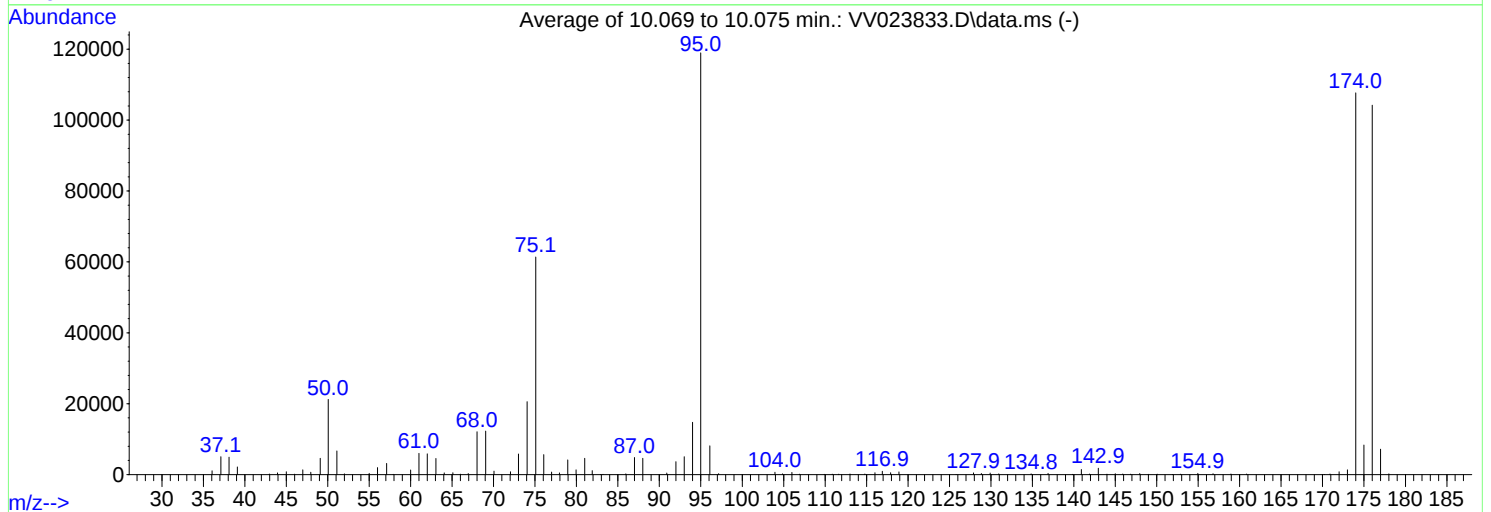


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120821\
 Data File : VV023833.D
 Acq On : 08 Dec 2021 09:29
 Operator : SY/MD
 Sample : BFB247
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB247

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Thu Dec 02 02:08:23 2021

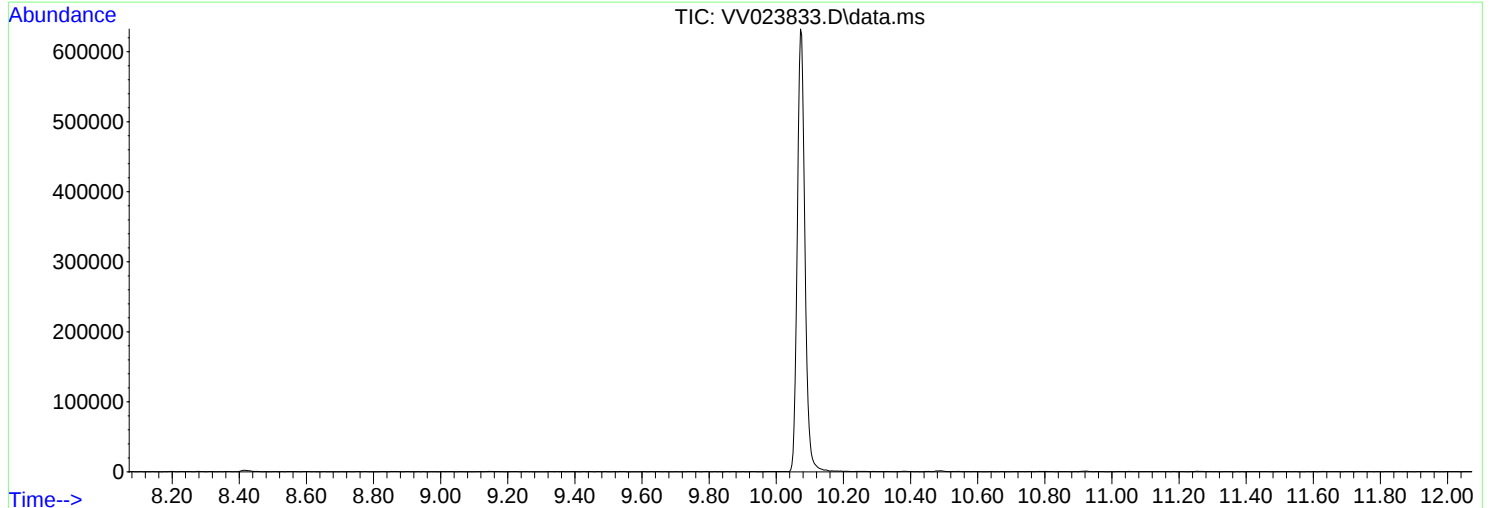

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	21208	PASS
75	95	30	80	51.6	61376	PASS
95	95	100	100	100.0	118968	PASS
96	95	5	9	6.8	8114	PASS
173	174	0.00	2	1.3	1371	PASS
174	95	50	120	90.5	107659	PASS
175	174	5	9	7.7	8342	PASS
176	174	95	105	96.8	104219	PASS
177	176	5	10	6.9	7198	PASS

m/z	Abundance
39.90	174.0
43.90	211.0

Instrument :
MSVOA_V
ClientSampleId :
BFB247

m/z	Abundance
36.10	1030.0
37.10	4803.0
38.10	4808.0
39.10	2115.0
39.90	165.0
43.00	199.0
44.00	685.0
45.00	811.0
46.00	124.0
47.00	1421.0
47.90	690.0
49.10	4509.0
50.10	20336.0
51.10	6472.0
52.00	251.0
55.00	331.0
56.00	1835.0
57.10	3228.0
57.90	163.0
60.00	1215.0
61.00	5918.0
62.00	5889.0
63.00	4372.0
64.00	473.0
65.10	506.0
66.00	125.0
67.00	347.0
68.00	12134.0
69.00	11979.0
70.00	955.0
72.10	800.0
73.00	5524.0
74.10	19952.0
75.10	58200.0
76.00	5384.0
77.00	751.0
78.00	422.0
79.00	3902.0
80.00	1191.0
81.00	4456.0
81.90	1124.0
82.90	127.0
85.90	224.0
87.00	4630.0
88.00	4239.0
90.90	445.0
92.00	3549.0
93.00	4916.0
94.00	14065.0
95.00	112976.0
96.10	7621.0
97.10	298.0
104.00	711.0
104.90	173.0
106.00	595.0
106.90	111.0
110.80	168.0
111.80	132.0
113.00	199.0
114.80	152.0
116.00	525.0
116.90	875.0
117.90	552.0
118.90	810.0
127.90	444.0
128.90	279.0
129.90	424.0
131.00	249.0
134.90	211.0
136.90	296.0
140.00	113.0
140.90	1367.0
141.90	169.0
142.90	1692.0
143.90	166.0
145.00	263.0
145.90	161.0
146.80	120.0
148.00	274.0
150.00	148.0
151.90	101.0
152.90	141.0
154.90	369.0
156.80	273.0
158.90	181.0
160.90	189.0
170.20	100.0
170.80	192.0
172.00	837.0
173.00	1299.0
174.00	99728.0
175.00	7645.0

Instrument :
MSVOA_V
ClientSampleId :
BFB247

176.00	96032.0
177.00	6775.0
178.00	205.0

Instrument :
MSVOA_V
ClientSampleId :
BFB247

m/z	Abundance
36.00	1154.0
37.10	5368.0
38.10	5158.0
39.10	2251.0
39.90	140.0
42.90	168.0
44.00	738.0
45.00	839.0
46.00	146.0
47.00	1380.0
47.90	728.0
49.10	4731.0
50.10	22008.0
51.10	6876.0
52.00	229.0
55.00	364.0
56.00	2058.0
57.10	3261.0
57.90	161.0
60.00	1336.0
61.00	6197.0
62.00	6057.0
63.00	4770.0
64.10	488.0
65.10	593.0
66.00	136.0
66.90	320.0
68.00	12519.0
69.00	12571.0
70.00	1017.0
72.00	845.0
73.00	6091.0
74.00	21352.0
75.10	63560.0
76.10	5901.0
77.00	753.0
77.90	516.0
78.90	4285.0
79.90	1389.0
81.00	4790.0
81.90	1140.0
83.20	115.0
86.00	220.0
87.00	5020.0
88.00	4706.0
90.90	447.0
92.00	3777.0
93.00	5263.0
94.00	15325.0
95.00	123000.0
96.10	8329.0
97.20	288.0
103.90	689.0
104.80	233.0
106.00	691.0
106.90	138.0
109.90	124.0
110.90	158.0
111.60	122.0
113.00	200.0
114.80	196.0
116.00	561.0
116.90	986.0
117.90	553.0
118.90	777.0
127.90	549.0
128.80	338.0
129.90	474.0
130.90	241.0
134.80	227.0
136.90	352.0
139.80	107.0
140.90	1469.0
141.90	201.0
142.90	1929.0
144.00	111.0
145.00	249.0
145.90	180.0
146.80	131.0
148.00	313.0
149.00	124.0
150.00	159.0
152.80	147.0
154.90	388.0
156.80	301.0
159.00	172.0
160.80	192.0
170.20	100.0
170.90	187.0
172.00	852.0
173.00	1370.0
174.00	111128.0

Instrument :
MSVOA_V
ClientSampleId :
BFB247

175.00	8738.0
176.00	107720.0
177.00	7515.0
178.00	204.0

Instrument :
MSVOA_V
ClientSampleId :
BFB247

m/z	Abundance
36.00	1121.0
37.10	5056.0
38.10	4782.0
39.10	2134.0
39.80	120.0
42.90	123.0
44.00	778.0
45.00	835.0
46.00	156.0
47.00	1238.0
48.00	692.0
49.10	4541.0
50.00	21280.0
51.10	6637.0
52.00	226.0
55.00	360.0
56.00	2086.0
57.10	3045.0
60.00	1332.0
61.00	5919.0
62.00	5662.0
63.10	4572.0
64.10	510.0
65.10	578.0
66.00	118.0
66.90	323.0
68.00	11669.0
69.10	12295.0
70.10	961.0
72.00	819.0
73.00	5868.0
74.00	20496.0
75.10	62368.0
76.10	5705.0
77.00	647.0
77.90	527.0
78.90	4223.0
79.90	1485.0
81.00	4556.0
81.90	1066.0
83.20	105.0
86.00	190.0
87.00	4795.0
88.00	4842.0
90.90	469.0
92.00	3612.0
93.00	4990.0
94.00	14870.0
95.00	120928.0
96.10	8392.0
97.20	213.0
103.90	653.0
104.80	287.0
106.00	674.0
106.90	158.0
109.90	133.0
110.90	127.0
111.50	106.0
113.00	172.0
114.80	233.0
116.00	533.0
116.90	1000.0
117.90	544.0
118.90	694.0
125.80	106.0
127.90	560.0
128.80	336.0
129.90	479.0
130.90	213.0
134.80	259.0
136.90	381.0
139.70	111.0
140.90	1533.0
141.90	193.0
143.00	1855.0
144.10	116.0
145.00	244.0
145.90	196.0
146.90	129.0
147.90	311.0
149.00	110.0
150.10	149.0
152.80	132.0
155.00	379.0
156.80	295.0
159.00	184.0
160.80	165.0
171.00	156.0
172.00	795.0
173.00	1445.0
174.00	112120.0
175.00	8644.0

Instrument :
MSVOA_V
ClientSampleId :
BFB247

176.00	108904.0
177.00	7303.0
178.00	228.0

Instrument :
MSVOA_V
ClientSampleId :
BFB247