




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
 Data File : VV029488.D
 Acq On : 08 Dec 2022 21:19
 Operator : SY/MD
 Sample : N5929-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ96

Manual IntegrationsAPPROVED

Quant Time: Dec 09 05:26:09 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Dec 08 01:48:46 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 12/09/2022
 Supervised By :Mahesh Dadoda 12/09/2022

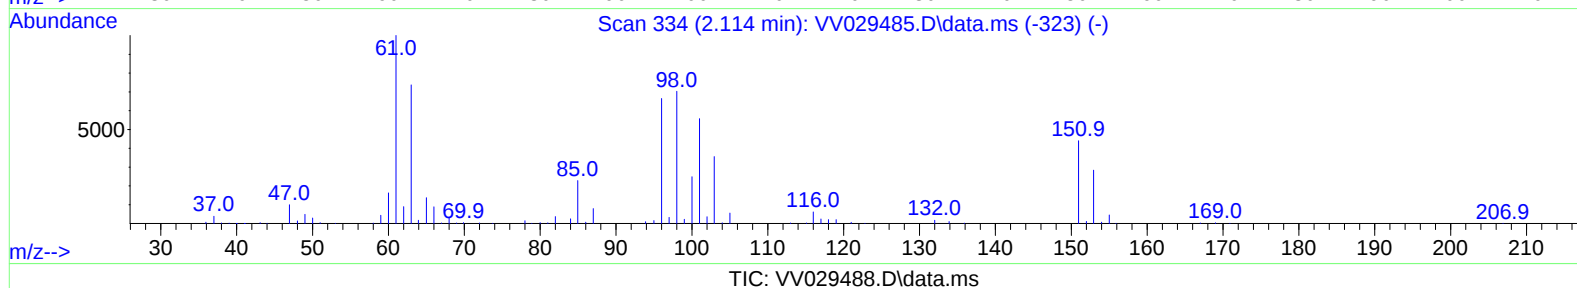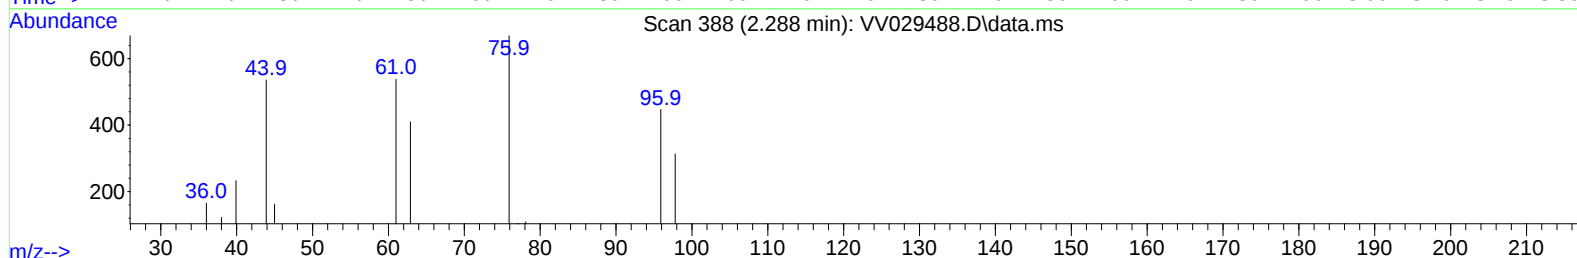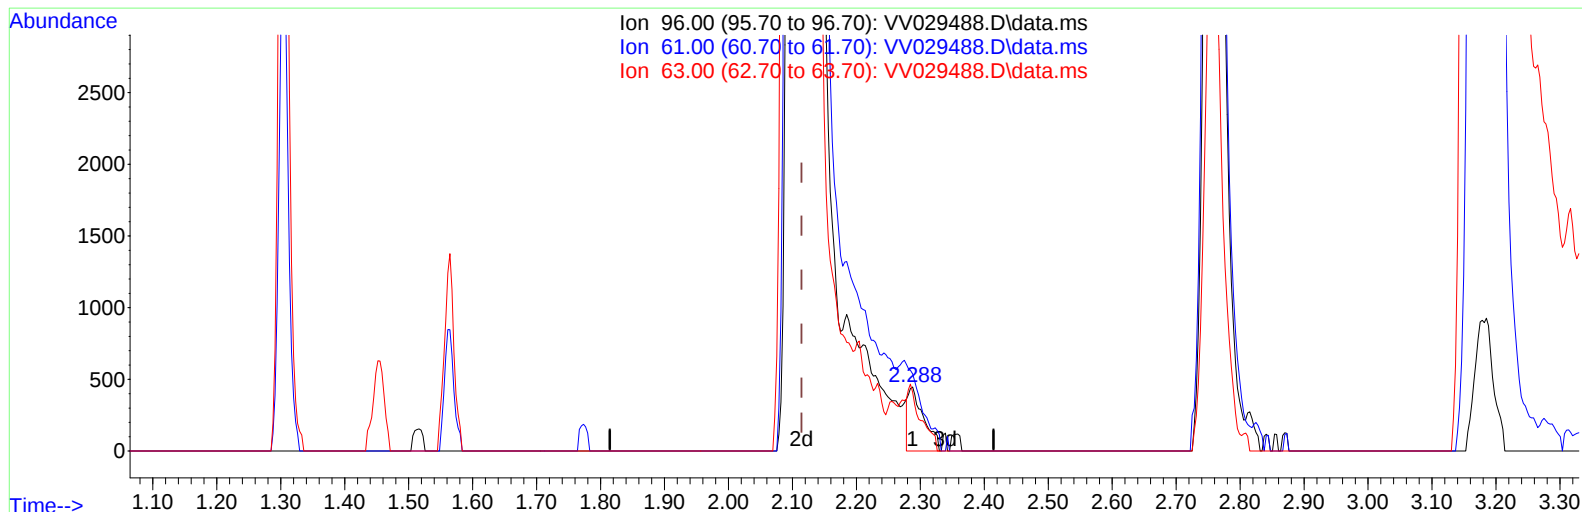

TIC: VV029488.D\data.ms

(12) 1,1-Dichloroethene (T)

2.288min (+ 0.173) 0.28 ug/L

response 748

Ion	Exp%	Act%
96.00	100.00	100.00
61.00	147.60	120.36
63.00	110.50	91.72
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
 Data File : VV029488.D
 Acq On : 08 Dec 2022 21:19
 Operator : SY/MD
 Sample : N5929-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ96

Manual IntegrationsAPPROVED

Quant Time: Dec 09 05:26:09 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Dec 08 01:48:46 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 12/09/2022
 Supervised By :Mahesh Dadoda 12/09/2022

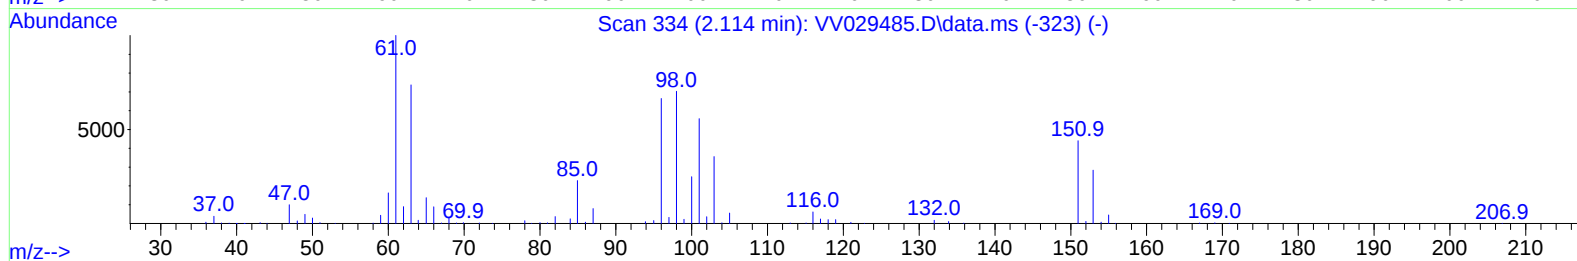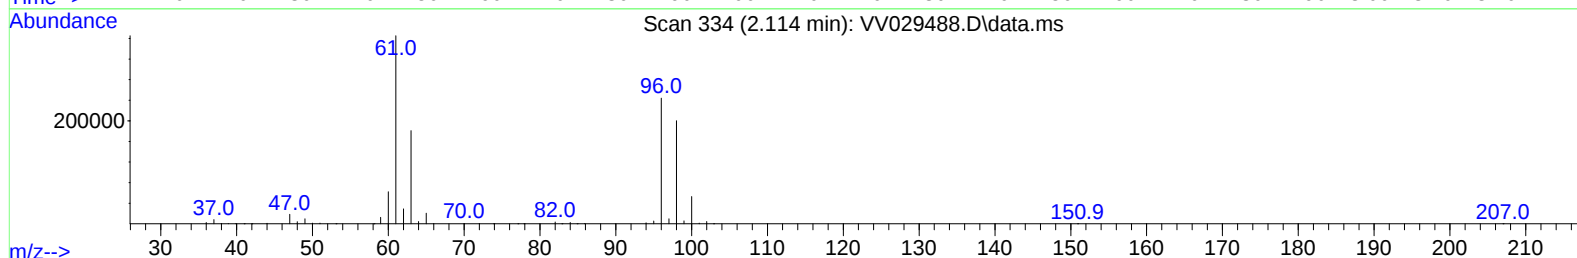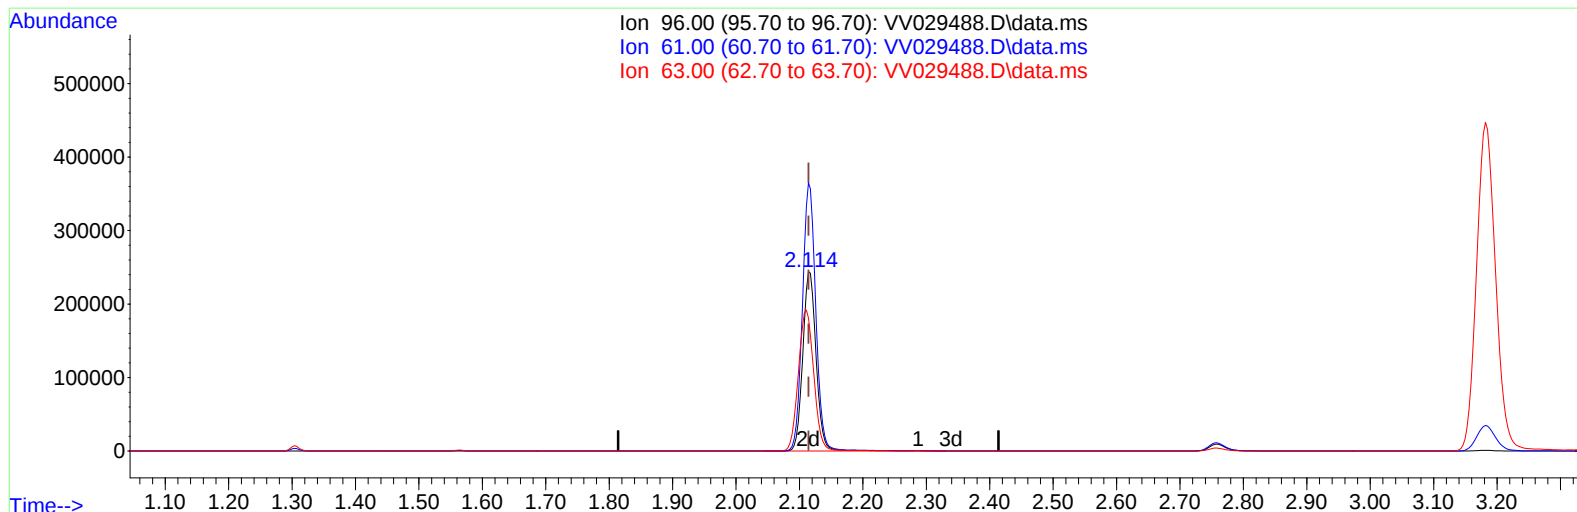

TIC: VV029488.D\data.ms

(12) 1,1-Dichloroethene (T)

2.114min (-0.000) 131.98 ug/L m

response 358248

Ion	Exp%	Act%
96.00	100.00	100.00
61.00	147.60	149.63
63.00	110.50	74.15#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120822\
 Data File : VW029488.D
 Acq On : 08 Dec 2022 21:19
 Operator : SY/MD
 Sample : N5929-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ96

Manual IntegrationsAPPROVED

Quant Time: Dec 09 05:26:09 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Dec 08 01:48:46 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 12/09/2022
 Supervised By :Mahesh Dadoda 12/09/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	507830	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.844	117	468791	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.239	152	235796	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	106851	34.360	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	68.720%		
7) Chloroethane-d5	1.564	69	101224	42.688	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	85.380%		
11) 1,1-Dichloroethene-d2	2.111	63	323767	66.751	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	133.500%#		
21) 2-Butanone-d5	3.866	46	203742	107.401	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	107.400%		
24) Chloroform-d	4.339	84	268096	45.813	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	91.620%		
26) 1,2-Dichloroethane-d4	5.024	65	160709	48.084	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	96.160%		
32) Benzene-d6	5.043	84	555803	44.870	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	89.740%		
36) 1,2-Dichloropropane-d6	6.063	67	177244	46.844	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	93.680%		
41) Toluene-d8	7.307	98	502929	43.091	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	86.180%		
43) trans-1,3-Dichloroprop...	7.612	79	83521	43.714	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	87.420%		
47) 2-Hexanone-d5	8.082	63	168575	104.335	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	104.330%		
56) 1,1,2,2-Tetrachloroeth...	10.207	84	260382	48.158	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	96.320%		
66) 1,2-Dichlorobenzene-d4	11.612	152	208204	46.385	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	92.760%		
Target Compounds						Qvalue
9) Trichlorofluoromethane	1.751	101	11618	2.432	ug/L	97
12) 1,1-Dichloroethene	2.114	96	358248m	131.977	ug/L	
17) trans-1,2-Dichloroethene	2.757	96	16996	5.434	ug/L	97
19) 1,1-Dichloroethane	3.182	63	934134	174.338	ug/L	99
20) cis-1,2-Dichloroethene	3.902	96	278821	81.070	ug/L	95
25) Chloroform	4.368	83	17346	3.123	ug/L	92
30) 1,1,1-Trichloroethane	4.600	97	2232817	437.168	ug/L	99
34) Trichloroethene	5.908	95	206756	62.441	ug/L	98
45) 1,1,2-Trichloroethane	7.834	97	7819	2.373	ug/L	93
46) Tetrachloroethene	7.966	164	247550	92.988	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Manual IntegrationsAPPROVED

Quant Time: Dec 09 05:26:09 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Dec 08 01:48:46 2022
Response via : Initial Calibration

