

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120822\
 Data File : VW029477.D
 Acq On : 08 Dec 2022 17:00
 Operator : SY/MD
 Sample : VIBLK306
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK306

Quant Time: Dec 09 02:01:23 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Dec 08 01:48:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	510696	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.844	117	466246	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.239	152	244744	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	115394	36.899	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	73.800%		
7) Chloroethane-d5	1.564	69	105961	44.435	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	88.860%		
11) 1,1-Dichloroethene-d2	2.105	63	162913	33.399	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	66.800%		
21) 2-Butanone-d5	3.870	46	210512	110.347	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	110.350%		
24) Chloroform-d	4.339	84	276754	47.027	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	94.060%		
26) 1,2-Dichloroethane-d4	5.024	65	170457	50.715	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	101.420%		
32) Benzene-d6	5.043	84	590248	47.910	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	95.820%		
36) 1,2-Dichloropropane-d6	6.063	67	184663	49.072	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	98.140%		
41) Toluene-d8	7.310	98	533103	45.925	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	91.860%		
43) trans-1,3-Dichloroprop...	7.612	79	87206	45.892	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	91.780%		
47) 2-Hexanone-d5	8.082	63	177074	110.193	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	110.190%		
56) 1,1,2,2-Tetrachloroeth...	10.207	84	272377	50.651	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	101.300%		
66) 1,2-Dichlorobenzene-d4	11.612	152	230125	49.394	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	98.780%		
Target Compounds						Qvalue
34) Trichloroethene	5.918	95	3649	1.108	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
Data File : VV029477.D
Acq On : 08 Dec 2022 17:00
Operator : SY/MD
Sample : VIBLK306
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK306

Quant Time: Dec 09 02:01:23 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Dec 08 01:48:46 2022
Response via : Initial Calibration

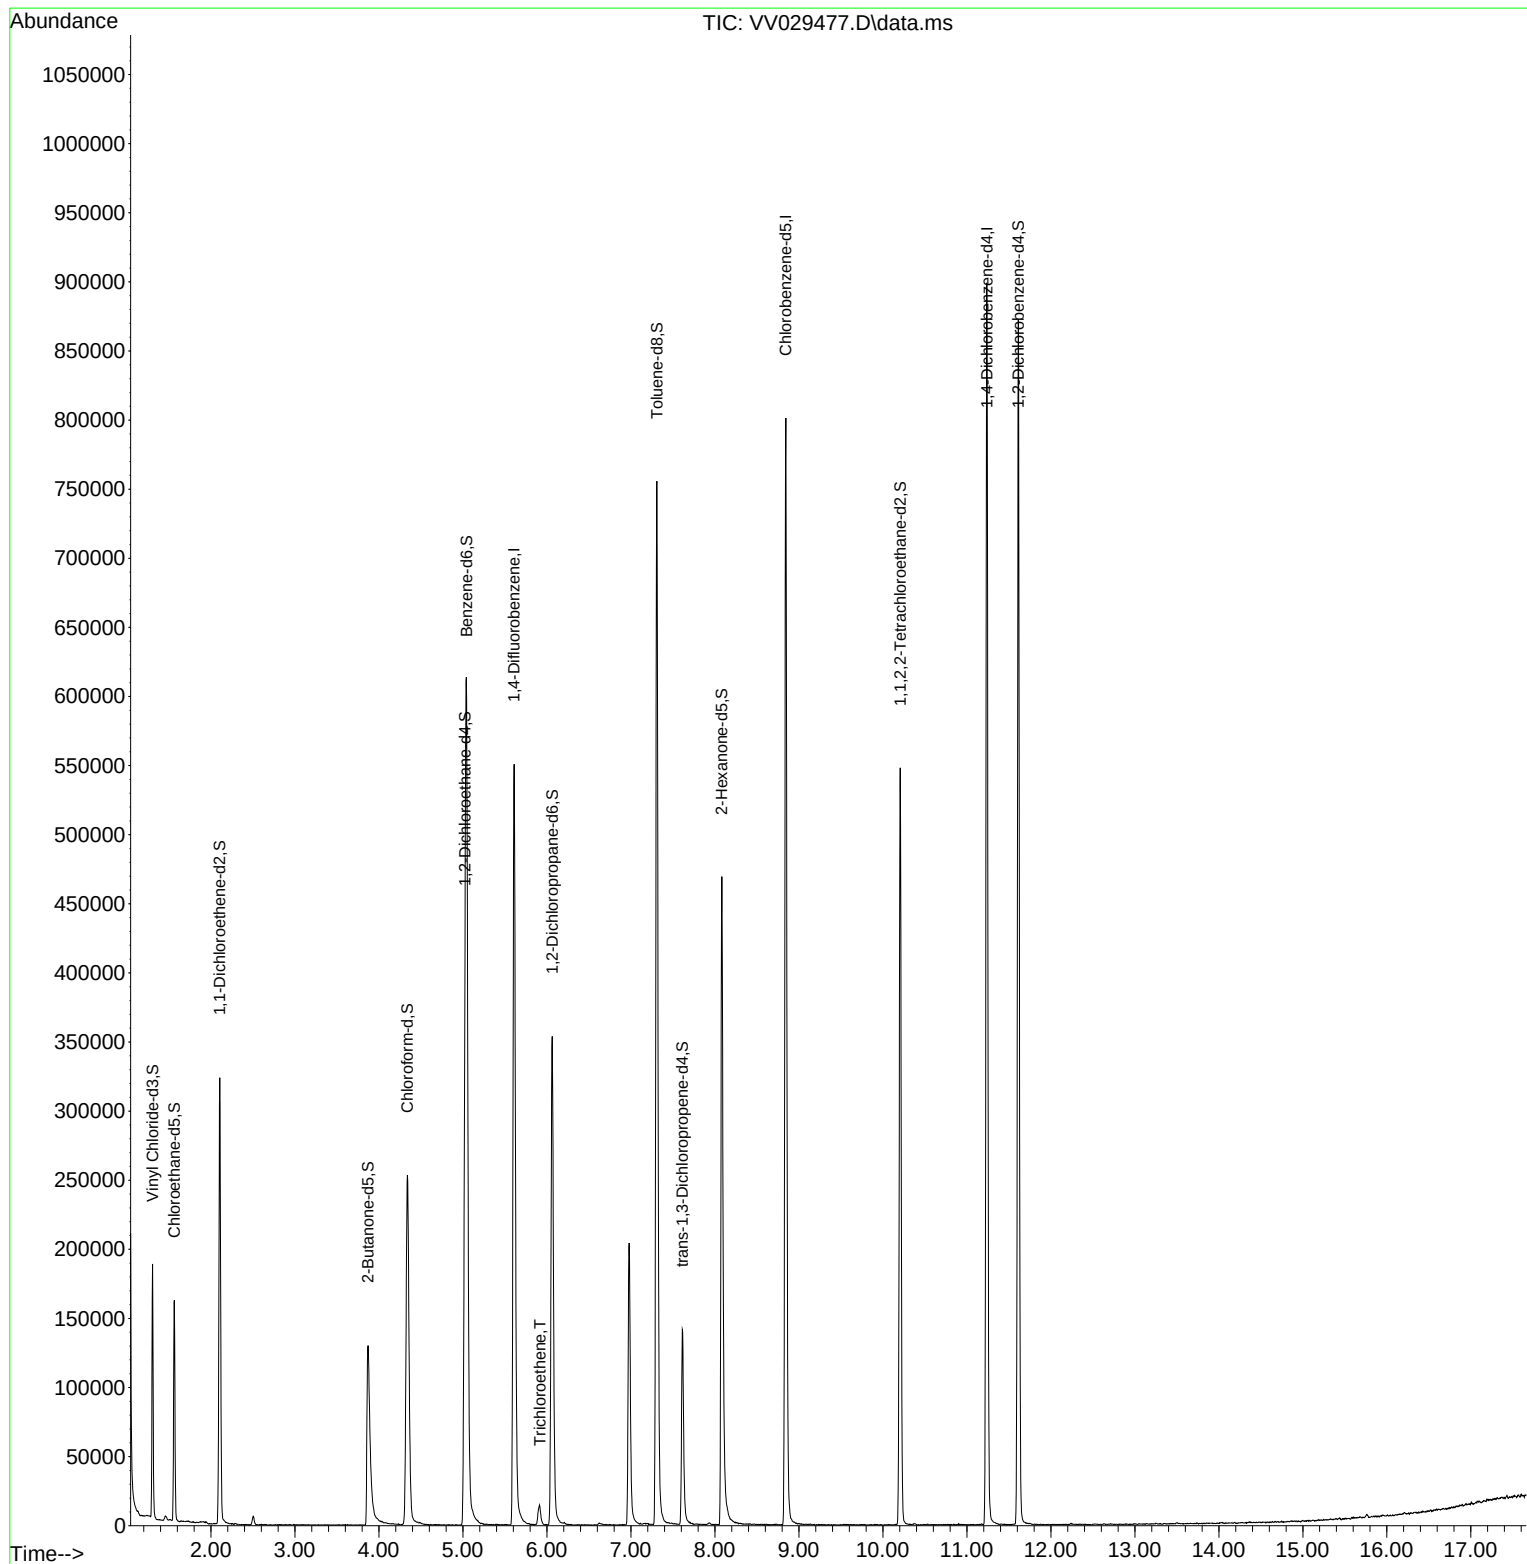

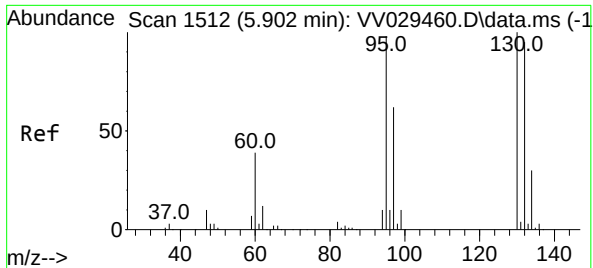

#34
 Trichloroethene
 Concen: 1.108 ug/L
 RT: 5.918 min Scan# 11
 Delta R.T. 0.010 min
 Lab File: VV029477.D
 Acq: 08 Dec 2022 17:00

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK306

Tgt Ion: 95 Resp: 3649

Ion	Ratio	Lower	Upper
95	100		
97	56.9	44.0	81.8
132	98.2	69.9	129.9
130	112.9	73.7	136.9

