

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
 Data File : VV029463.D
 Acq On : 08 Dec 2022 11:31
 Operator : SY/MD
 Sample : VV1208WBL04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK299

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M

Title : VOC Analysis

Signal : TIC: VV029463.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	95	rVB	213430	211739	12.83%	1.585%
2	1.561	155	162	175	rVB	171467	194829	11.80%	1.458%
3	2.105	320	331	352	rBV	341878	491550	29.78%	3.679%
4	2.500	447	454	464	rVB2	3674	5825	0.35%	0.044%
5	2.584	478	480	482	rBV	252	109	0.01%	0.001%
6	2.709	516	519	520	rBV	160	75	0.00%	0.001%
7	2.719	520	522	523	rVV	156	50	0.00%	0.000%
8	2.789	542	544	548	rVB	214	105	0.01%	0.001%
9	2.828	553	556	557	rBV	183	117	0.01%	0.001%
10	2.867	565	568	571	rBV2	234	176	0.01%	0.001%
11	3.053	621	626	629	rBV	304	320	0.02%	0.002%
12	3.246	683	686	688	rBV2	244	144	0.01%	0.001%
13	3.259	688	690	692	rBV2	260	95	0.01%	0.001%
14	3.349	714	718	719	rBV	207	163	0.01%	0.001%
15	3.375	724	726	727	rBV	237	81	0.00%	0.001%
16	3.442	744	747	748	rBV	166	73	0.00%	0.001%
17	3.516	767	770	772	rBV2	237	121	0.01%	0.001%
18	3.719	831	833	836	rBV	223	118	0.01%	0.001%
19	3.741	836	840	848	rVB2	300	343	0.02%	0.003%
20	3.802	856	859	861	rBV2	107	60	0.00%	0.000%
21	3.822	863	865	868	rBV2	246	153	0.01%	0.001%
22	3.867	869	879	916	rBV	137572	390045	23.63%	2.919%
23	4.339	1010	1026	1048	rBV	254750	630203	38.18%	4.717%
24	4.555	1091	1093	1095	rBV	285	81	0.00%	0.001%
25	4.760	1154	1157	1161	rVB3	480	337	0.02%	0.003%
26	4.799	1166	1169	1171	rBV	127	75	0.00%	0.001%
27	4.828	1177	1178	1180	rVB	136	33	0.00%	0.000%
28	4.844	1180	1183	1184	rBV	149	81	0.00%	0.001%
29	4.895	1197	1199	1203	rBV	199	128	0.01%	0.001%
30	5.040	1225	1244	1277	rBV2	629044	1650712	100.00%	12.355%
31	5.387	1350	1352	1355	rBV3	393	249	0.02%	0.002%
32	5.465	1370	1376	1380	rBV4	482	604	0.04%	0.005%
33	5.516	1389	1392	1395	rVB2	433	313	0.02%	0.002%
34	5.555	1401	1404	1407	rVB2	349	202	0.01%	0.002%
35	5.609	1407	1421	1464	rBV	567297	1163399	70.48%	8.708%
36	5.902	1502	1512	1525	rVB5	5694	11360	0.69%	0.085%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
 Data File : VV029463.D
 Acq On : 08 Dec 2022 11:31
 Operator : SY/MD
 Sample : VV1208WBL04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK299

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	5.998	1540	1542	1546	rBV2	273	210	0.01%	0.002%
38	6.063	1548	1562	1585	rBV	354075	736196	44.60%	5.510%
39	6.301	1634	1636	1640	rVB2	292	199	0.01%	0.001%
40	6.330	1642	1645	1648	rBV2	229	186	0.01%	0.001%
41	6.362	1651	1655	1656	rBV2	378	239	0.01%	0.002%
42	6.394	1664	1665	1666	rBV2	243	63	0.00%	0.000%
43	6.403	1666	1668	1674	rVB3	303	266	0.02%	0.002%
44	6.455	1681	1684	1685	rBV	230	133	0.01%	0.001%
45	6.490	1690	1695	1700	rVV2	326	320	0.02%	0.002%
46	6.513	1700	1702	1706	rVB	249	129	0.01%	0.001%
47	6.561	1713	1717	1722	rBV	367	361	0.02%	0.003%
48	6.587	1722	1725	1727	rBV2	343	175	0.01%	0.001%
49	6.619	1730	1735	1742	rBV4	1394	1954	0.12%	0.015%
50	6.735	1768	1771	1773	rBV2	80	54	0.00%	0.000%
51	6.747	1773	1775	1776	rBV2	299	152	0.01%	0.001%
52	6.783	1785	1786	1789	rVB2	273	72	0.00%	0.001%
53	6.799	1789	1791	1793	rBV2	113	53	0.00%	0.000%
54	6.815	1793	1796	1799	rBV2	354	230	0.01%	0.002%
55	6.883	1815	1817	1820	rVB2	200	130	0.01%	0.001%
56	6.979	1835	1847	1872	rBV	208382	382679	23.18%	2.864%
57	7.140	1895	1897	1899	rBV2	554	235	0.01%	0.002%
58	7.307	1937	1949	1985	rBV	769462	1375369	83.32%	10.294%
59	7.612	2034	2044	2069	rBV2	143546	250531	15.18%	1.875%
60	7.828	2109	2111	2113	rBV2	386	157	0.01%	0.001%
61	8.082	2179	2190	2227	rBV	460704	834698	50.57%	6.248%
62	8.603	2349	2352	2354	rBV3	326	267	0.02%	0.002%
63	8.741	2393	2395	2399	rBV	227	114	0.01%	0.001%
64	8.760	2399	2401	2405	rBV2	299	230	0.01%	0.002%
65	8.844	2411	2427	2457	rBV	816076	1355567	82.12%	10.146%
66	9.220	2540	2544	2546	rBV2	367	272	0.02%	0.002%
67	9.349	2580	2584	2586	rBV3	211	146	0.01%	0.001%
68	9.403	2599	2601	2605	rVB3	484	309	0.02%	0.002%
69	9.593	2658	2660	2662	rBV2	71	37	0.00%	0.000%
70	9.606	2662	2664	2667	rBV	175	119	0.01%	0.001%
71	9.889	2750	2752	2754	rBV	247	116	0.01%	0.001%
72	9.969	2775	2777	2778	rBV	148	63	0.00%	0.000%
73	9.979	2778	2780	2784	rVB2	254	124	0.01%	0.001%
74	10.005	2784	2788	2791	rBV3	288	253	0.02%	0.002%
75	10.079	2808	2811	2814	rBV	416	332	0.02%	0.002%
76	10.207	2836	2851	2873	rBV	539717	862957	52.28%	6.459%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
 Data File : VV029463.D
 Acq On : 08 Dec 2022 11:31
 Operator : SY/MD
 Sample : VV1208WBL04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK299

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.390	2905	2908	2916	rVB2	551	452	0.03%	0.003%
78	10.487	2937	2938	2941	rBV	220	65	0.00%	0.000%
79	10.525	2944	2950	2955	rBV4	970	994	0.06%	0.007%
80	10.548	2955	2957	2961	rVB2	464	247	0.01%	0.002%
81	10.706	3002	3006	3007	rBV2	338	288	0.02%	0.002%
82	10.847	3046	3050	3052	rBV	511	365	0.02%	0.003%
83	10.902	3063	3067	3075	rBV5	807	1185	0.07%	0.009%
84	11.008	3098	3100	3101	rBV	327	155	0.01%	0.001%
85	11.175	3144	3152	3158	rBV4	1277	1939	0.12%	0.015%
86	11.236	3159	3171	3199	rBV	912486	1440803	87.28%	10.784%
87	11.471	3243	3244	3250	rVB3	671	624	0.04%	0.005%
88	11.509	3250	3256	3258	rBV2	506	459	0.03%	0.003%
89	11.612	3275	3288	3313	rBV	868752	1345628	81.52%	10.072%
90	11.953	3392	3394	3395	rBV	176	76	0.00%	0.001%
91	12.204	3469	3472	3475	rBV2	446	287	0.02%	0.002%
92	13.496	3868	3874	3885	rVB	4355	7040	0.43%	0.053%


Sum of corrected areas: 13360372

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
Data File : VV029463.D
Acq On : 08 Dec 2022 11:31
Operator : SY/MD
Sample : VV1208WBL04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK299

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

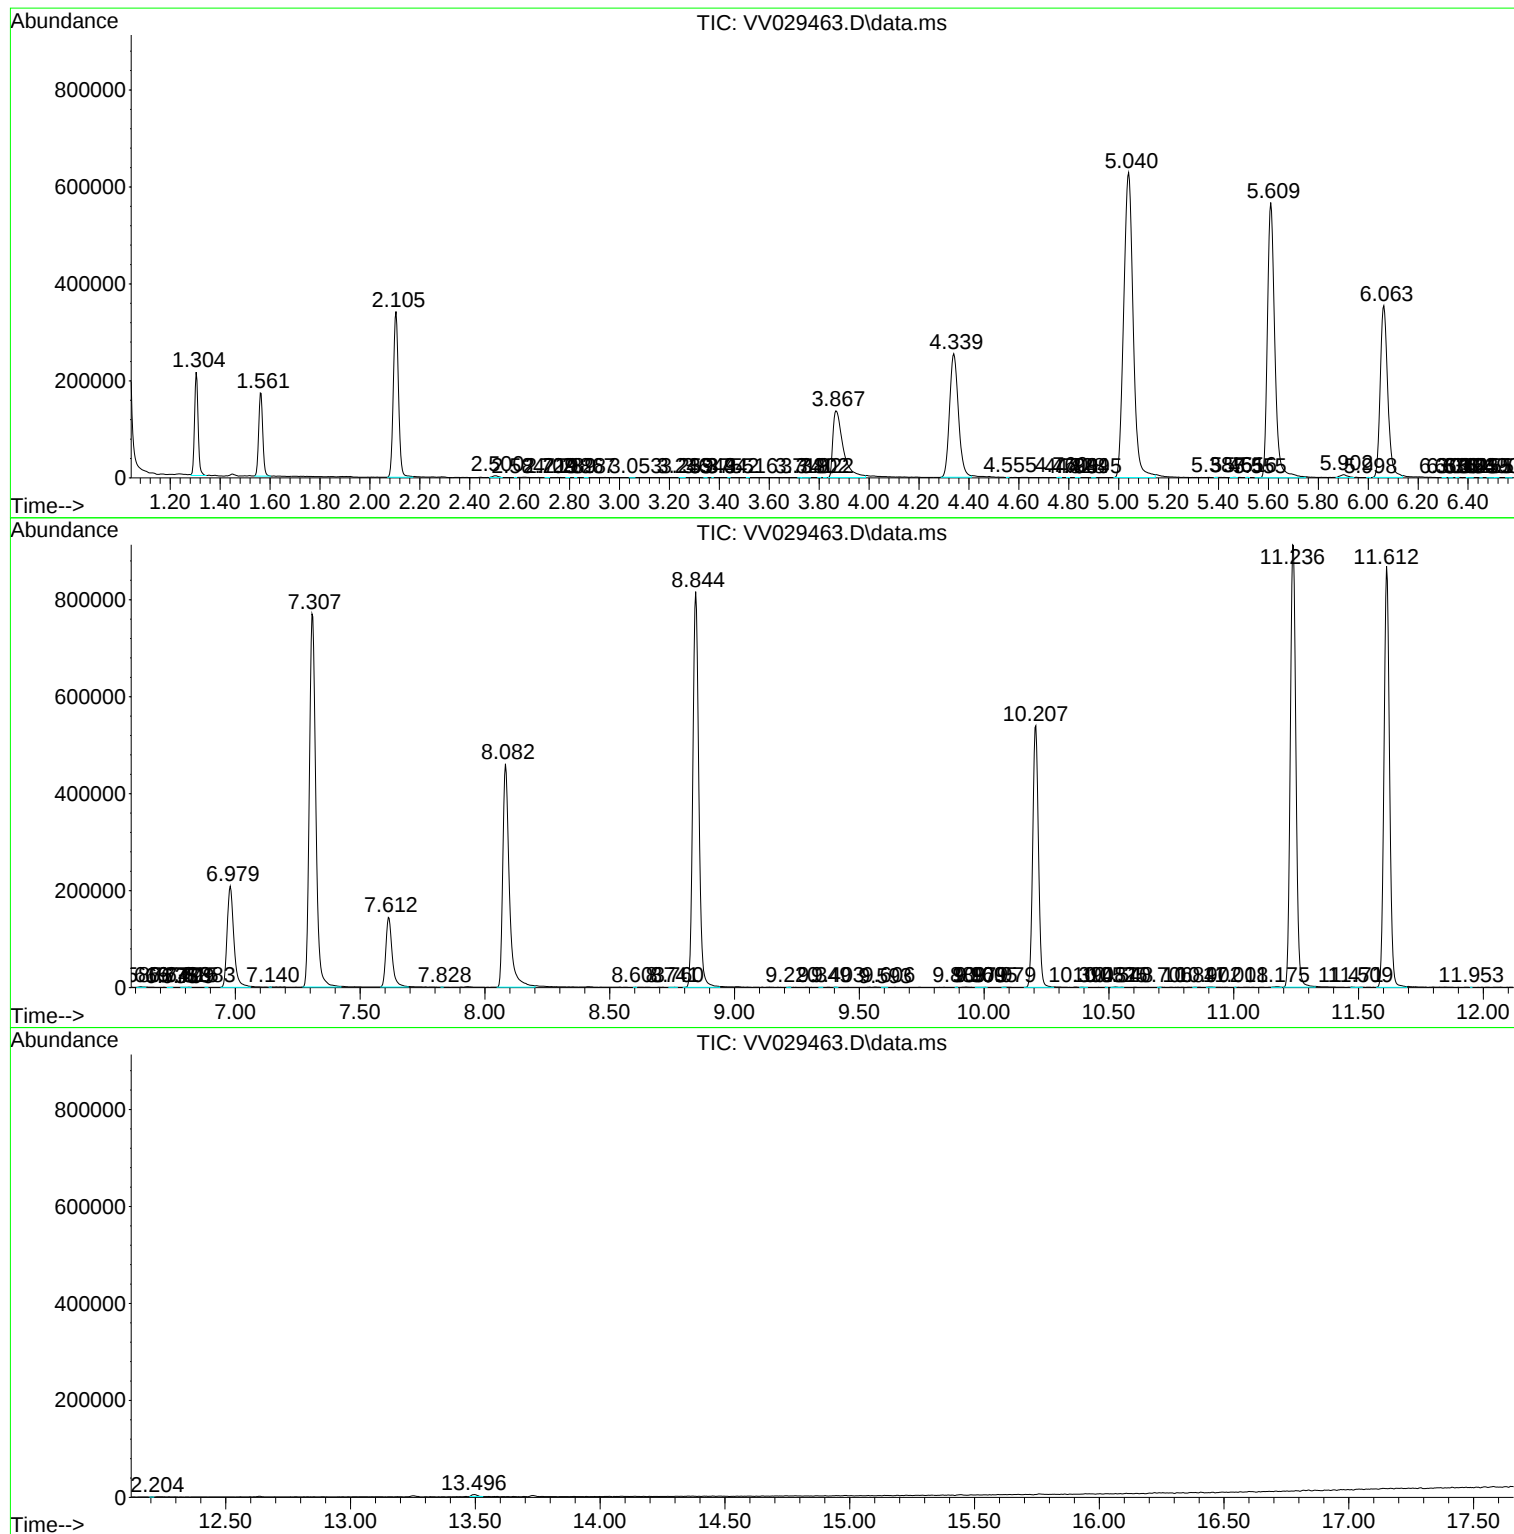

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
Data File : VV029463.D
Acq On : 08 Dec 2022 11:31
Operator : SY/MD
Sample : VV1208WBL04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK299

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
Data File : VV029463.D
Acq On : 08 Dec 2022 11:31
Operator : SY/MD
Sample : VV1208WBL04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK299

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc