

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
 Data File : VV029472.D
 Acq On : 08 Dec 2022 15:03
 Operator : SY/MD
 Sample : N5894-03DL 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M

Title : VOC Analysis

Signal : TIC: VV029472.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	99	rVB	191241	191527	11.82%	1.427%
2	1.564	155	163	179	rVB	165317	185488	11.45%	1.382%
3	2.105	321	331	345	rBV	315264	451270	27.85%	3.362%
4	2.503	446	455	467	rBV2	9525	14842	0.92%	0.111%
5	2.571	472	476	479	rBV2	318	326	0.02%	0.002%
6	2.671	505	507	514	rVB3	274	271	0.02%	0.002%
7	2.931	586	588	590	rBV	237	135	0.01%	0.001%
8	2.973	598	601	602	rBV	156	89	0.01%	0.001%
9	3.027	615	618	621	rBV2	175	118	0.01%	0.001%
10	3.060	625	628	633	rVB	279	183	0.01%	0.001%
11	3.092	634	638	641	rBV2	193	154	0.01%	0.001%
12	3.150	652	656	657	rBV	247	122	0.01%	0.001%
13	3.230	676	681	685	rBV2	346	332	0.02%	0.002%
14	3.288	696	699	702	rBV	134	95	0.01%	0.001%
15	3.458	749	752	754	rBV	251	172	0.01%	0.001%
16	3.497	760	764	766	rBV2	248	180	0.01%	0.001%
17	3.542	776	778	780	rVB2	226	97	0.01%	0.001%
18	3.561	780	784	786	rBV2	239	183	0.01%	0.001%
19	3.587	789	792	796	rBV3	317	206	0.01%	0.002%
20	3.658	811	814	820	rVB	238	180	0.01%	0.001%
21	3.699	821	827	829	rBV2	184	178	0.01%	0.001%
22	3.870	867	880	914	rBV	132982	368213	22.73%	2.743%
23	4.339	1009	1026	1054	rBV2	248697	619814	38.26%	4.617%
24	4.654	1119	1124	1126	rBV3	390	400	0.02%	0.003%
25	4.786	1163	1165	1166	rBV	155	84	0.01%	0.001%
26	4.809	1170	1172	1175	rBV	167	112	0.01%	0.001%
27	4.905	1197	1202	1206	rVB3	288	249	0.02%	0.002%
28	4.937	1209	1212	1215	rBV2	187	114	0.01%	0.001%
29	4.957	1215	1218	1220	rVV	154	87	0.01%	0.001%
30	5.040	1226	1244	1253	rBV2	613334	1579100	97.47%	11.764%
31	5.471	1375	1378	1381	rBV3	457	409	0.03%	0.003%
32	5.516	1389	1392	1394	rBV2	389	197	0.01%	0.001%
33	5.609	1404	1421	1457	rBV	568224	1157085	71.42%	8.620%
34	5.899	1502	1511	1530	rVB5	4649	10225	0.63%	0.076%
35	6.063	1547	1562	1599	rBV	344890	721059	44.51%	5.372%
36	6.272	1625	1627	1630	rBV2	338	176	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120822\
 Data File : VW029472.D
 Acq On : 08 Dec 2022 15:03
 Operator : SY/MD
 Sample : N5894-03DL 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.349	1648	1651	1655	rVB2	200	161	0.01%	0.001%
38	6.375	1655	1659	1661	rBV2	147	104	0.01%	0.001%
39	6.394	1661	1665	1668	rVB2	237	183	0.01%	0.001%
40	6.420	1670	1673	1674	rBV	195	95	0.01%	0.001%
41	6.487	1688	1694	1698	rBV2	211	287	0.02%	0.002%
42	6.551	1709	1714	1715	rBV2	118	91	0.01%	0.001%
43	6.580	1721	1723	1727	rBV2	292	170	0.01%	0.001%
44	6.625	1730	1737	1743	rBV6	1574	2633	0.16%	0.020%
45	6.764	1776	1780	1785	rVB2	249	179	0.01%	0.001%
46	6.873	1812	1814	1815	rBV2	215	85	0.01%	0.001%
47	6.902	1821	1823	1826	rVB2	231	122	0.01%	0.001%
48	6.924	1826	1830	1834	rBV2	291	301	0.02%	0.002%
49	6.979	1835	1847	1879	rBV	202634	371196	22.91%	2.765%
50	7.307	1937	1949	1981	rBV	748250	1323203	81.67%	9.857%
51	7.612	2034	2044	2069	rBV	137047	243131	15.01%	1.811%
52	8.082	2180	2190	2225	rBV	436573	787894	48.63%	5.869%
53	8.648	2363	2366	2367	rBV	378	219	0.01%	0.002%
54	8.686	2375	2378	2381	rVB2	286	176	0.01%	0.001%
55	8.796	2409	2412	2415	rBV3	304	179	0.01%	0.001%
56	8.844	2415	2427	2432	rBV	852531	1423277	87.85%	10.603%
57	9.214	2537	2542	2546	rBV4	407	400	0.02%	0.003%
58	9.262	2555	2557	2559	rBV	261	111	0.01%	0.001%
59	9.294	2564	2567	2568	rBV	165	93	0.01%	0.001%
60	9.323	2574	2576	2577	rBV	251	122	0.01%	0.001%
61	9.403	2599	2601	2604	rBV	141	106	0.01%	0.001%
62	9.445	2611	2614	2616	rBV	205	101	0.01%	0.001%
63	9.471	2620	2622	2623	rBV	260	113	0.01%	0.001%
64	9.532	2638	2641	2642	rBV	407	200	0.01%	0.001%
65	9.606	2658	2664	2668	rBV2	467	454	0.03%	0.003%
66	9.683	2685	2688	2693	rBV4	339	330	0.02%	0.002%
67	9.709	2693	2696	2698	rBV	237	184	0.01%	0.001%
68	9.754	2708	2710	2716	rVB2	404	327	0.02%	0.002%
69	9.789	2716	2721	2725	rBV2	478	421	0.03%	0.003%
70	9.825	2728	2732	2735	rBV2	243	208	0.01%	0.002%
71	9.886	2748	2751	2755	rBV2	316	266	0.02%	0.002%
72	9.908	2755	2758	2761	rBV	430	327	0.02%	0.002%
73	9.956	2768	2773	2774	rBV	187	151	0.01%	0.001%
74	10.030	2792	2796	2798	rBV2	407	312	0.02%	0.002%
75	10.066	2804	2807	2808	rBV2	248	143	0.01%	0.001%
76	10.127	2820	2826	2830	rBV2	247	359	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
 Data File : VV029472.D
 Acq On : 08 Dec 2022 15:03
 Operator : SY/MD
 Sample : N5894-03DL 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.207	2839	2851	2875	rBV	532293	839399	51.81%	6.253%
78	10.371	2896	2902	2911	rVB5	1858	2945	0.18%	0.022%
79	10.407	2911	2913	2917	rVB2	353	211	0.01%	0.002%
80	10.429	2917	2920	2923	rBV2	403	322	0.02%	0.002%
81	10.526	2945	2950	2951	rBV2	549	409	0.03%	0.003%
82	10.558	2958	2960	2962	rBV2	313	133	0.01%	0.001%
83	10.812	3035	3039	3043	rBV2	300	366	0.02%	0.003%
84	10.899	3062	3066	3069	rBV3	412	443	0.03%	0.003%
85	11.072	3119	3120	3123	rBV	246	140	0.01%	0.001%
86	11.108	3128	3131	3135	rBV2	344	343	0.02%	0.003%
87	11.172	3145	3151	3159	rVB5	4370	5702	0.35%	0.042%
88	11.239	3159	3172	3202	rBV2	907284	1620141	100.00%	12.069%
89	11.551	3259	3269	3270	rBV4	2539	2523	0.16%	0.019%
90	11.612	3276	3288	3315	rBV2	820527	1483532	91.57%	11.052%
91	11.818	3350	3352	3356	rBV3	272	187	0.01%	0.001%
92	11.863	3364	3366	3369	rVB3	341	164	0.01%	0.001%
93	11.921	3381	3384	3388	rBV2	481	286	0.02%	0.002%
94	11.960	3393	3396	3400	rVB3	409	286	0.02%	0.002%
95	12.072	3428	3431	3437	rBV2	264	189	0.01%	0.001%
96	12.686	3619	3622	3623	rBV	348	136	0.01%	0.001%
97	12.821	3661	3664	3670	rBV3	522	538	0.03%	0.004%
98	12.902	3686	3689	3693	rBV4	505	417	0.03%	0.003%
99	13.043	3729	3733	3735	rBV3	376	289	0.02%	0.002%
100	13.249	3791	3797	3806	rBV4	1831	2689	0.17%	0.020%




Sum of corrected areas: 13423676

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
Data File : VV029472.D
Acq On : 08 Dec 2022 15:03
Operator : SY/MD
Sample : N5894-03DL 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

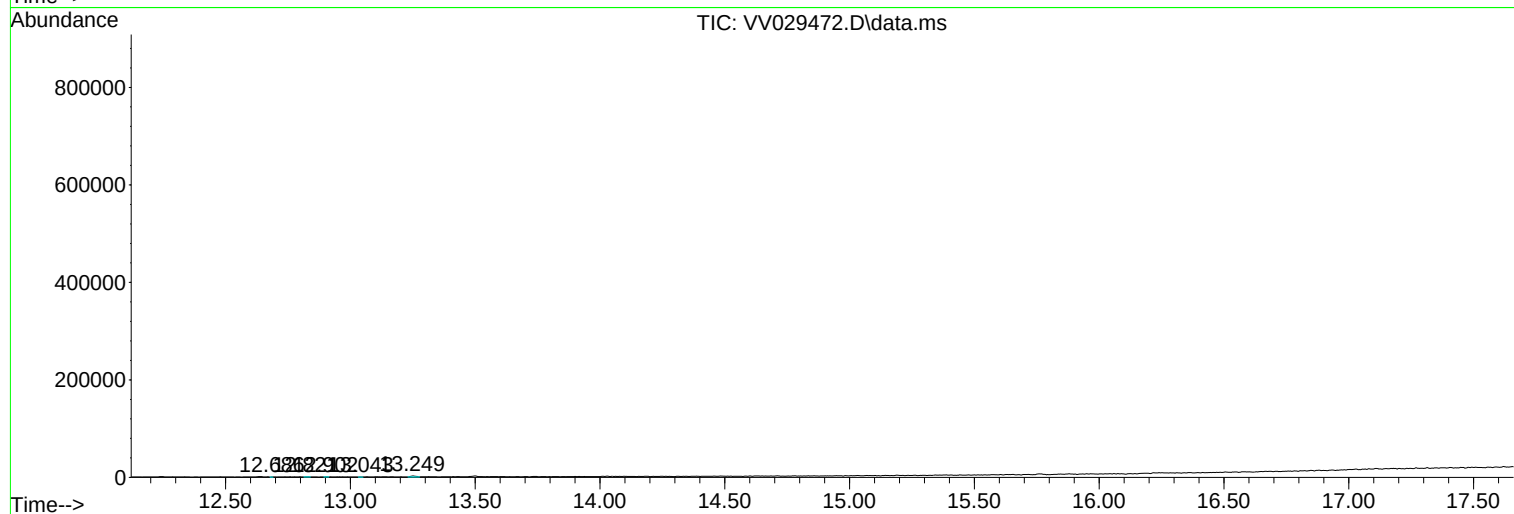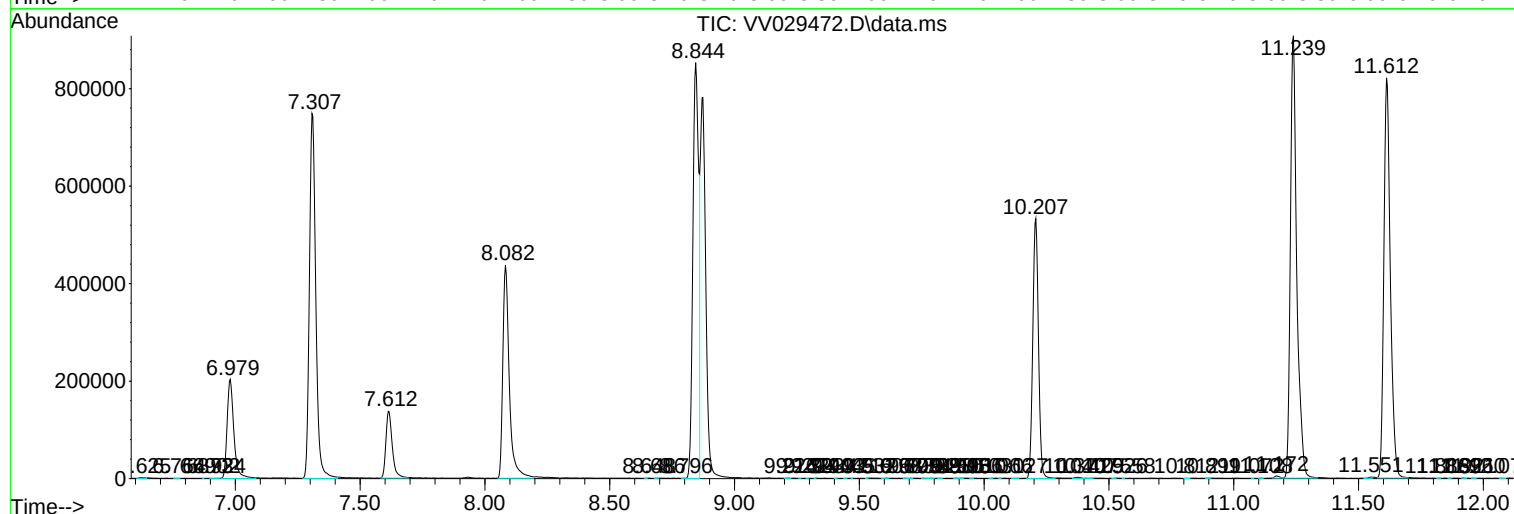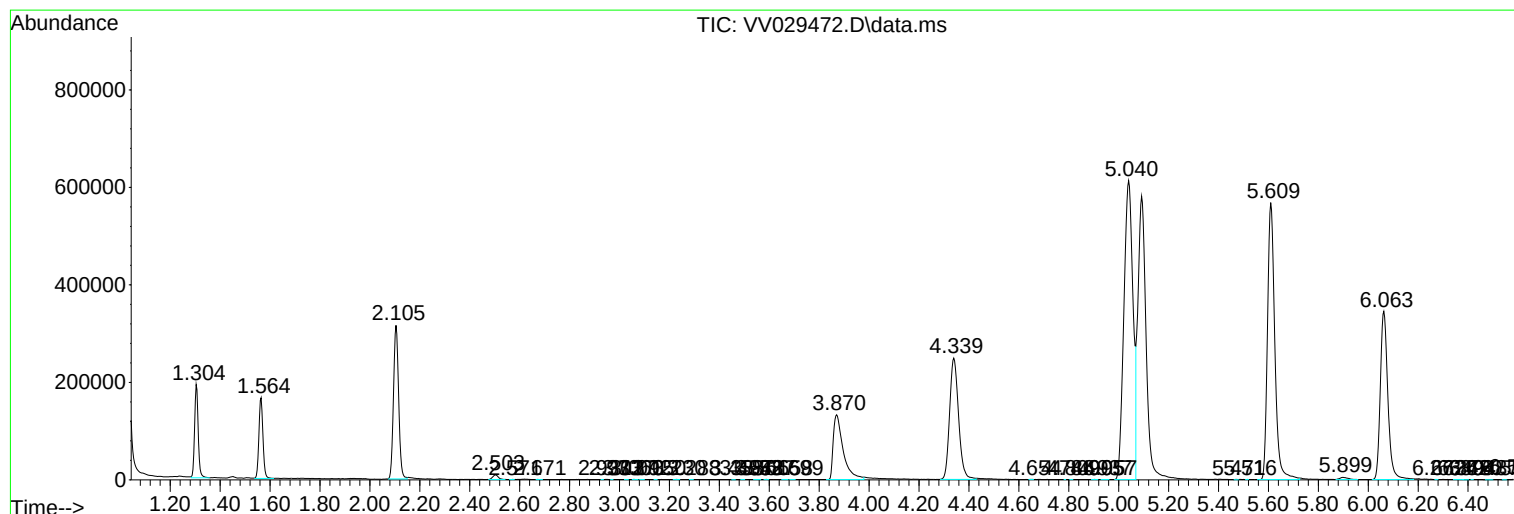

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
Data File : VV029472.D
Acq On : 08 Dec 2022 15:03
Operator : SY/MD
Sample : N5894-03DL 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
Data File : VV029472.D
Acq On : 08 Dec 2022 15:03
Operator : SY/MD
Sample : N5894-03DL 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------