

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
 Data File : VV029473.D
 Acq On : 08 Dec 2022 15:26
 Operator : SY/MD
 Sample : N5894-08DL 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB3DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M

Title : VOC Analysis

Signal : TIC: VV029473.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	97	rVB	186621	185295	11.24%	1.441%
2	1.561	154	162	181	rVB	154083	174529	10.59%	1.357%
3	1.793	232	234	236	rBV2	727	376	0.02%	0.003%
4	1.992	293	296	300	rBV3	381	312	0.02%	0.002%
5	2.031	304	308	310	rBV2	384	324	0.02%	0.003%
6	2.105	317	331	346	rBV	302380	433699	26.31%	3.373%
7	2.445	434	437	440	rVB2	349	251	0.02%	0.002%
8	2.503	445	455	469	rVB	9677	15102	0.92%	0.117%
9	2.616	487	490	493	rBV3	252	198	0.01%	0.002%
10	2.931	582	588	589	rBV2	226	219	0.01%	0.002%
11	2.989	603	606	611	rVB2	236	206	0.01%	0.002%
12	3.420	738	740	749	rVB2	278	291	0.02%	0.002%
13	3.471	749	756	761	rBV	152	261	0.02%	0.002%
14	3.870	866	880	932	rBV	116812	343252	20.83%	2.669%
15	4.339	1008	1026	1058	rBV	233068	578222	35.08%	4.496%
16	4.613	1106	1111	1112	rBV3	241	207	0.01%	0.002%
17	4.645	1117	1121	1124	rBV3	425	349	0.02%	0.003%
18	5.040	1223	1244	1252	rBV2	571541	1433045	86.94%	11.144%
19	5.397	1352	1355	1357	rBV2	312	244	0.01%	0.002%
20	5.410	1357	1359	1363	rVB2	365	275	0.02%	0.002%
21	5.542	1396	1400	1403	rBV3	463	420	0.03%	0.003%
22	5.609	1408	1421	1464	rBV	553866	1129123	68.50%	8.780%
23	5.902	1502	1512	1526	rBV3	4447	10199	0.62%	0.079%
24	5.966	1530	1532	1535	rVB2	507	262	0.02%	0.002%
25	6.063	1547	1562	1595	rBV	329572	675454	40.98%	5.253%
26	6.198	1599	1604	1610	rVV5	839	1036	0.06%	0.008%
27	6.265	1623	1625	1627	rVB2	456	197	0.01%	0.002%
28	6.326	1642	1644	1648	rVB3	310	237	0.01%	0.002%
29	6.368	1654	1657	1660	rBV2	368	224	0.01%	0.002%
30	6.561	1715	1717	1722	rVB3	347	211	0.01%	0.002%
31	6.619	1730	1735	1737	rBV3	971	873	0.05%	0.007%
32	6.783	1780	1786	1787	rBV	323	293	0.02%	0.002%
33	6.847	1800	1806	1809	rBV2	394	417	0.03%	0.003%
34	6.979	1835	1847	1879	rBV	187464	346608	21.03%	2.695%
35	7.140	1893	1897	1899	rBV4	459	367	0.02%	0.003%
36	7.307	1937	1949	1987	rBV	699144	1244688	75.52%	9.679%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120822\
 Data File : VW029473.D
 Acq On : 08 Dec 2022 15:26
 Operator : SY/MD
 Sample : N5894-08DL 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB3DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	7.612	2034	2044	2065	rBV	128453	226753	13.76%	1.763%
38	7.908	2133	2136	2137	rBV	424	214	0.01%	0.002%
39	7.934	2138	2144	2152	rVB4	2051	2971	0.18%	0.023%
40	8.082	2179	2190	2222	rBV	403270	732852	44.46%	5.699%
41	8.304	2256	2259	2266	rVB5	866	822	0.05%	0.006%
42	8.368	2275	2279	2282	rBV3	395	264	0.02%	0.002%
43	8.510	2319	2323	2326	rBV4	433	363	0.02%	0.003%
44	8.583	2341	2346	2349	rVB3	393	292	0.02%	0.002%
45	8.690	2376	2379	2382	rBV3	474	330	0.02%	0.003%
46	8.844	2415	2427	2432	rBV	854530	1391311	84.41%	10.819%
47	9.182	2530	2532	2538	rVB2	546	391	0.02%	0.003%
48	9.265	2554	2558	2562	rBV2	237	276	0.02%	0.002%
49	9.310	2567	2572	2575	rBV3	309	316	0.02%	0.002%
50	9.365	2585	2589	2593	rVB4	300	295	0.02%	0.002%
51	9.487	2620	2627	2630	rBV3	329	343	0.02%	0.003%
52	9.516	2633	2636	2639	rBV2	379	212	0.01%	0.002%
53	9.542	2642	2644	2647	rVB2	356	213	0.01%	0.002%
54	9.609	2659	2665	2669	rVB2	406	403	0.02%	0.003%
55	9.635	2669	2673	2677	rBV2	237	237	0.01%	0.002%
56	9.702	2690	2694	2698	rBV2	341	314	0.02%	0.002%
57	9.918	2758	2761	2764	rVV	358	240	0.01%	0.002%
58	10.053	2797	2803	2804	rVV2	277	271	0.02%	0.002%
59	10.133	2821	2828	2830	rBV2	310	389	0.02%	0.003%
60	10.207	2838	2851	2868	rBV	499580	784268	47.58%	6.099%
61	10.371	2899	2902	2911	rVB3	1428	1776	0.11%	0.014%
62	10.452	2925	2927	2932	rVB2	375	234	0.01%	0.002%
63	10.490	2932	2939	2944	rVB3	283	373	0.02%	0.003%
64	10.529	2948	2951	2957	rBV3	659	686	0.04%	0.005%
65	10.596	2968	2972	2977	rBV2	282	323	0.02%	0.003%
66	10.619	2977	2979	2983	rBV2	325	243	0.01%	0.002%
67	10.680	2996	2998	3005	rVB	315	274	0.02%	0.002%
68	10.763	3021	3024	3027	rVB2	351	200	0.01%	0.002%
69	10.789	3027	3032	3035	rBV2	266	282	0.02%	0.002%
70	10.863	3053	3055	3059	rVB2	442	234	0.01%	0.002%
71	10.899	3059	3066	3068	rBV3	491	548	0.03%	0.004%
72	10.915	3069	3071	3075	rVV3	752	523	0.03%	0.004%
73	10.937	3075	3078	3079	rVV	306	199	0.01%	0.002%
74	10.950	3080	3082	3085	rVV2	440	221	0.01%	0.002%
75	10.979	3088	3091	3093	rBV2	390	222	0.01%	0.002%
76	11.001	3096	3098	3103	rVB2	382	303	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
 Data File : VV029473.D
 Acq On : 08 Dec 2022 15:26
 Operator : SY/MD
 Sample : N5894-08DL 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB3DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	11.030	3103	3107	3109	rBV	284	235	0.01%	0.002%
78	11.127	3131	3137	3141	rBV3	312	415	0.03%	0.003%
79	11.175	3144	3152	3159	rBV3	5061	7550	0.46%	0.059%
80	11.239	3160	3172	3200	rVV2	929891	1648255	100.00%	12.817%
81	11.429	3229	3231	3236	rVB2	675	415	0.03%	0.003%
82	11.548	3265	3268	3272	rBV4	528	457	0.03%	0.004%
83	11.567	3272	3274	3276	rVV2	591	302	0.02%	0.002%
84	11.616	3276	3289	3314	rVV2	816587	1464746	88.87%	11.390%
85	11.808	3344	3349	3354	rVB3	486	673	0.04%	0.005%
86	11.834	3354	3357	3363	rBV3	527	639	0.04%	0.005%
87	12.017	3410	3414	3416	rBV2	257	219	0.01%	0.002%
88	12.246	3478	3485	3487	rBV3	540	710	0.04%	0.006%
89	12.297	3499	3501	3506	rVB2	549	412	0.02%	0.003%
90	12.336	3510	3513	3514	rBV	431	248	0.02%	0.002%
91	12.390	3527	3530	3533	rBV2	437	327	0.02%	0.003%
92	12.551	3576	3580	3583	rBV3	306	270	0.02%	0.002%
93	12.603	3592	3596	3599	rBV2	445	404	0.02%	0.003%
94	12.779	3649	3651	3653	rBV	360	212	0.01%	0.002%
95	12.969	3707	3710	3712	rBV3	487	362	0.02%	0.003%
96	13.037	3729	3731	3737	rVB3	591	482	0.03%	0.004%
97	13.252	3793	3798	3804	rVB5	1619	1987	0.12%	0.015%
98	13.368	3832	3834	3837	rVB	577	345	0.02%	0.003%
99	13.397	3839	3843	3847	rBV2	718	675	0.04%	0.005%
100	13.496	3867	3874	3877	rBV4	753	1022	0.06%	0.008%




Sum of corrected areas: 12859609

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
Data File : VV029473.D
Acq On : 08 Dec 2022 15:26
Operator : SY/MD
Sample : N5894-08DL 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

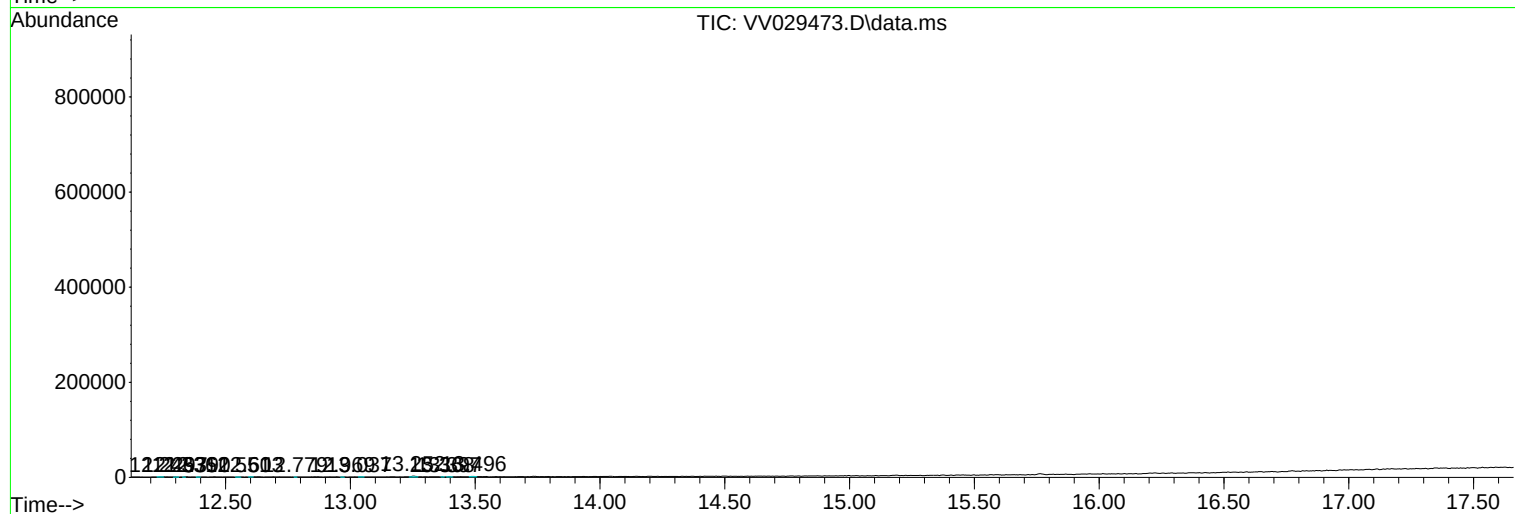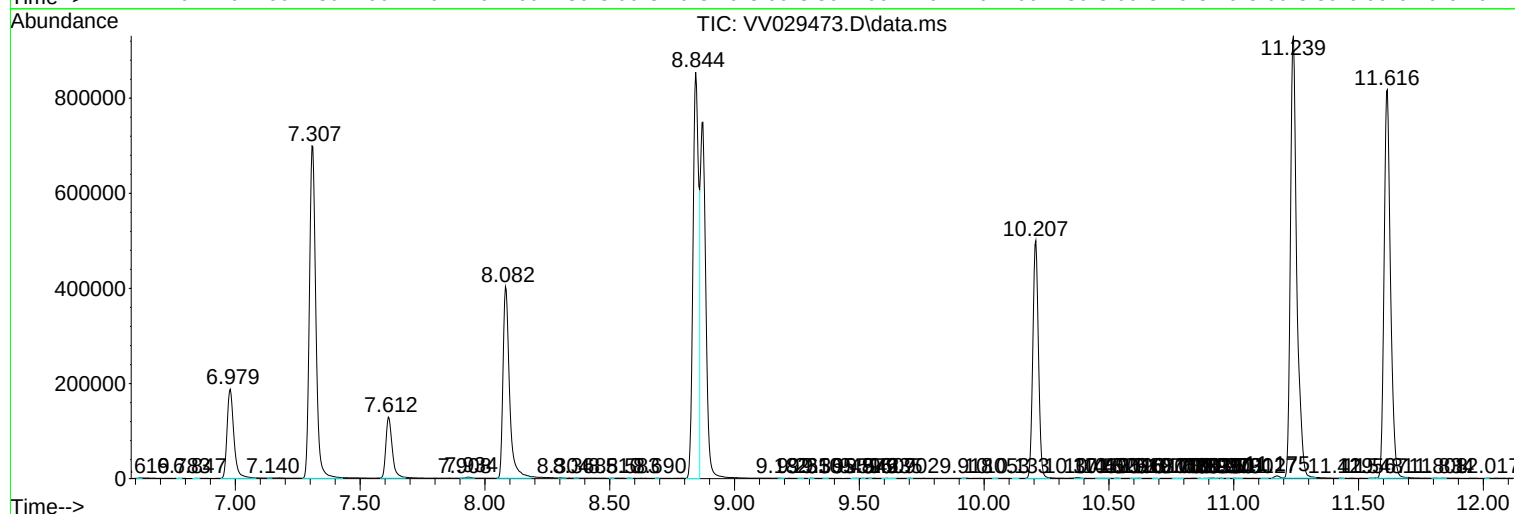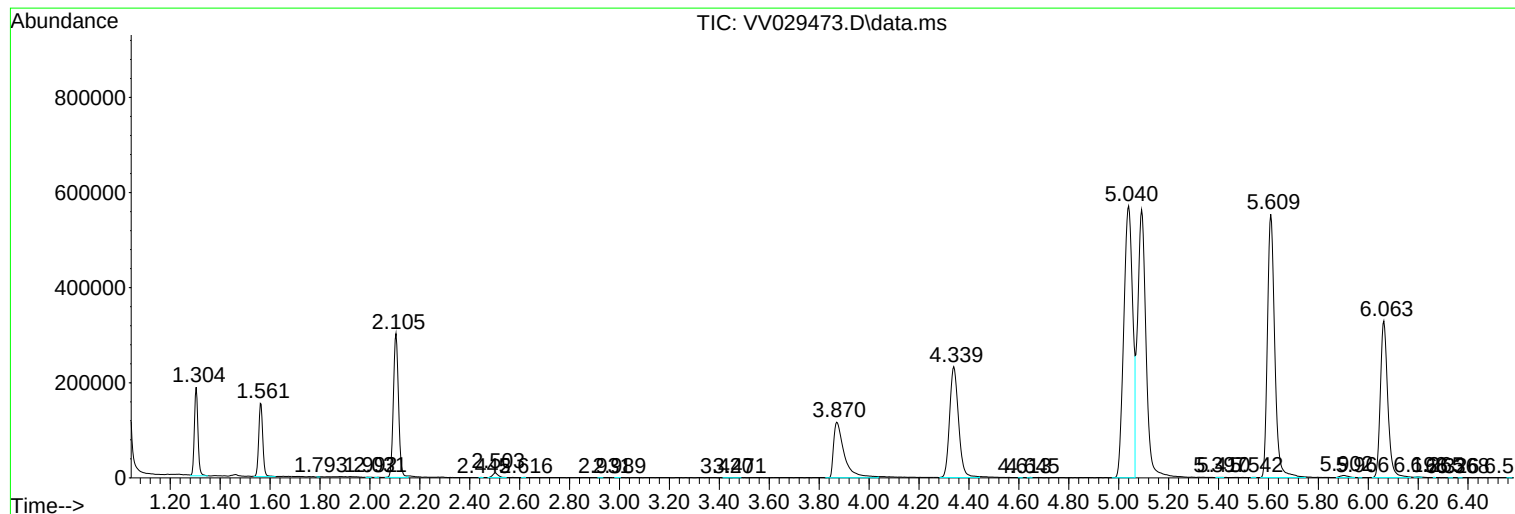

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
Data File : VV029473.D
Acq On : 08 Dec 2022 15:26
Operator : SY/MD
Sample : N5894-08DL 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
Data File : VV029473.D
Acq On : 08 Dec 2022 15:26
Operator : SY/MD
Sample : N5894-08DL 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------