

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
 Data File : VV029475.D
 Acq On : 08 Dec 2022 16:13
 Operator : SY/MD
 Sample : N5919-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EE9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M

Title : VOC Analysis

Signal : TIC: VV029475.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	99	rVB	177927	177263	11.70%	1.420%
2	1.561	155	162	175	rVB	154637	170329	11.25%	1.365%
3	2.105	320	331	345	rBV	297237	425517	28.09%	3.410%
4	2.362	407	411	415	rBV2	454	420	0.03%	0.003%
5	2.503	446	455	467	rVB2	9804	15259	1.01%	0.122%
6	3.066	628	630	633	rVB	257	144	0.01%	0.001%
7	3.098	633	640	645	rBV2	236	351	0.02%	0.003%
8	3.220	674	678	683	rBV2	119	103	0.01%	0.001%
9	3.249	683	687	689	rBV2	227	160	0.01%	0.001%
10	3.384	726	729	734	rVB2	311	230	0.02%	0.002%
11	3.439	743	746	749	rVB	138	79	0.01%	0.001%
12	3.478	751	758	761	rBV	167	219	0.01%	0.002%
13	3.600	794	796	799	rVB2	215	103	0.01%	0.001%
14	3.654	808	813	815	rBV	129	129	0.01%	0.001%
15	3.751	841	843	844	rBV	189	63	0.00%	0.001%
16	3.777	849	851	856	rVB2	189	146	0.01%	0.001%
17	3.812	856	862	866	rBV2	182	245	0.02%	0.002%
18	3.870	866	880	919	rBV	128715	371190	24.51%	2.974%
19	4.339	1009	1026	1048	rBV	233493	578371	38.18%	4.634%
20	4.609	1106	1110	1113	rBV2	247	209	0.01%	0.002%
21	4.645	1118	1121	1124	rBV3	428	347	0.02%	0.003%
22	4.699	1135	1138	1140	rBV2	130	82	0.01%	0.001%
23	4.715	1140	1143	1145	rVB2	190	97	0.01%	0.001%
24	4.728	1145	1147	1148	rBV	176	55	0.00%	0.000%
25	4.754	1152	1155	1159	rVB2	242	110	0.01%	0.001%
26	4.793	1166	1167	1173	rVB2	329	172	0.01%	0.001%
27	4.822	1173	1176	1177	rBV2	249	124	0.01%	0.001%
28	4.915	1203	1205	1209	rVV3	187	148	0.01%	0.001%
29	4.947	1209	1215	1220	rVB3	274	299	0.02%	0.002%
30	5.040	1225	1244	1300	rBV2	568878	1514688	100.00%	12.137%
31	5.397	1352	1355	1358	rBV2	490	409	0.03%	0.003%
32	5.423	1361	1363	1365	rVV	207	102	0.01%	0.001%
33	5.458	1372	1374	1376	rBV2	283	135	0.01%	0.001%
34	5.522	1388	1394	1396	rBV3	214	234	0.02%	0.002%
35	5.609	1408	1421	1451	rBV	542659	1100210	72.64%	8.816%
36	5.899	1504	1511	1524	rVB7	4215	8939	0.59%	0.072%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120822\
 Data File : VW029475.D
 Acq On : 08 Dec 2022 16:13
 Operator : SY/MD
 Sample : N5919-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EE9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.063	1547	1562	1598	rBV	329076	681512	44.99%	5.461%
38	6.288	1628	1632	1634	rBV	316	215	0.01%	0.002%
39	6.333	1641	1646	1648	rBV2	189	153	0.01%	0.001%
40	6.375	1657	1659	1664	rVB3	359	201	0.01%	0.002%
41	6.529	1705	1707	1714	rVB3	208	170	0.01%	0.001%
42	6.616	1727	1734	1736	rBV4	1505	1403	0.09%	0.011%
43	6.725	1765	1768	1771	rBV	257	204	0.01%	0.002%
44	6.812	1793	1795	1798	rVB2	288	154	0.01%	0.001%
45	6.828	1798	1800	1804	rBV2	277	229	0.02%	0.002%
46	6.883	1814	1817	1822	rVB2	262	211	0.01%	0.002%
47	6.921	1826	1829	1833	rBV	305	175	0.01%	0.001%
48	6.979	1835	1847	1874	rBV	187795	351656	23.22%	2.818%
49	7.310	1936	1950	1989	rBV	701089	1253236	82.74%	10.042%
50	7.612	2034	2044	2066	rBV	130338	231408	15.28%	1.854%
51	7.934	2137	2144	2153	rVB4	2063	3520	0.23%	0.028%
52	8.027	2170	2173	2176	rBV2	447	343	0.02%	0.003%
53	8.082	2180	2190	2229	rBV	435672	794375	52.44%	6.365%
54	8.484	2311	2315	2316	rBV2	313	243	0.02%	0.002%
55	8.609	2351	2354	2356	rBV3	383	231	0.02%	0.002%
56	8.709	2381	2385	2391	rVB3	451	491	0.03%	0.004%
57	8.744	2391	2396	2402	rBV4	325	405	0.03%	0.003%
58	8.844	2414	2427	2460	rBV	791346	1312897	86.68%	10.520%
59	9.082	2499	2501	2505	rBV2	403	218	0.01%	0.002%
60	9.191	2531	2535	2542	rVB3	316	406	0.03%	0.003%
61	9.223	2542	2545	2546	rBV	328	158	0.01%	0.001%
62	9.236	2547	2549	2551	rVB2	234	80	0.01%	0.001%
63	9.268	2554	2559	2561	rBV3	275	236	0.02%	0.002%
64	9.317	2571	2574	2575	rBV	211	133	0.01%	0.001%
65	9.390	2593	2597	2599	rBV3	199	161	0.01%	0.001%
66	9.426	2605	2608	2610	rBV3	254	157	0.01%	0.001%
67	9.484	2622	2626	2627	rBV2	261	189	0.01%	0.002%
68	9.532	2637	2641	2643	rBV2	280	188	0.01%	0.002%
69	9.561	2648	2650	2652	rBV	228	95	0.01%	0.001%
70	9.596	2659	2661	2665	rVB2	322	161	0.01%	0.001%
71	9.619	2665	2668	2671	rBV	236	227	0.01%	0.002%
72	9.680	2685	2687	2689	rBV	252	103	0.01%	0.001%
73	9.709	2694	2696	2700	rBV2	256	199	0.01%	0.002%
74	9.844	2736	2738	2742	rBV2	261	138	0.01%	0.001%
75	9.915	2756	2760	2761	rBV2	446	331	0.02%	0.003%
76	9.989	2778	2783	2786	rVB2	330	263	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120822\
 Data File : VW029475.D
 Acq On : 08 Dec 2022 16:13
 Operator : SY/MD
 Sample : N5919-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EE9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.005	2786	2788	2792	rBV2	222	172	0.01%	0.001%
78	10.043	2797	2800	2808	rBV3	354	483	0.03%	0.004%
79	10.079	2808	2811	2813	rBV	299	214	0.01%	0.002%
80	10.149	2831	2833	2836	rBV2	226	148	0.01%	0.001%
81	10.207	2839	2851	2873	rVV	517795	813859	53.73%	6.521%
82	10.371	2893	2902	2904	rBV3	1263	1449	0.10%	0.012%
83	10.484	2935	2937	2938	rBV3	165	71	0.00%	0.001%
84	10.638	2983	2985	2987	rBV	167	121	0.01%	0.001%
85	10.831	3043	3045	3046	rBV2	273	109	0.01%	0.001%
86	10.847	3046	3050	3055	rBV2	431	459	0.03%	0.004%
87	10.905	3063	3068	3077	rBV4	729	795	0.05%	0.006%
88	10.940	3077	3079	3085	rBV3	303	296	0.02%	0.002%
89	10.992	3093	3095	3097	rVV2	264	135	0.01%	0.001%
90	11.008	3097	3100	3102	rVV	422	264	0.02%	0.002%
91	11.040	3106	3110	3111	rBV2	269	175	0.01%	0.001%
92	11.095	3124	3127	3130	rBV2	334	196	0.01%	0.002%
93	11.172	3147	3151	3154	rBV3	473	427	0.03%	0.003%
94	11.239	3159	3172	3201	rBV	907174	1393856	92.02%	11.169%
95	11.439	3232	3234	3239	rBV4	502	543	0.04%	0.004%
96	11.509	3254	3256	3257	rBV	351	165	0.01%	0.001%
97	11.551	3266	3269	3275	rVB3	641	653	0.04%	0.005%
98	11.612	3275	3288	3309	rBV	807935	1260751	83.24%	10.102%
99	12.014	3409	3413	3420	rBV3	406	440	0.03%	0.004%
100	12.638	3603	3607	3612	rBV5	685	779	0.05%	0.006%




Sum of corrected areas: 12480116

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
Data File : VV029475.D
Acq On : 08 Dec 2022 16:13
Operator : SY/MD
Sample : N5919-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EE9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

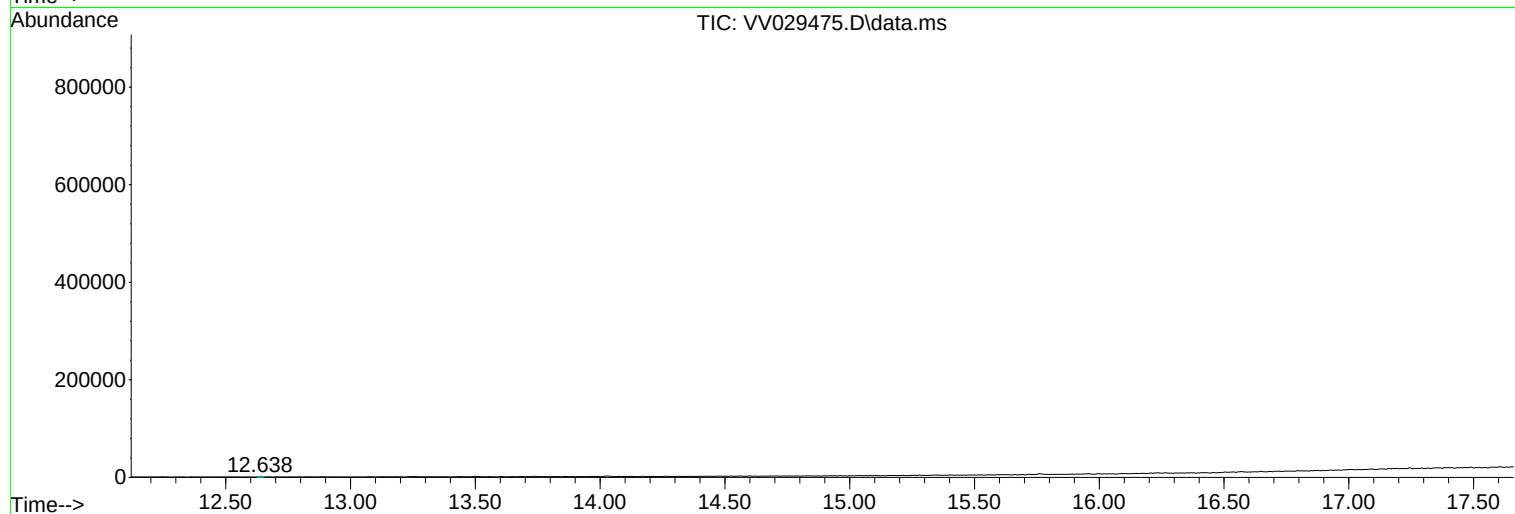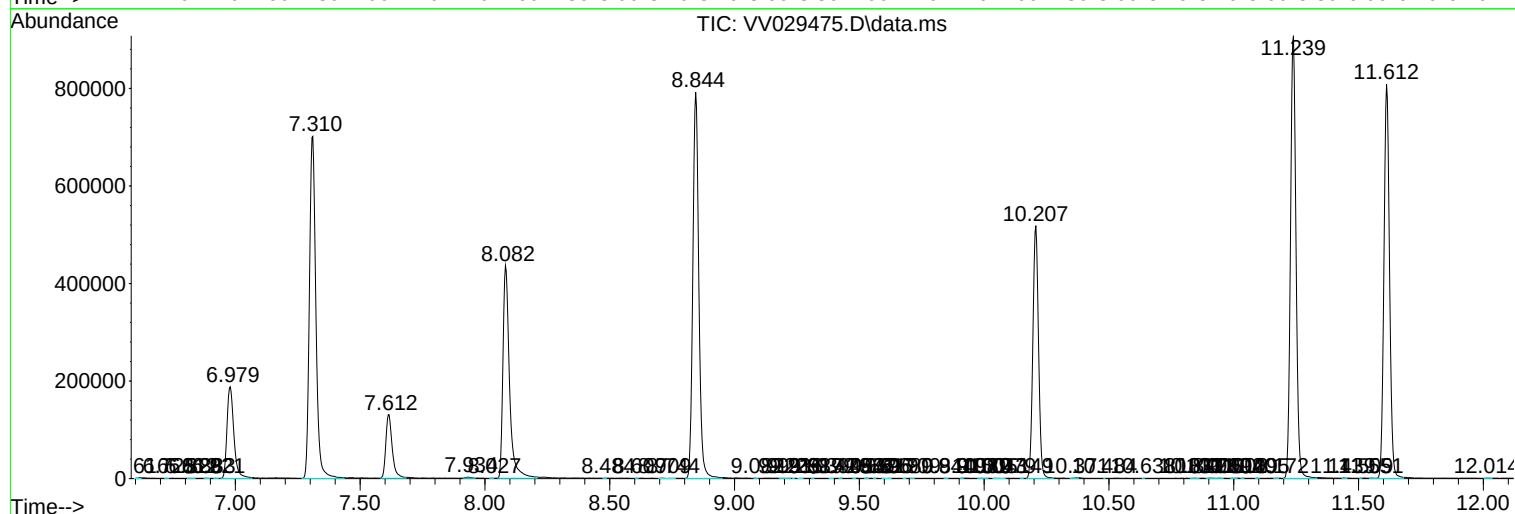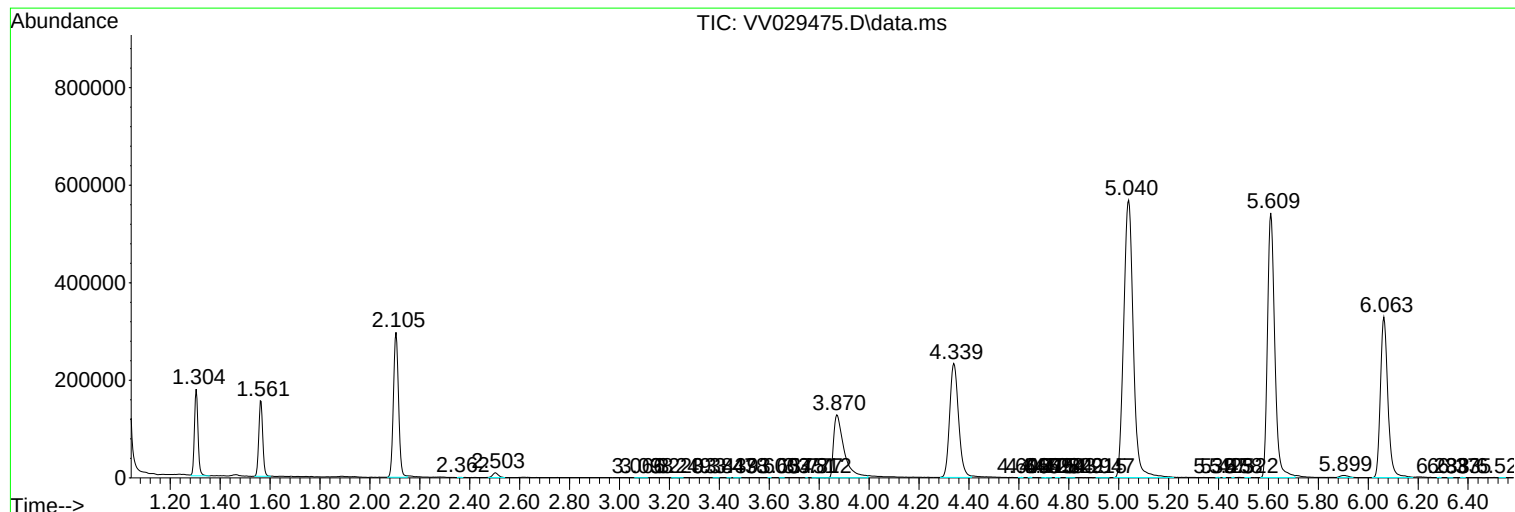

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
Data File : VV029475.D
Acq On : 08 Dec 2022 16:13
Operator : SY/MD
Sample : N5919-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EE9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
Data File : VV029475.D
Acq On : 08 Dec 2022 16:13
Operator : SY/MD
Sample : N5919-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EE9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------