

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
 Data File : VV029478.D
 Acq On : 08 Dec 2022 17:24
 Operator : SY/MD
 Sample : N5920-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EJ2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M

Title : VOC Analysis

Signal : TIC: VV029478.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	95	rVB	180705	180490	11.31%	1.447%
2	1.564	155	163	178	rVB	160157	181364	11.36%	1.454%
3	2.105	320	331	343	rBV	307935	442059	27.69%	3.545%
4	2.426	427	431	432	rBV2	420	303	0.02%	0.002%
5	2.561	468	473	474	rBV	277	239	0.01%	0.002%
6	2.767	533	537	540	rBV2	271	182	0.01%	0.001%
7	2.924	584	586	588	rBV	234	105	0.01%	0.001%
8	2.944	590	592	594	rVV2	293	121	0.01%	0.001%
9	2.992	601	607	610	rBV2	224	183	0.01%	0.001%
10	3.027	613	618	623	rVV2	348	367	0.02%	0.003%
11	3.143	652	654	660	rVB2	384	273	0.02%	0.002%
12	3.178	661	665	666	rBV	137	103	0.01%	0.001%
13	3.207	671	674	682	rVB	262	221	0.01%	0.002%
14	3.243	682	685	686	rBV	194	94	0.01%	0.001%
15	3.404	733	735	738	rVB2	208	108	0.01%	0.001%
16	3.436	744	745	749	rVB2	181	67	0.00%	0.001%
17	3.535	774	776	780	rVB	238	127	0.01%	0.001%
18	3.555	780	782	785	rBV2	92	61	0.00%	0.000%
19	3.622	798	803	807	rBV	305	270	0.02%	0.002%
20	3.641	807	809	811	rBV	44	18	0.00%	0.000%
21	3.658	811	814	816	rBV2	78	50	0.00%	0.000%
22	3.690	819	824	827	rBV2	307	322	0.02%	0.003%
23	3.706	827	829	831	rVV	118	51	0.00%	0.000%
24	3.822	863	865	867	rBV	103	59	0.00%	0.000%
25	3.867	869	879	913	rBV	127850	348518	21.83%	2.795%
26	4.339	1008	1026	1056	rBV	249208	622477	38.99%	4.991%
27	4.622	1110	1114	1118	rBV3	378	367	0.02%	0.003%
28	4.722	1143	1145	1146	rBV	156	71	0.00%	0.001%
29	4.776	1160	1162	1163	rBV	191	91	0.01%	0.001%
30	4.828	1177	1178	1183	rVB	278	107	0.01%	0.001%
31	4.857	1183	1187	1189	rVV2	171	104	0.01%	0.001%
32	4.876	1192	1193	1194	rBB2	83	16	0.00%	0.000%
33	4.969	1220	1222	1223	rBV	122	35	0.00%	0.000%
34	4.979	1223	1225	1226	rBV	214	105	0.01%	0.001%
35	5.040	1226	1244	1295	rVV2	603797	1596337	100.00%	12.800%
36	5.519	1389	1393	1394	rBV	362	248	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120822\
 Data File : VW029478.D
 Acq On : 08 Dec 2022 17:24
 Operator : SY/MD
 Sample : N5920-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EJ2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	5.609	1404	1421	1460	rBV	501575	1022465	64.05%	8.199%
38	5.905	1501	1513	1529	rVB8	8824	19550	1.22%	0.157%
39	5.989	1536	1539	1546	rVB3	483	516	0.03%	0.004%
40	6.063	1546	1562	1598	rBV	345639	724798	45.40%	5.812%
41	6.256	1620	1622	1625	rVB	577	298	0.02%	0.002%
42	6.294	1625	1634	1646	rBV3	6796	14754	0.92%	0.118%
43	6.445	1680	1681	1686	rVB2	234	108	0.01%	0.001%
44	6.526	1698	1706	1707	rBV2	1356	1273	0.08%	0.010%
45	6.587	1723	1725	1729	rVB	181	74	0.00%	0.001%
46	6.622	1729	1736	1742	rBV7	1610	2584	0.16%	0.021%
47	6.747	1772	1775	1778	rBV	224	157	0.01%	0.001%
48	6.792	1785	1789	1792	rBV2	220	173	0.01%	0.001%
49	6.815	1792	1796	1800	rVV4	244	203	0.01%	0.002%
50	6.895	1817	1821	1823	rBV2	235	177	0.01%	0.001%
51	6.911	1823	1826	1832	rVB2	376	316	0.02%	0.003%
52	6.937	1832	1834	1836	rBV	345	210	0.01%	0.002%
53	6.979	1836	1847	1879	rBV	201958	372790	23.35%	2.989%
54	7.156	1897	1902	1905	rBV4	760	921	0.06%	0.007%
55	7.307	1937	1949	1969	rBV	745460	1312633	82.23%	10.525%
56	7.612	2034	2044	2075	rBV	138396	243238	15.24%	1.950%
57	8.082	2180	2190	2231	rBV	454798	832722	52.16%	6.677%
58	8.593	2347	2349	2350	rBV	334	104	0.01%	0.001%
59	8.606	2351	2353	2359	rVV2	347	329	0.02%	0.003%
60	8.648	2364	2366	2367	rBV2	261	85	0.01%	0.001%
61	8.699	2379	2382	2383	rBV2	395	230	0.01%	0.002%
62	8.735	2390	2393	2395	rBV3	376	224	0.01%	0.002%
63	8.844	2414	2427	2456	rBV	732509	1208256	75.69%	9.688%
64	9.136	2512	2518	2528	rVB6	1709	2647	0.17%	0.021%
65	9.239	2548	2550	2554	rBV2	231	148	0.01%	0.001%
66	9.278	2560	2562	2564	rBV	191	99	0.01%	0.001%
67	9.345	2580	2583	2588	rVB3	228	256	0.02%	0.002%
68	9.378	2588	2593	2595	rBV	308	241	0.02%	0.002%
69	9.410	2601	2603	2605	rBV2	237	150	0.01%	0.001%
70	9.461	2616	2619	2622	rBV2	263	176	0.01%	0.001%
71	9.484	2622	2626	2627	rBV3	179	118	0.01%	0.001%
72	9.561	2639	2650	2664	rBV2	5738	10442	0.65%	0.084%
73	9.686	2686	2689	2694	rBV3	255	288	0.02%	0.002%
74	9.744	2704	2707	2708	rBV2	187	100	0.01%	0.001%
75	9.808	2719	2727	2737	rBV4	2307	3396	0.21%	0.027%
76	9.866	2742	2745	2748	rBV2	282	152	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
 Data File : VV029478.D
 Acq On : 08 Dec 2022 17:24
 Operator : SY/MD
 Sample : N5920-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EJ2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	9.924	2759	2763	2768	rVB2	637	572	0.04%	0.005%
78	9.947	2768	2770	2771	rBV	207	68	0.00%	0.001%
79	9.979	2774	2780	2781	rBV2	302	321	0.02%	0.003%
80	10.040	2798	2799	2804	rVB2	234	118	0.01%	0.001%
81	10.062	2804	2806	2807	rBV2	123	55	0.00%	0.000%
82	10.136	2825	2829	2831	rBV2	242	186	0.01%	0.001%
83	10.207	2838	2851	2873	rBV	531842	848925	53.18%	6.807%
84	10.529	2949	2951	2953	rBV	413	265	0.02%	0.002%
85	10.712	3006	3008	3010	rVB2	150	42	0.00%	0.000%
86	10.725	3010	3012	3014	rBV	138	73	0.00%	0.001%
87	10.824	3040	3043	3045	rBV2	250	152	0.01%	0.001%
88	11.037	3106	3109	3110	rBV	443	256	0.02%	0.002%
89	11.111	3127	3132	3134	rBV2	367	358	0.02%	0.003%
90	11.140	3138	3141	3147	rBV3	856	1047	0.07%	0.008%
91	11.239	3160	3172	3194	rBV	775522	1203470	75.39%	9.650%
92	11.448	3235	3237	3240	rBV	255	136	0.01%	0.001%
93	11.468	3240	3243	3246	rBV3	336	270	0.02%	0.002%
94	11.551	3261	3269	3276	rBV7	3279	5734	0.36%	0.046%
95	11.612	3276	3288	3317	rVV	787331	1253344	78.51%	10.050%
96	11.934	3384	3388	3391	rBV	398	305	0.02%	0.002%
97	11.950	3391	3393	3394	rBV	226	74	0.00%	0.001%
98	12.342	3511	3515	3518	rBV3	1067	797	0.05%	0.006%
99	13.252	3794	3798	3804	rBV3	1142	1385	0.09%	0.011%




Sum of corrected areas: 12471067

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
Data File : VV029478.D
Acq On : 08 Dec 2022 17:24
Operator : SY/MD
Sample : N5920-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EJ2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

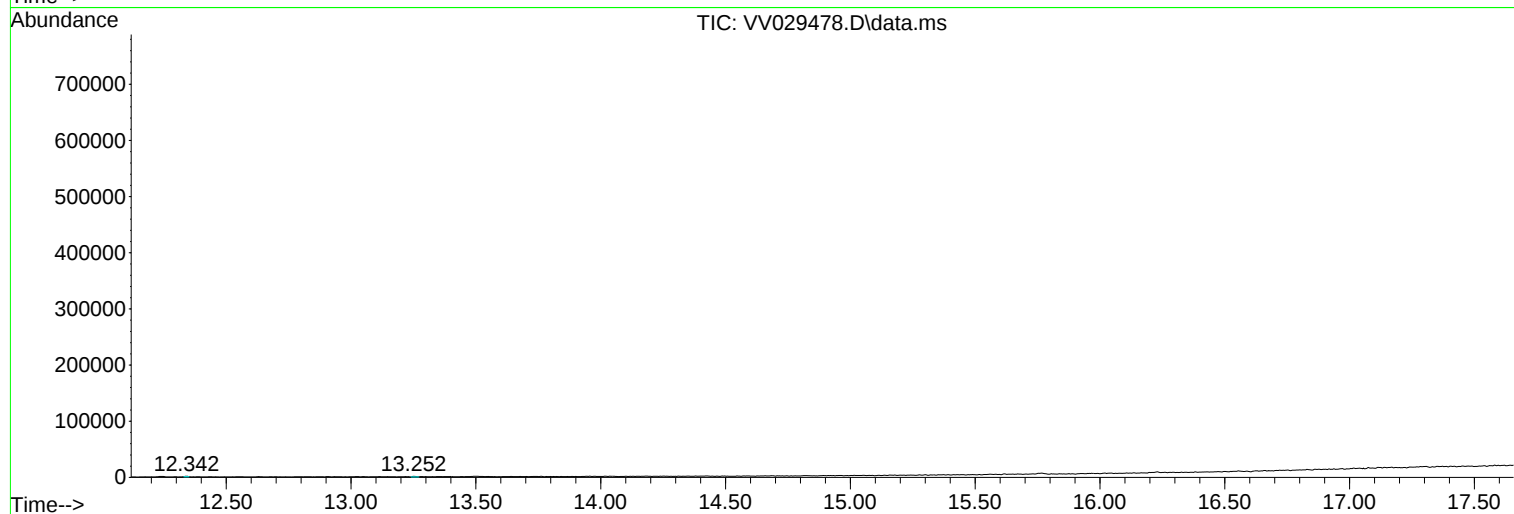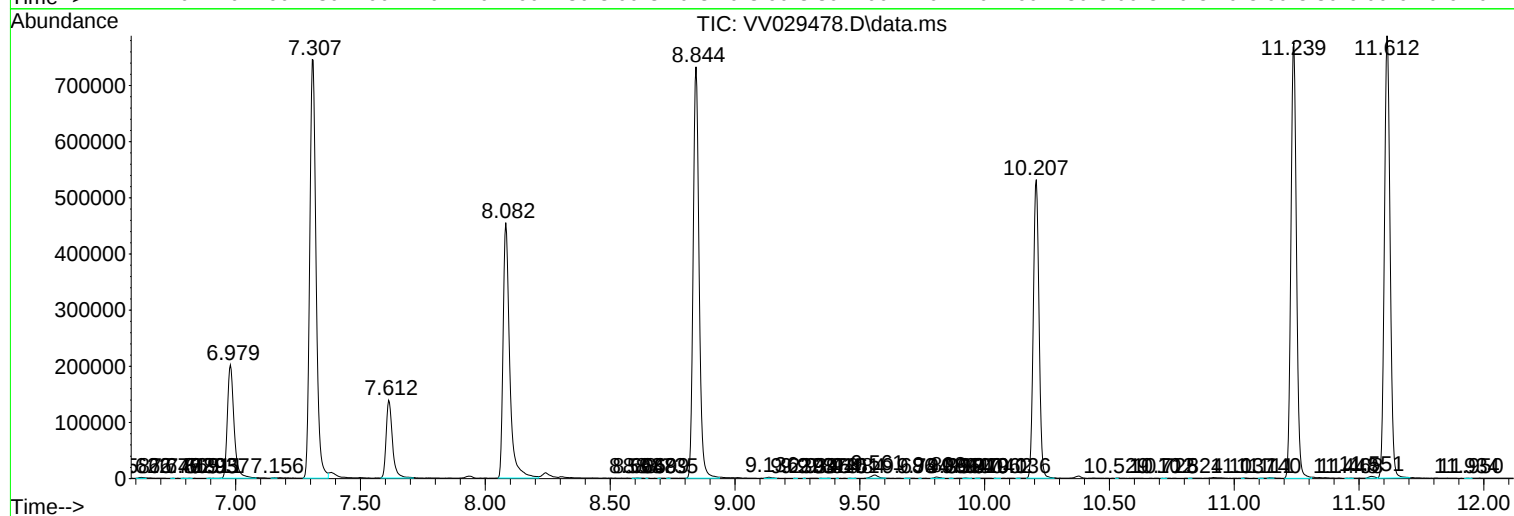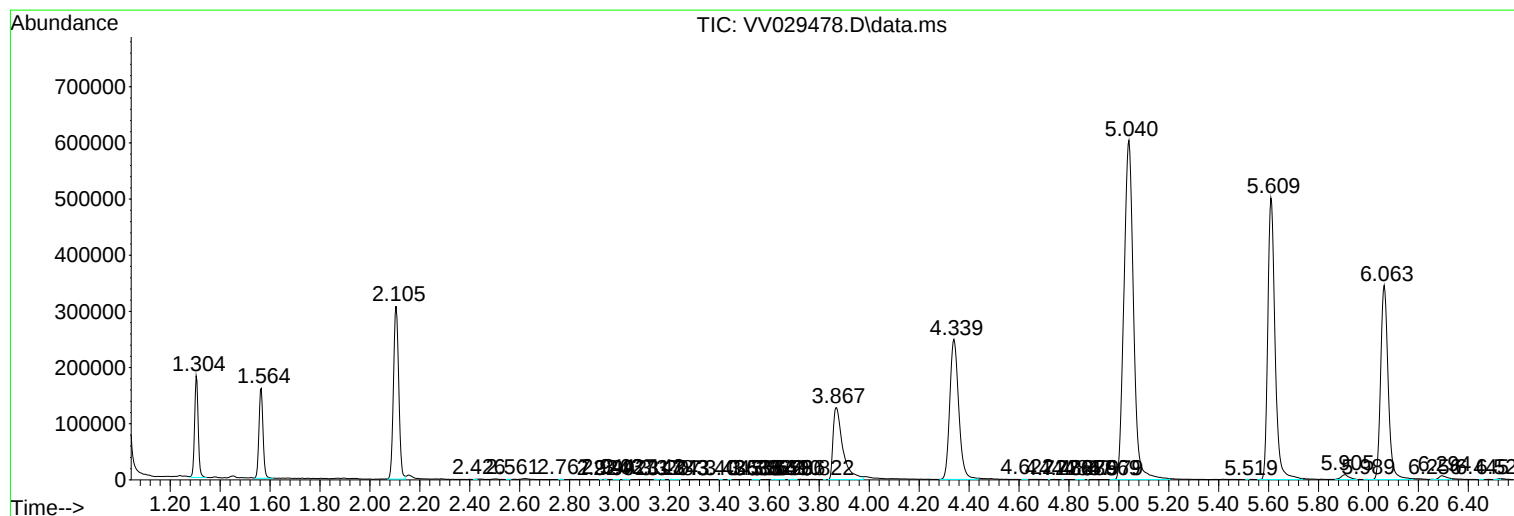

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
Data File : VV029478.D
Acq On : 08 Dec 2022 17:24
Operator : SY/MD
Sample : N5920-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EJ2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
Data File : VV029478.D
Acq On : 08 Dec 2022 17:24
Operator : SY/MD
Sample : N5920-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EJ2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------