

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
 Data File : VV029479.D
 Acq On : 08 Dec 2022 17:47
 Operator : SY/MD
 Sample : N5920-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EJ4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029479.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	99	rVB	179409	182100	4.94%	1.126%
2	1.564	155	163	181	rVB	157280	177969	4.83%	1.100%
3	1.873	253	259	269	rVB3	3351	4903	0.13%	0.030%
4	2.108	320	332	346	rBV2	359152	588539	15.97%	3.638%
5	2.272	376	383	399	rVB3	5382	10738	0.29%	0.066%
6	2.503	448	455	462	rVV	1286	1733	0.05%	0.011%
7	2.622	485	492	495	rBV4	796	1035	0.03%	0.006%
8	2.764	528	536	548	rVB4	1977	3424	0.09%	0.021%
9	2.854	559	564	568	rVB3	347	256	0.01%	0.002%
10	2.963	596	598	602	rVB3	438	223	0.01%	0.001%
11	3.143	649	654	655	rVV2	298	254	0.01%	0.002%
12	3.182	655	666	680	rVV2	3086	6424	0.17%	0.040%
13	3.391	728	731	742	rVB2	170	293	0.01%	0.002%
14	3.436	742	745	749	rBV3	283	267	0.01%	0.002%
15	3.667	812	817	823	rBV2	185	222	0.01%	0.001%
16	3.873	865	881	884	rBV	133774	236650	6.42%	1.463%
17	4.339	1009	1026	1056	rBV	239088	595628	16.16%	3.682%
18	4.603	1090	1108	1127	rBV2	56918	145390	3.94%	0.899%
19	4.725	1143	1146	1149	rBV3	289	229	0.01%	0.001%
20	4.789	1160	1166	1169	rBV	363	314	0.01%	0.002%
21	5.040	1226	1244	1287	rBV2	576780	1522596	41.31%	9.413%
22	5.394	1351	1354	1357	rBV2	363	243	0.01%	0.002%
23	5.609	1408	1421	1468	rBV	522130	1058195	28.71%	6.542%
24	5.905	1498	1513	1549	rBV	1870745	3685727	100.00%	22.786%
25	6.063	1549	1562	1592	rVB	330367	682960	18.53%	4.222%
26	6.326	1639	1644	1648	rBV5	470	440	0.01%	0.003%
27	6.455	1681	1684	1687	rVV2	350	238	0.01%	0.001%
28	6.616	1726	1734	1735	rBV4	1150	1094	0.03%	0.007%
29	6.751	1774	1776	1779	rBV2	312	250	0.01%	0.002%
30	6.886	1811	1818	1822	rVB3	297	363	0.01%	0.002%
31	6.915	1822	1827	1828	rBV2	250	206	0.01%	0.001%
32	6.979	1832	1847	1873	rBV	192804	355229	9.64%	2.196%
33	7.143	1895	1898	1900	rBV	473	387	0.01%	0.002%
34	7.166	1900	1905	1906	rVV3	565	503	0.01%	0.003%
35	7.307	1936	1949	1978	rBV	701169	1252476	33.98%	7.743%
36	7.612	2034	2044	2076	rVV	133072	234052	6.35%	1.447%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120822\
 Data File : VW029479.D
 Acq On : 08 Dec 2022 17:47
 Operator : SY/MD
 Sample : N5920-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EJ4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	7.838	2106	2114	2123	rVB4	2354	3776	0.10%	0.023%
38	7.876	2123	2126	2129	rBV2	284	274	0.01%	0.002%
39	7.931	2134	2143	2151	rBV4	3139	5659	0.15%	0.035%
40	8.082	2177	2190	2225	rBV	429481	786676	21.34%	4.863%
41	8.506	2320	2322	2326	rBV3	255	208	0.01%	0.001%
42	8.529	2326	2329	2331	rVV3	287	209	0.01%	0.001%
43	8.555	2334	2337	2340	rBV2	474	341	0.01%	0.002%
44	8.606	2347	2353	2355	rBV4	382	396	0.01%	0.002%
45	8.677	2372	2375	2378	rBV	277	206	0.01%	0.001%
46	8.844	2414	2427	2457	rBV	765809	1247320	33.84%	7.711%
47	9.082	2497	2501	2504	rVB4	282	228	0.01%	0.001%
48	9.130	2511	2516	2517	rBV2	332	277	0.01%	0.002%
49	9.146	2519	2521	2525	rVB3	644	411	0.01%	0.003%
50	9.175	2525	2530	2533	rBV3	461	507	0.01%	0.003%
51	9.272	2551	2560	2564	rVB3	523	769	0.02%	0.005%
52	9.445	2611	2614	2619	rBV3	301	357	0.01%	0.002%
53	9.532	2637	2641	2643	rBV2	435	301	0.01%	0.002%
54	9.641	2671	2675	2679	rVV3	348	262	0.01%	0.002%
55	9.767	2709	2714	2718	rBV3	260	266	0.01%	0.002%
56	9.844	2735	2738	2742	rVB4	457	282	0.01%	0.002%
57	9.921	2756	2762	2763	rBV3	474	353	0.01%	0.002%
58	10.095	2811	2816	2820	rBV2	244	223	0.01%	0.001%
59	10.207	2838	2851	2871	rBV	511494	811214	22.01%	5.015%
60	10.371	2895	2902	2913	rVB3	3492	6188	0.17%	0.038%
61	10.413	2913	2915	2919	rBV2	292	229	0.01%	0.001%
62	10.455	2925	2928	2936	rVB3	411	449	0.01%	0.003%
63	10.487	2936	2938	2942	rBV2	379	257	0.01%	0.002%
64	10.529	2948	2951	2957	rBV4	671	733	0.02%	0.005%
65	10.599	2969	2973	2977	rBV3	331	398	0.01%	0.002%
66	10.638	2981	2985	2989	rBV3	278	270	0.01%	0.002%
67	10.667	2989	2994	2997	rVB3	313	273	0.01%	0.002%
68	10.735	3010	3015	3019	rVB	329	296	0.01%	0.002%
69	10.757	3019	3022	3027	rBV3	205	237	0.01%	0.001%
70	10.841	3046	3048	3053	rBV2	302	221	0.01%	0.001%
71	10.882	3059	3061	3064	rVB2	398	213	0.01%	0.001%
72	10.908	3064	3069	3073	rBV5	856	824	0.02%	0.005%
73	11.005	3096	3099	3105	rVB2	404	309	0.01%	0.002%
74	11.111	3128	3132	3139	rVV2	470	454	0.01%	0.003%
75	11.156	3143	3146	3149	rBV3	377	236	0.01%	0.001%
76	11.178	3149	3153	3158	rVB4	778	729	0.02%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120822\
 Data File : VW029479.D
 Acq On : 08 Dec 2022 17:47
 Operator : SY/MD
 Sample : N5920-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EJ4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	11.239	3159	3172	3191	rBV	828046	1291723	35.05%	7.986%
78	11.452	3232	3238	3245	rBV5	481	614	0.02%	0.004%
79	11.554	3262	3270	3276	rBV4	2538	4214	0.11%	0.026%
80	11.612	3276	3288	3311	rVV	785306	1245275	33.79%	7.698%
81	11.751	3329	3331	3336	rVB5	526	386	0.01%	0.002%
82	11.808	3347	3349	3352	rVB2	547	293	0.01%	0.002%
83	11.841	3356	3359	3365	rVB4	450	420	0.01%	0.003%
84	11.908	3374	3380	3383	rBV3	325	299	0.01%	0.002%
85	12.072	3428	3431	3433	rBV2	292	231	0.01%	0.001%
86	12.133	3448	3450	3453	rBV2	426	257	0.01%	0.002%
87	12.214	3471	3475	3477	rBV2	283	240	0.01%	0.001%
88	12.243	3477	3484	3490	rVB4	877	1373	0.04%	0.008%
89	12.397	3529	3532	3535	rBV2	301	240	0.01%	0.001%
90	12.802	3653	3658	3660	rBV2	458	390	0.01%	0.002%
91	12.976	3710	3712	3721	rVB3	431	483	0.01%	0.003%
92	13.030	3728	3729	3732	rBV3	371	237	0.01%	0.001%
93	13.255	3793	3799	3800	rBV3	536	537	0.01%	0.003%
94	13.496	3868	3874	3877	rBV4	639	598	0.02%	0.004%
95	13.603	3903	3907	3910	rBV3	426	475	0.01%	0.003%
96	13.619	3910	3912	3918	rVV5	491	463	0.01%	0.003%
97	13.673	3927	3929	3934	rVB2	514	326	0.01%	0.002%
98	13.828	3973	3977	3984	rBV5	643	905	0.02%	0.006%
99	13.905	3996	4001	4003	rBV3	538	544	0.01%	0.003%
100	14.223	4098	4100	4107	rBV7	776	728	0.02%	0.005%




Sum of corrected areas: 16175632

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
Data File : VV029479.D
Acq On : 08 Dec 2022 17:47
Operator : SY/MD
Sample : N5920-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EJ4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

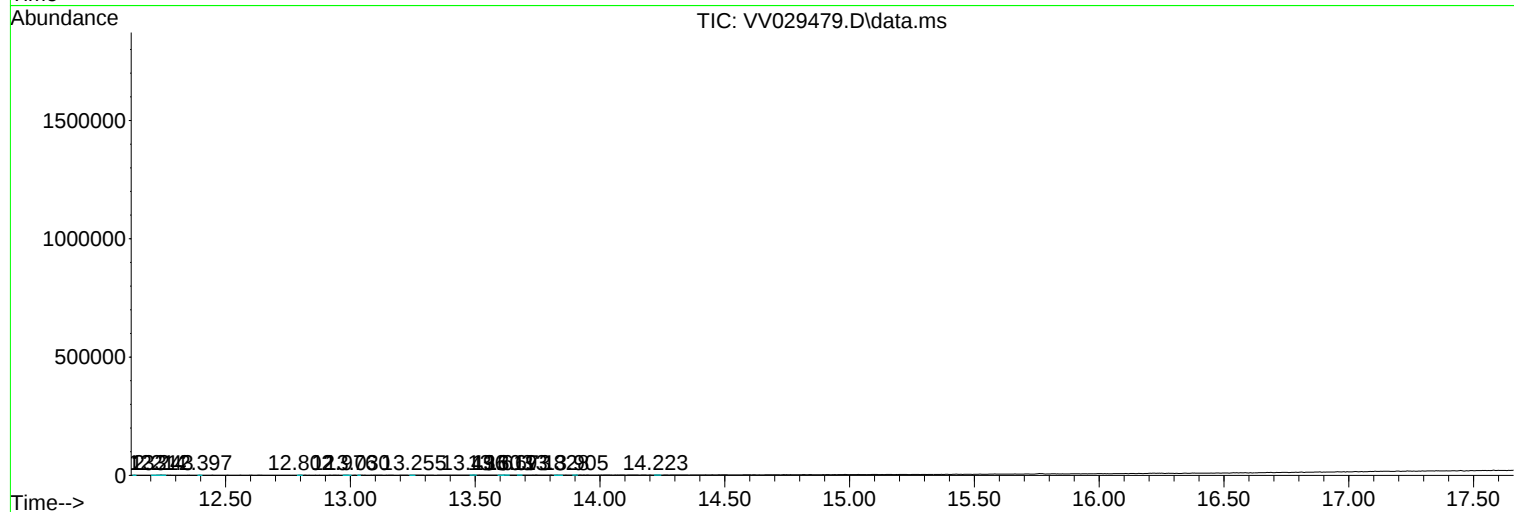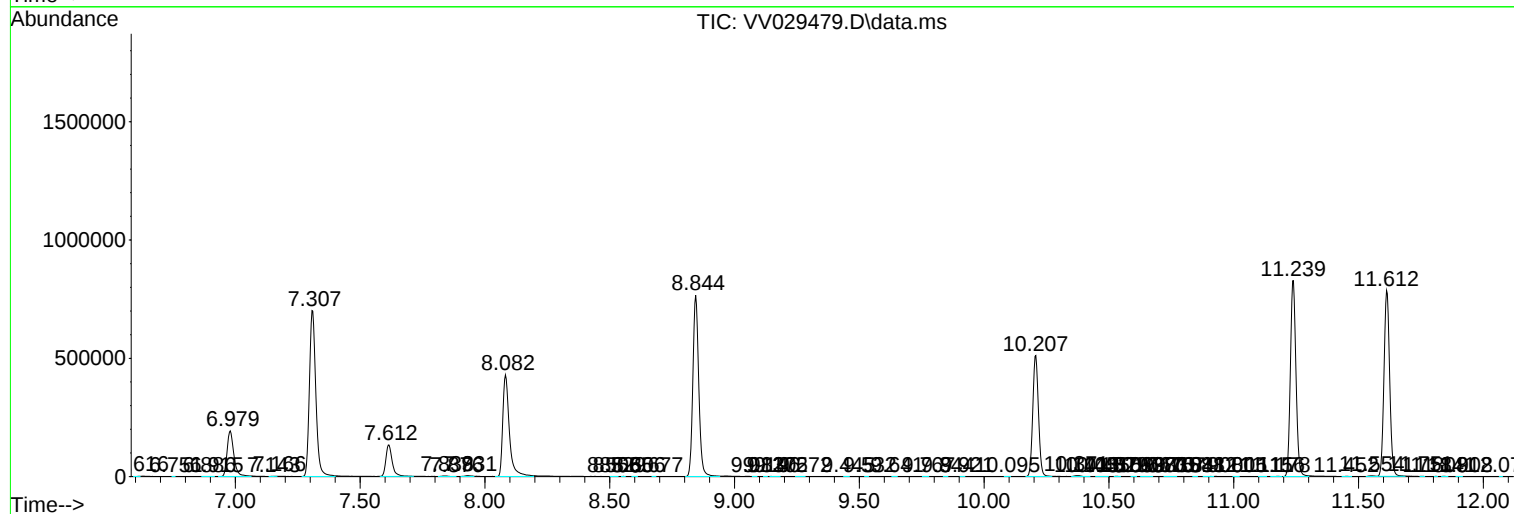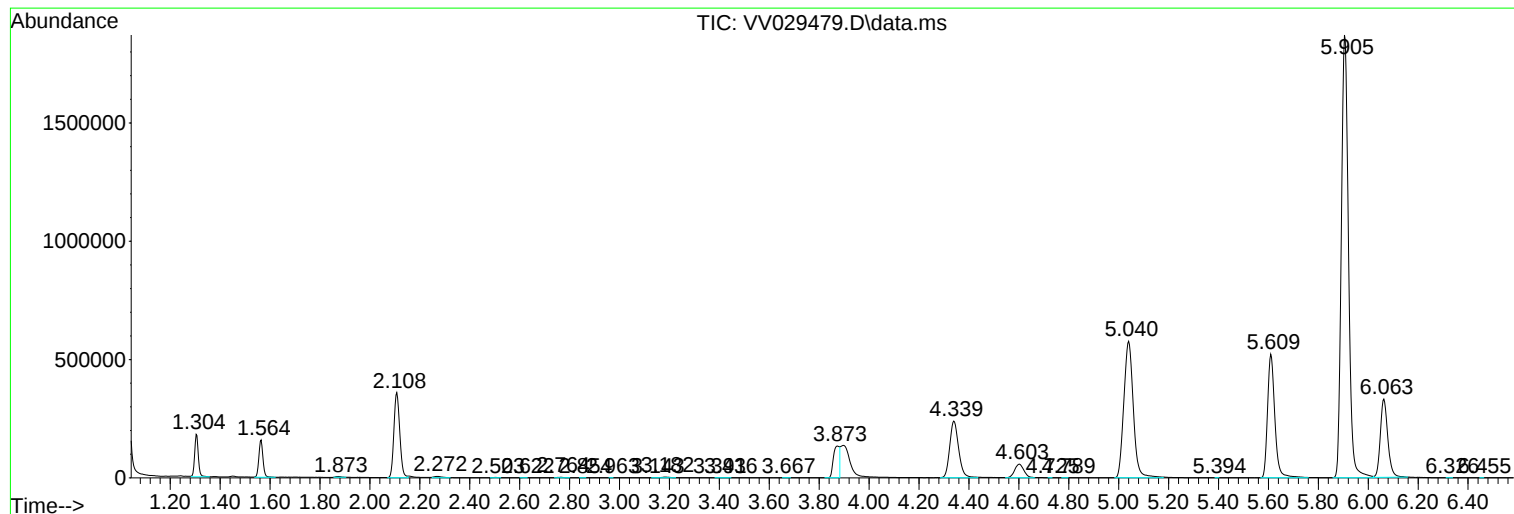

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
Data File : VV029479.D
Acq On : 08 Dec 2022 17:47
Operator : SY/MD
Sample : N5920-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EJ4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
Data File : VV029479.D
Acq On : 08 Dec 2022 17:47
Operator : SY/MD
Sample : N5920-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EJ4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------