

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
 Data File : VV029480.D
 Acq On : 08 Dec 2022 18:11
 Operator : SY/MD
 Sample : N5920-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EJ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029480.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	95	rVB	173477	168207	11.59%	1.437%
2	1.564	155	163	175	rVB	146507	164060	11.31%	1.401%
3	2.105	320	331	344	rBV	282716	408037	28.13%	3.485%
4	2.503	448	455	464	rVB6	1345	2124	0.15%	0.018%
5	2.571	473	476	477	rBV	229	146	0.01%	0.001%
6	2.738	525	528	531	rBV2	224	154	0.01%	0.001%
7	2.815	549	552	555	rVB	326	206	0.01%	0.002%
8	2.841	555	560	563	rBV2	304	295	0.02%	0.003%
9	2.934	585	589	593	rBV	127	136	0.01%	0.001%
10	2.953	593	595	598	rBV2	226	129	0.01%	0.001%
11	3.037	619	621	624	rVB2	211	105	0.01%	0.001%
12	3.317	705	708	714	rVB2	187	183	0.01%	0.002%
13	3.365	718	723	727	rBV	230	266	0.02%	0.002%
14	3.397	729	733	738	rVB2	428	291	0.02%	0.002%
15	3.423	738	741	744	rBV2	177	111	0.01%	0.001%
16	3.609	797	799	804	rVB2	255	146	0.01%	0.001%
17	3.686	818	823	825	rBV	121	107	0.01%	0.001%
18	3.722	830	834	837	rVV3	176	140	0.01%	0.001%
19	3.748	837	842	844	rBV2	130	132	0.01%	0.001%
20	3.867	870	879	916	rBV	118087	323324	22.29%	2.761%
21	4.339	1010	1026	1058	rBV2	227306	563804	38.86%	4.815%
22	4.600	1100	1107	1108	rBV3	788	786	0.05%	0.007%
23	4.654	1122	1124	1127	rVB2	285	131	0.01%	0.001%
24	4.674	1127	1130	1134	rBV3	330	276	0.02%	0.002%
25	4.735	1146	1149	1152	rBV2	286	203	0.01%	0.002%
26	4.834	1177	1180	1184	rVB2	339	230	0.02%	0.002%
27	4.860	1184	1188	1192	rVB	274	182	0.01%	0.002%
28	4.883	1192	1195	1196	rBV	278	153	0.01%	0.001%
29	4.966	1218	1221	1225	rBV	139	140	0.01%	0.001%
30	5.040	1225	1244	1274	rBV2	550059	1450693	100.00%	12.390%
31	5.397	1352	1355	1358	rBV3	363	263	0.02%	0.002%
32	5.413	1358	1360	1365	rVB4	316	196	0.01%	0.002%
33	5.471	1372	1378	1380	rBV	360	374	0.03%	0.003%
34	5.609	1407	1421	1465	rBV	505469	1046826	72.16%	8.941%
35	5.905	1503	1513	1530	rVB5	9647	22437	1.55%	0.192%
36	6.063	1548	1562	1592	rBV	316552	656611	45.26%	5.608%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120822\
 Data File : VW029480.D
 Acq On : 08 Dec 2022 18:11
 Operator : SY/MD
 Sample : N5920-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EJ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.288	1629	1632	1633	rBV	216	108	0.01%	0.001%
38	6.323	1639	1643	1644	rBV2	289	128	0.01%	0.001%
39	6.374	1653	1659	1666	rBV2	413	597	0.04%	0.005%
40	6.439	1676	1679	1682	rBV2	206	123	0.01%	0.001%
41	6.509	1698	1701	1703	rBV2	213	125	0.01%	0.001%
42	6.545	1709	1712	1715	rVB	177	121	0.01%	0.001%
43	6.571	1715	1720	1722	rBV2	240	199	0.01%	0.002%
44	6.622	1729	1736	1738	rBV3	850	841	0.06%	0.007%
45	6.731	1767	1770	1773	rBV2	183	150	0.01%	0.001%
46	6.805	1789	1793	1797	rBV4	486	491	0.03%	0.004%
47	6.857	1806	1809	1812	rVB3	376	202	0.01%	0.002%
48	6.876	1813	1815	1819	rVB2	234	136	0.01%	0.001%
49	6.899	1819	1822	1826	rBV2	168	102	0.01%	0.001%
50	6.921	1826	1829	1830	rBV	173	102	0.01%	0.001%
51	6.979	1835	1847	1871	rBV	181328	333690	23.00%	2.850%
52	7.262	1931	1935	1937	rBV	399	262	0.02%	0.002%
53	7.310	1937	1950	1983	rBV	665354	1194604	82.35%	10.203%
54	7.612	2034	2044	2073	rBV	125412	221302	15.25%	1.890%
55	7.747	2083	2086	2088	rBV2	581	304	0.02%	0.003%
56	7.834	2110	2113	2117	rBV2	380	395	0.03%	0.003%
57	7.934	2134	2144	2158	rVB3	4051	7931	0.55%	0.068%
58	7.989	2158	2161	2164	rBV3	399	213	0.01%	0.002%
59	8.027	2170	2173	2176	rBV	356	291	0.02%	0.002%
60	8.082	2180	2190	2232	rBV	407823	753220	51.92%	6.433%
61	8.545	2331	2334	2336	rBV3	416	250	0.02%	0.002%
62	8.689	2376	2379	2381	rBV3	264	189	0.01%	0.002%
63	8.773	2403	2405	2410	rVB2	216	163	0.01%	0.001%
64	8.844	2414	2427	2455	rBV	752433	1228639	84.69%	10.493%
65	9.107	2506	2509	2514	rBV2	424	345	0.02%	0.003%
66	9.127	2514	2515	2519	rBV3	495	322	0.02%	0.003%
67	9.165	2524	2527	2528	rBV2	306	166	0.01%	0.001%
68	9.185	2532	2533	2536	rVV	345	211	0.01%	0.002%
69	9.217	2540	2543	2547	rVB4	247	176	0.01%	0.002%
70	9.278	2560	2562	2566	rVB2	284	99	0.01%	0.001%
71	9.368	2588	2590	2595	rVB2	276	204	0.01%	0.002%
72	9.400	2597	2600	2604	rBV2	165	131	0.01%	0.001%
73	9.448	2612	2615	2618	rVB2	253	169	0.01%	0.001%
74	9.535	2638	2642	2644	rBV	274	205	0.01%	0.002%
75	9.561	2648	2650	2653	rVB2	193	114	0.01%	0.001%
76	9.583	2653	2657	2659	rBV3	337	239	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
 Data File : VV029480.D
 Acq On : 08 Dec 2022 18:11
 Operator : SY/MD
 Sample : N5920-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EJ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	9.622	2666	2669	2672	rBV2	243	195	0.01%	0.002%
78	9.699	2689	2693	2696	rBV2	323	243	0.02%	0.002%
79	9.751	2701	2709	2714	rBV2	335	482	0.03%	0.004%
80	9.808	2723	2727	2729	rBV	280	228	0.02%	0.002%
81	9.837	2733	2736	2738	rVV	256	175	0.01%	0.001%
82	9.853	2739	2741	2744	rVB2	326	157	0.01%	0.001%
83	9.934	2758	2766	2772	rBV4	618	743	0.05%	0.006%
84	10.207	2838	2851	2878	rVB	489383	773973	53.35%	6.610%
85	10.374	2894	2903	2913	rBV2	4948	8091	0.56%	0.069%
86	10.525	2945	2950	2951	rBV2	493	365	0.03%	0.003%
87	10.593	2968	2971	2980	rBV2	434	614	0.04%	0.005%
88	10.673	2990	2996	2997	rBV	213	145	0.01%	0.001%
89	10.844	3046	3049	3056	rBV3	616	465	0.03%	0.004%
90	10.886	3059	3062	3063	rBV	202	141	0.01%	0.001%
91	11.236	3158	3171	3202	rBV	785544	1225642	84.49%	10.468%
92	11.467	3240	3243	3246	rBV4	337	280	0.02%	0.002%
93	11.509	3253	3256	3257	rBV	428	215	0.01%	0.002%
94	11.551	3263	3269	3276	rBV3	2323	3264	0.22%	0.028%
95	11.612	3276	3288	3312	rVV	719248	1132639	78.08%	9.673%
96	11.905	3375	3379	3381	rBV	434	307	0.02%	0.003%
97	12.467	3550	3554	3556	rBV3	371	332	0.02%	0.003%
98	12.529	3570	3573	3578	rBV2	387	412	0.03%	0.004%
99	12.805	3657	3659	3661	rBV	396	160	0.01%	0.001%
100	13.631	3911	3916	3918	rBV3	641	561	0.04%	0.005%




Sum of corrected areas: 11708692

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
Data File : VV029480.D
Acq On : 08 Dec 2022 18:11
Operator : SY/MD
Sample : N5920-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EJ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

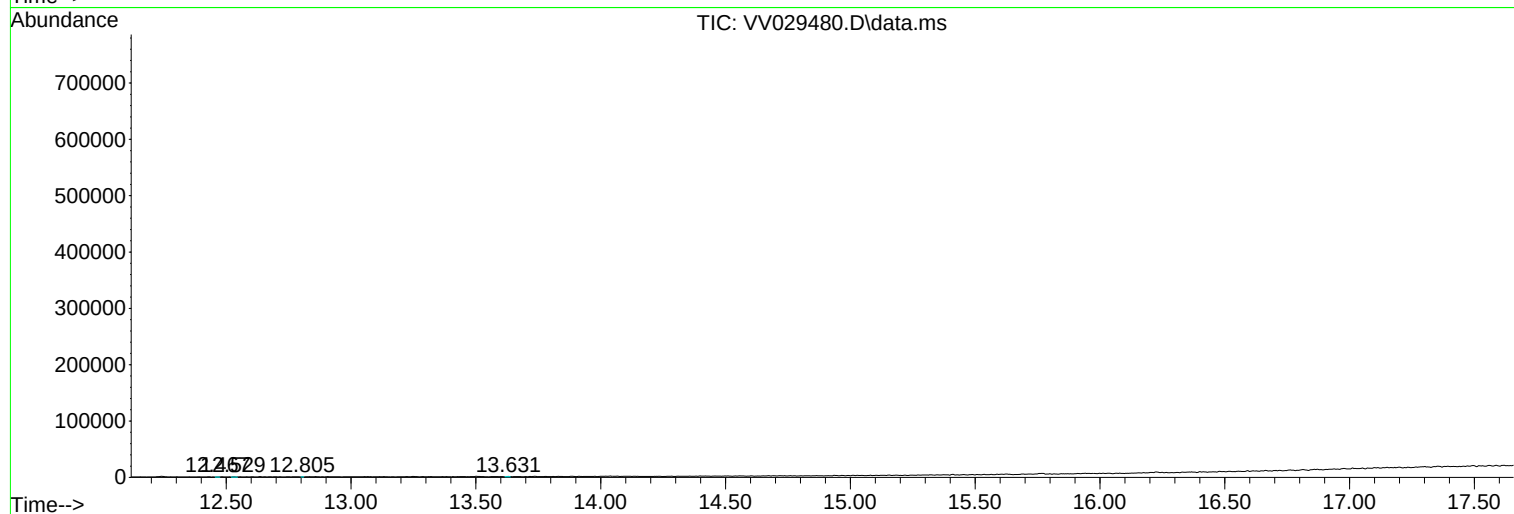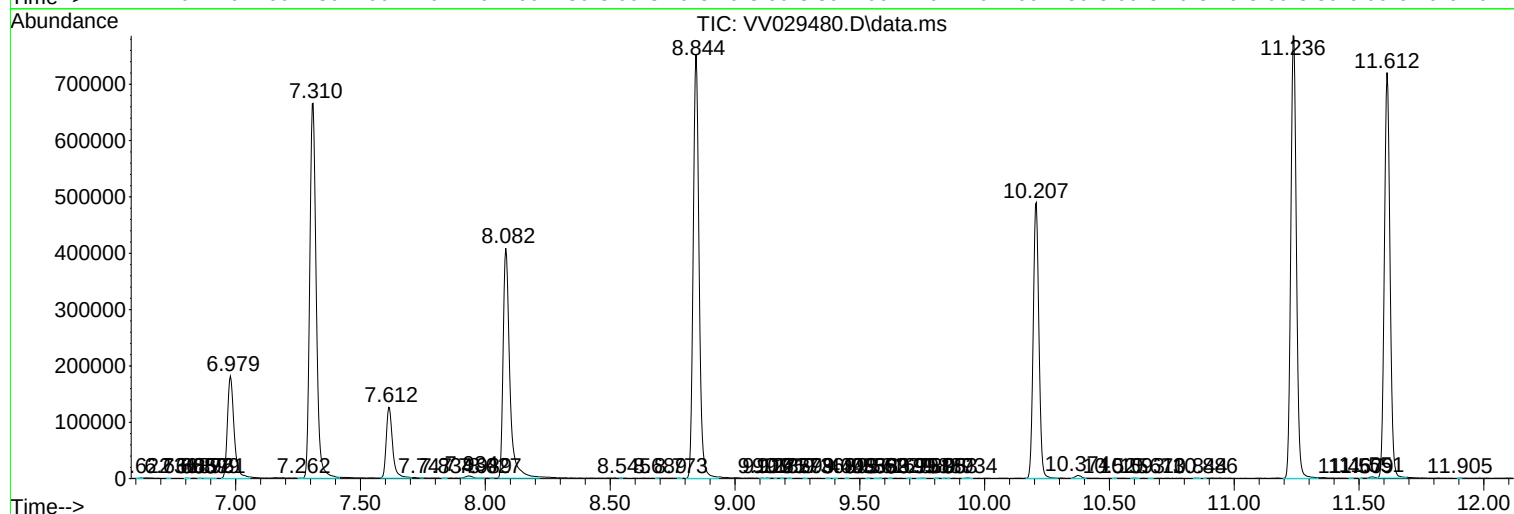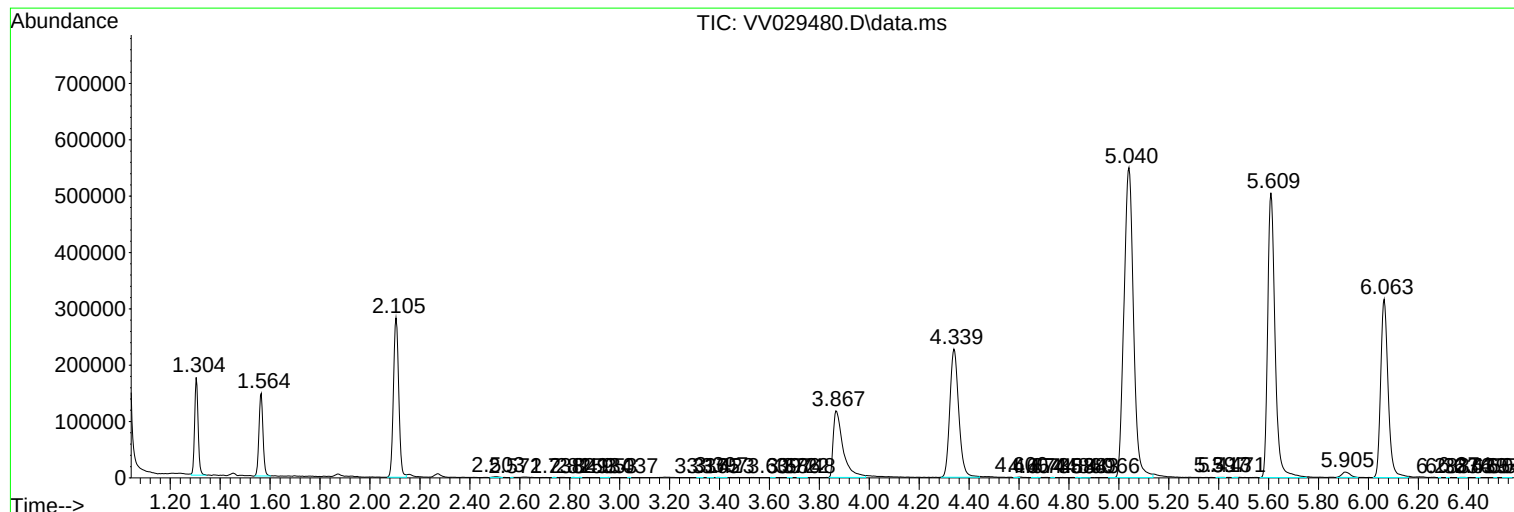

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
Data File : VV029480.D
Acq On : 08 Dec 2022 18:11
Operator : SY/MD
Sample : N5920-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EJ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
Data File : VV029480.D
Acq On : 08 Dec 2022 18:11
Operator : SY/MD
Sample : N5920-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EJ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------