

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120822\
 Data File : VW029482.D
 Acq On : 08 Dec 2022 18:58
 Operator : SY/MD
 Sample : N5920-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EJ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VW029482.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	100	rVB	172406	174858	11.28%	1.377%
2	1.564	156	163	177	rVB	153096	173580	11.20%	1.366%
3	2.105	320	331	343	rBV	294508	424112	27.37%	3.339%
4	2.503	449	455	462	rVB4	1261	1855	0.12%	0.015%
5	2.568	472	475	479	rBV	157	137	0.01%	0.001%
6	2.709	517	519	521	rBV	201	106	0.01%	0.001%
7	2.944	590	592	594	rBV	267	116	0.01%	0.001%
8	3.175	660	664	666	rBV	392	255	0.02%	0.002%
9	3.262	688	691	694	rBV2	304	186	0.01%	0.001%
10	3.497	762	764	766	rBV2	206	75	0.00%	0.001%
11	3.574	785	788	789	rBV2	231	134	0.01%	0.001%
12	3.629	802	805	810	rBV3	355	331	0.02%	0.003%
13	3.674	817	819	823	rVB	191	73	0.00%	0.001%
14	3.748	835	842	845	rBV2	257	283	0.02%	0.002%
15	3.767	845	848	853	rVB2	165	133	0.01%	0.001%
16	3.870	870	880	919	rBV	121697	331468	21.39%	2.609%
17	4.339	1010	1026	1067	rBV	241481	602327	38.87%	4.742%
18	4.635	1115	1118	1120	rBV	230	137	0.01%	0.001%
19	4.648	1120	1122	1124	rBV2	127	61	0.00%	0.000%
20	4.719	1142	1144	1147	rBV3	271	153	0.01%	0.001%
21	4.770	1157	1160	1164	rBV2	292	169	0.01%	0.001%
22	4.796	1167	1168	1171	rVB2	291	137	0.01%	0.001%
23	4.818	1172	1175	1178	rBV3	446	267	0.02%	0.002%
24	4.854	1183	1186	1190	rBV	242	204	0.01%	0.002%
25	4.963	1216	1220	1224	rBV2	357	270	0.02%	0.002%
26	5.040	1226	1244	1289	rBV2	585948	1549623	100.00%	12.199%
27	5.391	1350	1353	1356	rBV	392	320	0.02%	0.003%
28	5.445	1368	1370	1373	rBV2	118	65	0.00%	0.001%
29	5.551	1400	1403	1404	rBV	288	149	0.01%	0.001%
30	5.609	1408	1421	1465	rBV	569186	1168590	75.41%	9.200%
31	5.902	1502	1512	1513	rBV4	5154	6238	0.40%	0.049%
32	5.995	1540	1541	1547	rBV3	364	330	0.02%	0.003%
33	6.063	1548	1562	1599	rVV	335150	700683	45.22%	5.516%
34	6.323	1642	1643	1648	rBV2	244	158	0.01%	0.001%
35	6.342	1648	1649	1653	rVV2	202	125	0.01%	0.001%
36	6.375	1654	1659	1661	rVB3	421	270	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120822\
 Data File : VW029482.D
 Acq On : 08 Dec 2022 18:58
 Operator : SY/MD
 Sample : N5920-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EJ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.452	1680	1683	1687	rVV2	316	241	0.02%	0.002%
38	6.471	1687	1689	1691	rVV	161	100	0.01%	0.001%
39	6.497	1695	1697	1702	rVB	85	63	0.00%	0.000%
40	6.522	1702	1705	1707	rBV2	167	94	0.01%	0.001%
41	6.539	1707	1710	1713	rBV2	226	144	0.01%	0.001%
42	6.567	1713	1719	1723	rBV2	316	328	0.02%	0.003%
43	6.619	1728	1735	1739	rBV5	1359	1909	0.12%	0.015%
44	6.719	1764	1766	1768	rVB	283	77	0.00%	0.001%
45	6.748	1772	1775	1777	rBV	185	106	0.01%	0.001%
46	6.760	1777	1779	1786	rBV2	239	235	0.02%	0.002%
47	6.815	1794	1796	1798	rVB2	231	82	0.01%	0.001%
48	6.831	1798	1801	1806	rVB2	291	199	0.01%	0.002%
49	6.863	1806	1811	1814	rBV3	348	345	0.02%	0.003%
50	6.899	1817	1822	1826	rBV3	175	193	0.01%	0.002%
51	6.918	1826	1828	1833	rVB3	252	170	0.01%	0.001%
52	6.979	1833	1847	1880	rBV	191386	357667	23.08%	2.816%
53	7.307	1937	1949	1978	rBV	719493	1281056	82.67%	10.085%
54	7.612	2034	2044	2070	rBV	134178	236337	15.25%	1.861%
55	8.082	2180	2190	2227	rBV	433401	794782	51.29%	6.257%
56	8.471	2308	2311	2312	rBV	265	186	0.01%	0.001%
57	8.587	2344	2347	2350	rBV2	335	174	0.01%	0.001%
58	8.725	2386	2390	2394	rVB	440	433	0.03%	0.003%
59	8.747	2394	2397	2400	rBV3	556	420	0.03%	0.003%
60	8.760	2400	2401	2406	rVB2	468	266	0.02%	0.002%
61	8.844	2414	2427	2458	rBV	834245	1382908	89.24%	10.887%
62	9.091	2502	2504	2507	rVB2	349	178	0.01%	0.001%
63	9.108	2507	2509	2511	rBV2	212	108	0.01%	0.001%
64	9.181	2529	2532	2537	rVB3	338	237	0.02%	0.002%
65	9.207	2537	2540	2541	rBV	145	66	0.00%	0.001%
66	9.291	2562	2566	2569	rBV2	303	278	0.02%	0.002%
67	9.471	2619	2622	2626	rVB	375	250	0.02%	0.002%
68	9.493	2626	2629	2632	rBV3	238	233	0.02%	0.002%
69	9.558	2647	2649	2652	rVV	335	126	0.01%	0.001%
70	9.580	2654	2656	2660	rVB2	187	125	0.01%	0.001%
71	9.651	2671	2678	2681	rBV2	274	306	0.02%	0.002%
72	9.683	2686	2688	2689	rBV	222	96	0.01%	0.001%
73	9.812	2725	2728	2731	rBV2	494	373	0.02%	0.003%
74	9.870	2745	2746	2749	rBV2	208	118	0.01%	0.001%
75	9.982	2780	2781	2788	rVB2	179	101	0.01%	0.001%
76	10.088	2808	2814	2817	rBV2	360	399	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120822\
 Data File : VW029482.D
 Acq On : 08 Dec 2022 18:58
 Operator : SY/MD
 Sample : N5920-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EJ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.108	2817	2820	2825	rVB	323	275	0.02%	0.002%
78	10.207	2839	2851	2871	rVV	523720	825169	53.25%	6.496%
79	10.374	2896	2903	2913	rVB2	4829	8049	0.52%	0.063%
80	10.426	2916	2919	2921	rBV3	251	126	0.01%	0.001%
81	10.461	2926	2930	2932	rBV2	266	175	0.01%	0.001%
82	10.599	2970	2973	2975	rBV2	239	156	0.01%	0.001%
83	10.680	2995	2998	2999	rBV2	182	98	0.01%	0.001%
84	10.689	2999	3001	3002	rBV	556	233	0.02%	0.002%
85	10.815	3037	3040	3044	rBV2	227	187	0.01%	0.001%
86	10.834	3044	3046	3048	rBV	228	90	0.01%	0.001%
87	10.882	3056	3061	3063	rBV2	315	272	0.02%	0.002%
88	10.905	3064	3068	3073	rVV5	448	536	0.03%	0.004%
89	11.156	3142	3146	3149	rBV2	498	428	0.03%	0.003%
90	11.239	3159	3172	3200	rBV	923614	1439650	92.90%	11.333%
91	11.551	3263	3269	3275	rBV4	2007	2844	0.18%	0.022%
92	11.612	3277	3288	3314	rVB	781207	1216134	78.48%	9.574%
93	11.818	3350	3352	3355	rVB2	481	278	0.02%	0.002%
94	11.834	3355	3357	3360	rVB3	414	224	0.01%	0.002%
95	11.850	3360	3362	3363	rBV	180	60	0.00%	0.000%
96	11.863	3363	3366	3370	rVB3	453	415	0.03%	0.003%
97	11.995	3401	3407	3417	rVB3	1188	1662	0.11%	0.013%
98	12.451	3546	3549	3550	rBV	287	147	0.01%	0.001%
99	12.828	3663	3666	3667	rBV2	317	188	0.01%	0.001%
100	12.992	3709	3717	3724	rBV5	4048	5733	0.37%	0.045%




Sum of corrected areas: 12702616

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
Data File : VV029482.D
Acq On : 08 Dec 2022 18:58
Operator : SY/MD
Sample : N5920-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EJ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

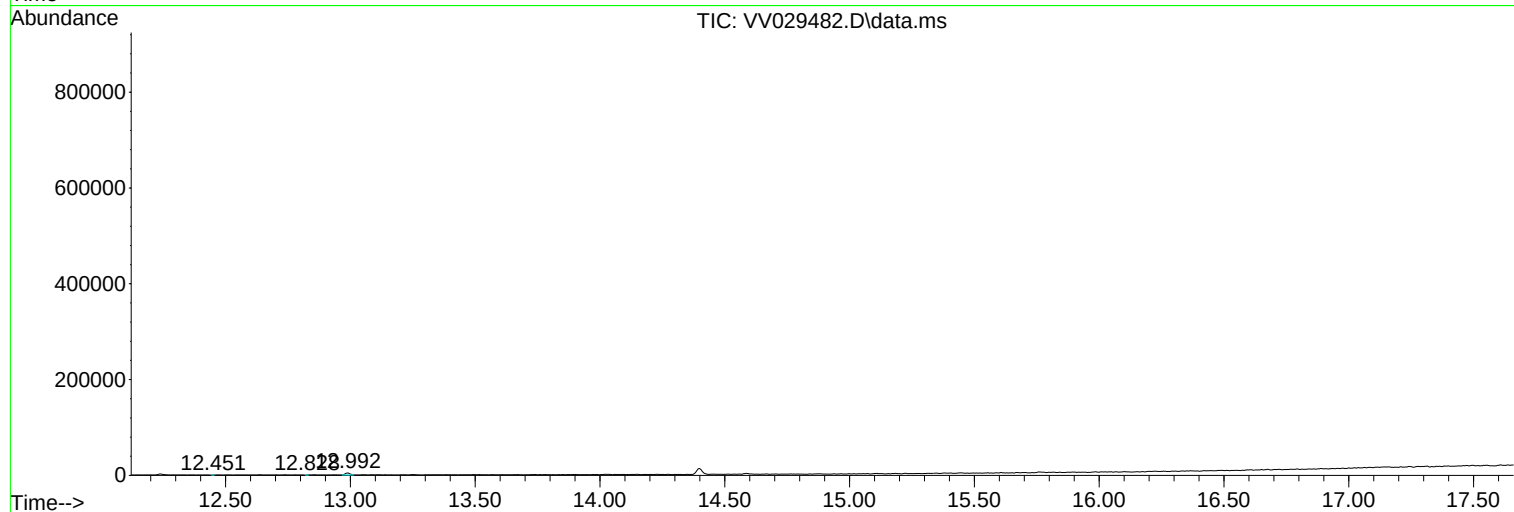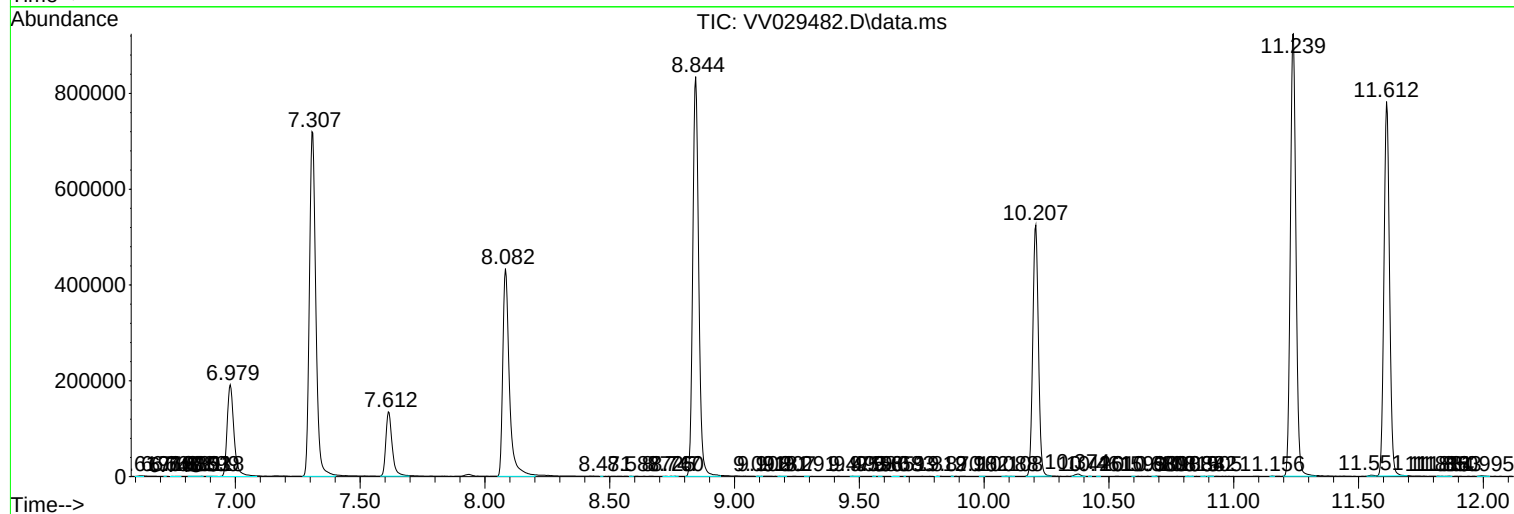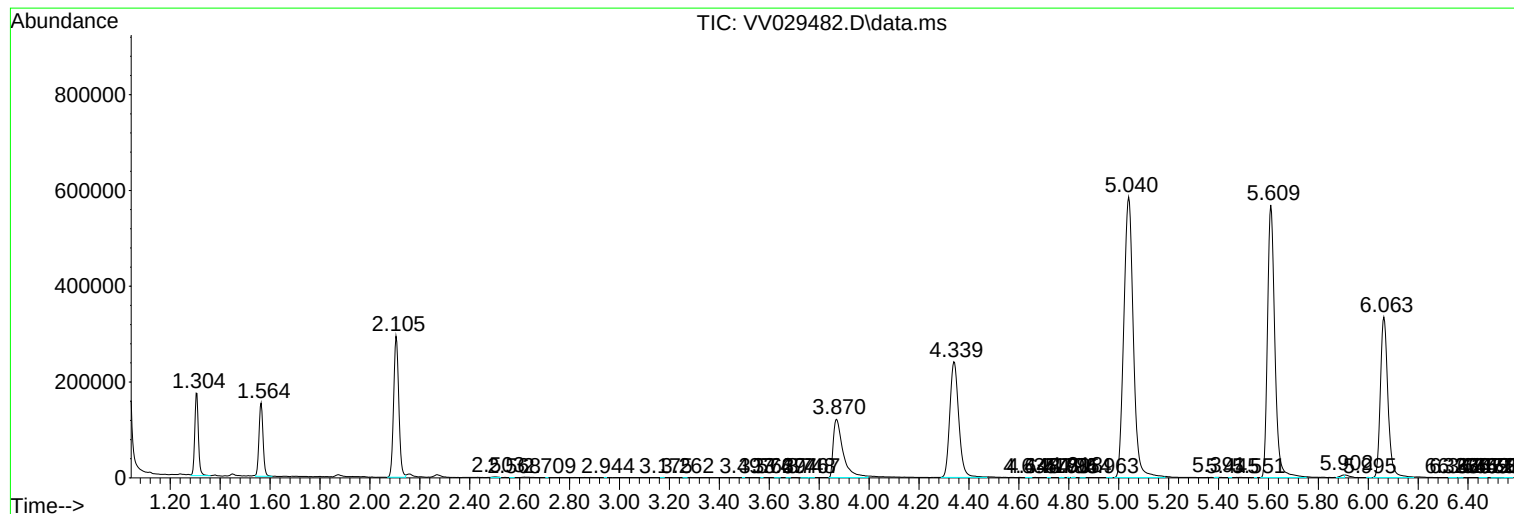

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
Data File : VV029482.D
Acq On : 08 Dec 2022 18:58
Operator : SY/MD
Sample : N5920-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EJ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
Data File : VV029482.D
Acq On : 08 Dec 2022 18:58
Operator : SY/MD
Sample : N5920-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EJ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------