

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
 Data File : VV029486.D
 Acq On : 08 Dec 2022 20:32
 Operator : SY/MD
 Sample : VV1208WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK302

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M

Title : VOC Analysis

Signal : TIC: VV029486.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	103	rVB	193158	192027	12.12%	1.472%
2	1.564	155	163	180	rVB	168576	189187	11.94%	1.450%
3	2.105	320	331	348	rBV	317249	456240	28.80%	3.497%
4	2.506	447	456	465	rVV	5299	8011	0.51%	0.061%
5	2.568	469	475	479	rVB3	383	414	0.03%	0.003%
6	2.587	479	481	482	rBV3	192	71	0.00%	0.001%
7	2.638	494	497	500	rBV2	148	118	0.01%	0.001%
8	2.658	500	503	509	rVB2	363	290	0.02%	0.002%
9	2.690	510	513	518	rBV4	243	194	0.01%	0.001%
10	2.741	526	529	530	rBV	219	124	0.01%	0.001%
11	2.850	559	563	568	rVB2	383	339	0.02%	0.003%
12	2.960	595	597	599	rBV	228	106	0.01%	0.001%
13	2.992	604	607	609	rBV	135	94	0.01%	0.001%
14	3.088	635	637	640	rVB	292	135	0.01%	0.001%
15	3.188	666	668	672	rVB	247	102	0.01%	0.001%
16	3.211	672	675	677	rBV	202	132	0.01%	0.001%
17	3.252	684	688	691	rBV2	160	136	0.01%	0.001%
18	3.307	701	705	709	rBV	134	117	0.01%	0.001%
19	3.330	710	712	715	rVV2	205	112	0.01%	0.001%
20	3.362	719	722	725	rBV2	142	102	0.01%	0.001%
21	3.400	731	734	737	rBV2	313	234	0.01%	0.002%
22	3.471	753	756	758	rBV2	171	97	0.01%	0.001%
23	3.490	759	762	763	rBV2	174	98	0.01%	0.001%
24	3.545	775	779	782	rBV2	244	161	0.01%	0.001%
25	3.703	824	828	829	rBV	157	74	0.00%	0.001%
26	3.715	830	832	834	rVB	190	83	0.01%	0.001%
27	3.770	845	849	854	rBV2	290	272	0.02%	0.002%
28	3.873	871	881	932	rBV	126871	374607	23.65%	2.872%
29	4.339	1010	1026	1054	rBV	247801	608933	38.44%	4.668%
30	4.548	1089	1091	1095	rBV2	452	271	0.02%	0.002%
31	4.567	1095	1097	1100	rVB2	316	172	0.01%	0.001%
32	4.632	1115	1117	1120	rBV3	519	342	0.02%	0.003%
33	4.937	1210	1212	1214	rBV	215	122	0.01%	0.001%
34	5.040	1224	1244	1276	rBV2	609894	1584269	100.00%	12.145%
35	5.461	1371	1375	1378	rBV3	350	324	0.02%	0.002%
36	5.609	1408	1421	1450	rBV	565835	1142562	72.12%	8.759%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
 Data File : VV029486.D
 Acq On : 08 Dec 2022 20:32
 Operator : SY/MD
 Sample : VV1208WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK302

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	5.905	1503	1513	1528	rVB9	6582	14230	0.90%	0.109%
38	6.063	1547	1562	1597	rBV	344252	716412	45.22%	5.492%
39	6.265	1623	1625	1628	rBV2	476	266	0.02%	0.002%
40	6.278	1628	1629	1632	rVB	442	148	0.01%	0.001%
41	6.304	1632	1637	1638	rBV2	197	121	0.01%	0.001%
42	6.371	1655	1658	1660	rBV2	186	79	0.00%	0.001%
43	6.381	1660	1661	1667	rVB2	257	244	0.02%	0.002%
44	6.416	1667	1672	1673	rBV2	232	178	0.01%	0.001%
45	6.426	1673	1675	1676	rBV	162	85	0.01%	0.001%
46	6.448	1680	1682	1685	rVV2	260	156	0.01%	0.001%
47	6.516	1701	1703	1706	rVB	208	67	0.00%	0.001%
48	6.548	1710	1713	1717	rBB2	205	115	0.01%	0.001%
49	6.574	1717	1721	1723	rBV2	166	136	0.01%	0.001%
50	6.587	1723	1725	1728	rVB3	188	113	0.01%	0.001%
51	6.628	1729	1738	1746	rBV4	1236	2513	0.16%	0.019%
52	6.728	1767	1769	1774	rVB2	200	154	0.01%	0.001%
53	6.792	1787	1789	1792	rVB2	348	229	0.01%	0.002%
54	6.815	1792	1796	1798	rBV2	375	225	0.01%	0.002%
55	6.834	1799	1802	1807	rVB3	340	314	0.02%	0.002%
56	6.860	1807	1810	1813	rBV2	172	148	0.01%	0.001%
57	6.905	1823	1824	1826	rBV	240	102	0.01%	0.001%
58	6.979	1835	1847	1877	rBV	195998	363169	22.92%	2.784%
59	7.310	1936	1950	1983	rBV	740204	1307125	82.51%	10.020%
60	7.616	2034	2045	2073	rBV	134716	239429	15.11%	1.835%
61	8.085	2180	2191	2227	rBV	466075	852594	53.82%	6.536%
62	8.554	2335	2337	2338	rBV	221	70	0.00%	0.001%
63	8.564	2338	2340	2342	rVV2	340	108	0.01%	0.001%
64	8.664	2368	2371	2374	rBV	217	163	0.01%	0.001%
65	8.844	2415	2427	2455	rBV	813874	1353371	85.43%	10.375%
66	9.133	2512	2517	2518	rBV5	742	560	0.04%	0.004%
67	9.178	2526	2531	2536	rVB3	385	386	0.02%	0.003%
68	9.201	2536	2538	2539	rBV3	276	149	0.01%	0.001%
69	9.275	2559	2561	2562	rBV2	206	78	0.00%	0.001%
70	9.429	2602	2609	2615	rBB4	364	549	0.03%	0.004%
71	9.455	2615	2617	2620	rVB2	157	99	0.01%	0.001%
72	9.480	2620	2625	2628	rBV	314	365	0.02%	0.003%
73	9.644	2673	2676	2682	rVB3	336	313	0.02%	0.002%
74	9.677	2682	2686	2690	rBV3	207	225	0.01%	0.002%
75	9.760	2709	2712	2714	rBV	205	146	0.01%	0.001%
76	9.773	2714	2716	2719	rVV2	280	174	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
 Data File : VV029486.D
 Acq On : 08 Dec 2022 20:32
 Operator : SY/MD
 Sample : VV1208WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK302

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	9.818	2725	2730	2731	rBV	114	107	0.01%	0.001%
78	9.834	2731	2735	2740	rVV	8396	6038	0.38%	0.046%
79	9.956	2770	2773	2774	rBV	180	106	0.01%	0.001%
80	9.979	2777	2780	2785	rVV3	255	260	0.02%	0.002%
81	10.075	2807	2810	2815	rVB4	646	532	0.03%	0.004%
82	10.117	2821	2823	2824	rBV4	258	86	0.01%	0.001%
83	10.207	2839	2851	2869	rBV	536642	844562	53.31%	6.474%
84	10.374	2897	2903	2909	rBV5	553	632	0.04%	0.005%
85	10.506	2940	2944	2945	rBV	312	209	0.01%	0.002%
86	10.625	2979	2981	2984	rBV	211	95	0.01%	0.001%
87	10.644	2984	2987	2991	rVB3	301	206	0.01%	0.002%
88	10.664	2991	2993	2995	rBV	244	171	0.01%	0.001%
89	10.693	3000	3002	3005	rVB	286	143	0.01%	0.001%
90	10.754	3019	3021	3024	rBV2	234	125	0.01%	0.001%
91	10.792	3030	3033	3036	rVB2	281	161	0.01%	0.001%
92	10.908	3060	3069	3075	rBV3	1403	2094	0.13%	0.016%
93	11.111	3128	3132	3134	rBV2	218	181	0.01%	0.001%
94	11.172	3145	3151	3159	rBV5	1821	2671	0.17%	0.020%
95	11.239	3159	3172	3201	rBV	921660	1442576	91.06%	11.059%
96	11.503	3253	3254	3255	rBV	249	87	0.01%	0.001%
97	11.612	3276	3288	3317	rBV	829271	1309238	82.64%	10.036%
98	12.635	3601	3606	3615	rVB5	2945	3851	0.24%	0.030%
99	13.249	3791	3797	3808	rVB5	4395	6384	0.40%	0.049%
100	13.731	3941	3947	3957	rVB5	4914	8538	0.54%	0.065%


Sum of corrected areas: 13044833

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
Data File : VV029486.D
Acq On : 08 Dec 2022 20:32
Operator : SY/MD
Sample : VV1208WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK302

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

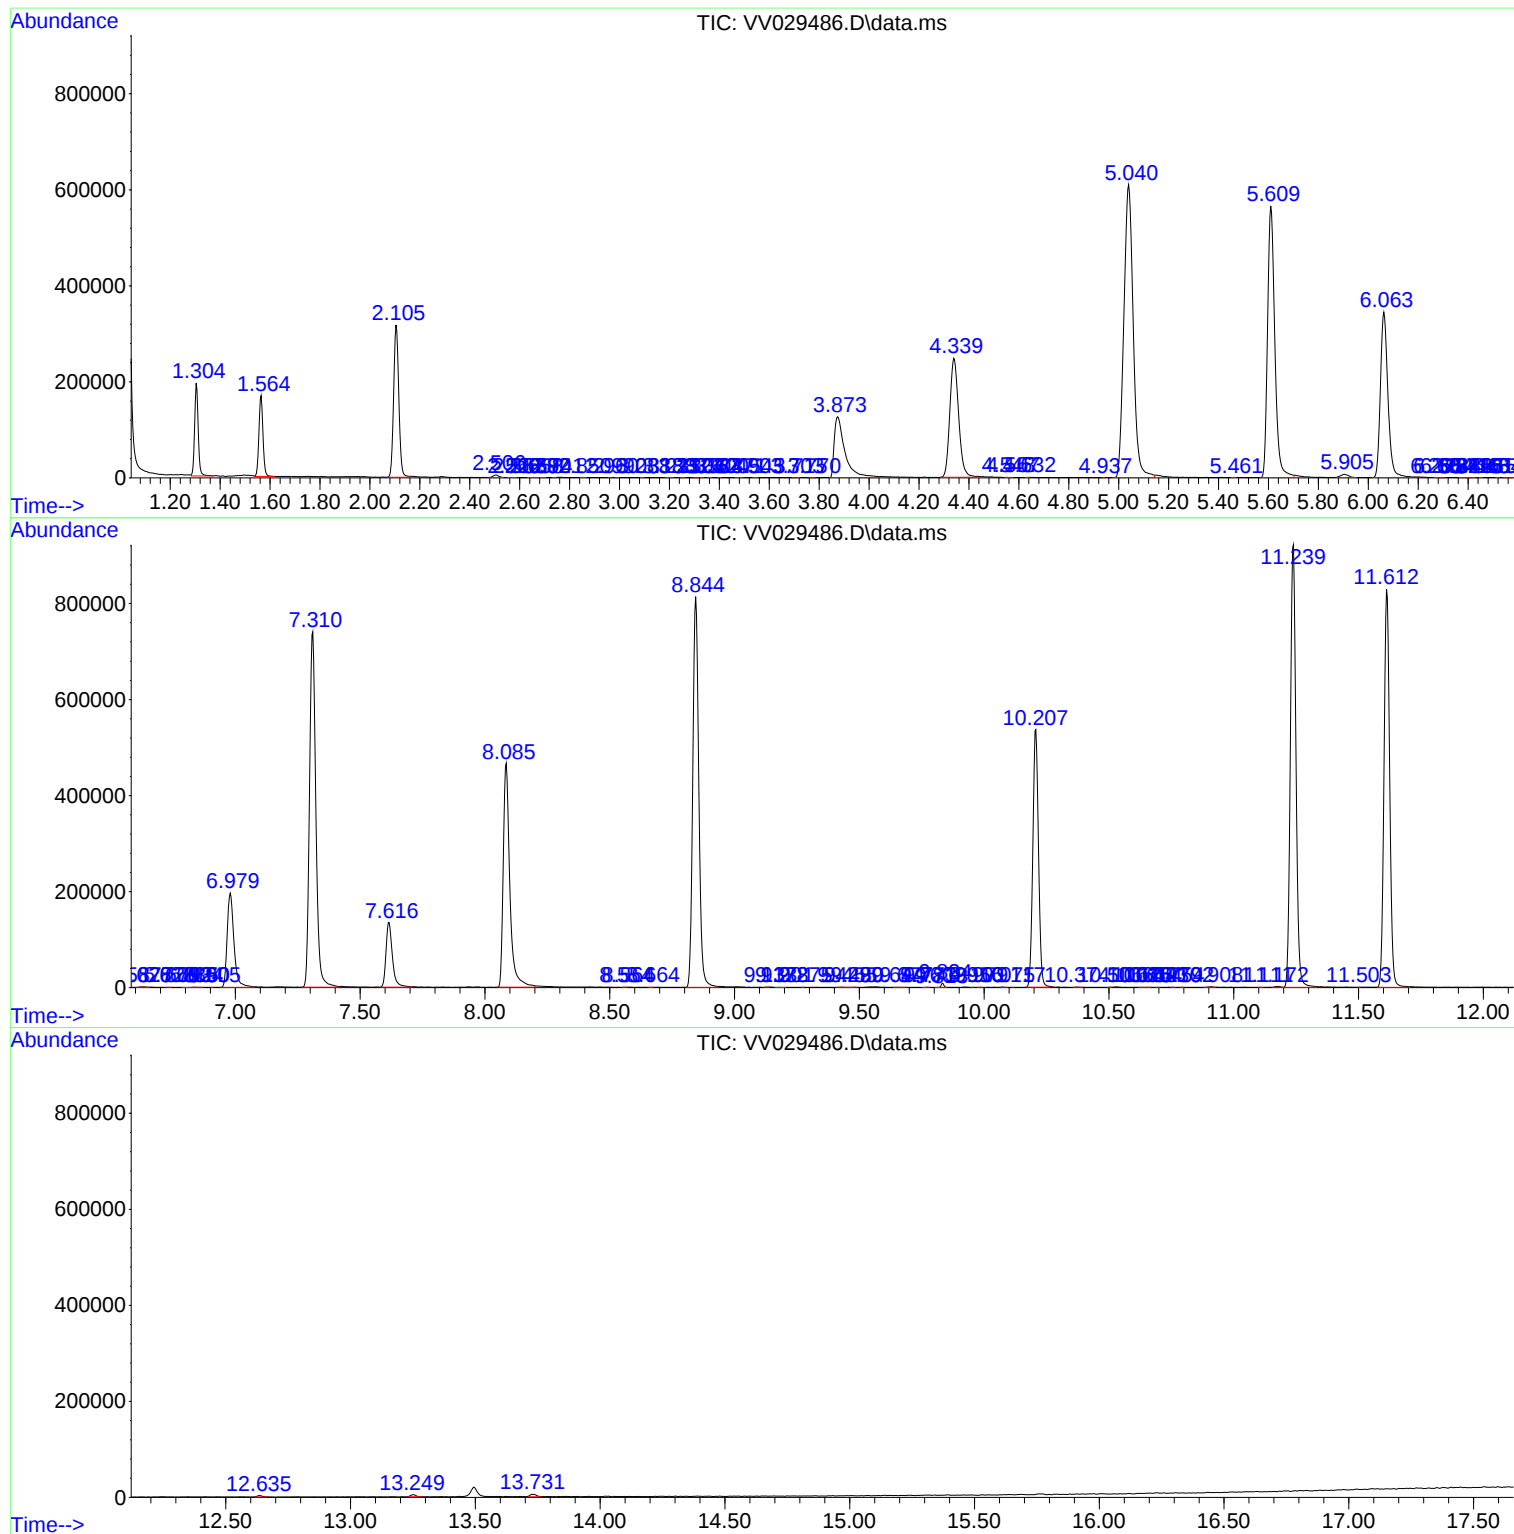

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
Data File : VV029486.D
Acq On : 08 Dec 2022 20:32
Operator : SY/MD
Sample : VV1208WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK302

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
Data File : VV029486.D
Acq On : 08 Dec 2022 20:32
Operator : SY/MD
Sample : VV1208WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK302

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------