

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
 Data File : VV029487.D
 Acq On : 08 Dec 2022 20:56
 Operator : SY/MD
 Sample : N5920-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EJ8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029487.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	96	rVB	175380	175148	11.25%	1.365%
2	1.564	155	163	178	rVB	157284	175188	11.26%	1.365%
3	2.105	319	331	348	rBV	302388	437775	28.13%	3.411%
4	2.265	379	381	383	rBV	445	237	0.02%	0.002%
5	2.288	383	388	396	rVB3	1481	2181	0.14%	0.017%
6	2.429	428	432	434	rBV3	445	264	0.02%	0.002%
7	2.497	449	453	455	rBV3	738	654	0.04%	0.005%
8	2.616	487	490	501	rVB3	956	1410	0.09%	0.011%
9	2.760	532	535	537	rBV	456	332	0.02%	0.003%
10	2.950	585	594	595	rBV4	839	775	0.05%	0.006%
11	3.172	659	663	664	rBV2	441	262	0.02%	0.002%
12	3.275	691	695	699	rVB2	213	200	0.01%	0.002%
13	3.635	805	807	812	rVB2	300	223	0.01%	0.002%
14	3.867	869	879	913	rBV	125582	335662	21.57%	2.615%
15	4.233	989	993	996	rBV4	417	352	0.02%	0.003%
16	4.339	1008	1026	1057	rBV	242779	603457	38.77%	4.702%
17	4.561	1093	1095	1098	rBV3	398	258	0.02%	0.002%
18	4.580	1098	1101	1103	rVB	333	203	0.01%	0.002%
19	4.603	1103	1108	1113	rBV3	281	275	0.02%	0.002%
20	4.664	1125	1127	1133	rVB3	313	268	0.02%	0.002%
21	4.754	1150	1155	1160	rVB2	494	367	0.02%	0.003%
22	4.895	1196	1199	1203	rVB2	352	294	0.02%	0.002%
23	5.040	1223	1244	1278	rBV2	587141	1556454	100.00%	12.127%
24	5.278	1316	1318	1324	rVB3	239	230	0.01%	0.002%
25	5.609	1407	1421	1463	rBV	557195	1146014	73.63%	8.929%
26	5.850	1494	1496	1501	rVB2	445	320	0.02%	0.002%
27	5.902	1501	1512	1528	rBV6	5539	12247	0.79%	0.095%
28	5.989	1534	1539	1542	rBV	391	308	0.02%	0.002%
29	6.063	1548	1562	1596	rBV	341932	705521	45.33%	5.497%
30	6.259	1621	1623	1627	rVB2	540	449	0.03%	0.003%
31	6.288	1627	1632	1636	rBV4	496	579	0.04%	0.005%
32	6.574	1719	1721	1725	rBV2	379	258	0.02%	0.002%
33	6.625	1728	1737	1740	rBV4	1247	1972	0.13%	0.015%
34	6.728	1765	1769	1773	rVB3	238	231	0.01%	0.002%
35	6.760	1773	1779	1783	rBV3	426	526	0.03%	0.004%
36	6.979	1833	1847	1876	rBV	196792	361955	23.26%	2.820%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120822\
 Data File : VW029487.D
 Acq On : 08 Dec 2022 20:56
 Operator : SY/MD
 Sample : N5920-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EJ8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	7.130	1892	1894	1896	rBV2	429	209	0.01%	0.002%
38	7.217	1917	1921	1925	rBV3	412	425	0.03%	0.003%
39	7.307	1936	1949	1982	rBV	729591	1299978	83.52%	10.128%
40	7.577	2029	2033	2034	rBV2	379	251	0.02%	0.002%
41	7.612	2034	2044	2069	rVV	134672	236653	15.20%	1.844%
42	7.805	2101	2104	2106	rBV	466	289	0.02%	0.002%
43	7.934	2132	2144	2154	rBV2	3556	6792	0.44%	0.053%
44	8.082	2178	2190	2226	rBV	442685	808489	51.94%	6.299%
45	8.448	2302	2304	2307	rVB3	548	252	0.02%	0.002%
46	8.545	2332	2334	2337	rBV3	333	235	0.02%	0.002%
47	8.690	2376	2379	2381	rVB	346	197	0.01%	0.002%
48	8.741	2391	2395	2402	rVB4	464	456	0.03%	0.004%
49	8.844	2412	2427	2458	rBV	811975	1352787	86.91%	10.540%
50	9.056	2489	2493	2495	rBV4	386	262	0.02%	0.002%
51	9.079	2497	2500	2504	rVB2	420	298	0.02%	0.002%
52	9.133	2512	2517	2523	rVV4	792	965	0.06%	0.008%
53	9.233	2545	2548	2551	rVB3	411	323	0.02%	0.003%
54	9.262	2553	2557	2560	rBV2	591	407	0.03%	0.003%
55	9.448	2612	2615	2618	rBV2	319	213	0.01%	0.002%
56	9.542	2640	2644	2647	rVV4	716	671	0.04%	0.005%
57	9.567	2649	2652	2656	rVB4	980	873	0.06%	0.007%
58	9.747	2701	2708	2711	rBV2	393	453	0.03%	0.004%
59	9.792	2718	2722	2724	rBV2	264	193	0.01%	0.002%
60	9.821	2726	2731	2733	rBV2	212	225	0.01%	0.002%
61	9.921	2755	2762	2772	rVB5	754	1246	0.08%	0.010%
62	9.992	2778	2784	2786	rBV2	370	414	0.03%	0.003%
63	10.207	2836	2851	2872	rBV	534037	837667	53.82%	6.526%
64	10.374	2895	2903	2912	rVV4	4020	6405	0.41%	0.050%
65	10.410	2912	2914	2918	rVV2	279	227	0.01%	0.002%
66	10.480	2932	2936	2943	rBV	299	447	0.03%	0.003%
67	10.535	2946	2953	2959	rVB3	627	1020	0.07%	0.008%
68	10.590	2965	2970	2973	rBV3	262	199	0.01%	0.002%
69	10.648	2983	2988	2991	rBV2	357	299	0.02%	0.002%
70	10.770	3022	3026	3028	rVB2	292	227	0.01%	0.002%
71	10.911	3062	3070	3075	rBV2	925	1295	0.08%	0.010%
72	11.088	3123	3125	3131	rVB3	282	236	0.02%	0.002%
73	11.169	3141	3150	3160	rBV4	1383	2493	0.16%	0.019%
74	11.236	3160	3171	3200	rBV	914549	1426891	91.68%	11.117%
75	11.484	3243	3248	3251	rBV2	241	269	0.02%	0.002%
76	11.551	3261	3269	3276	rBV4	3279	5360	0.34%	0.042%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
 Data File : VV029487.D
 Acq On : 08 Dec 2022 20:56
 Operator : SY/MD
 Sample : N5920-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EJ8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	11.612	3276	3288	3316	rVV	814152	1287364	82.71%	10.030%
78	11.828	3352	3355	3361	rVB4	461	355	0.02%	0.003%
79	11.860	3361	3365	3368	rBV2	425	334	0.02%	0.003%
80	11.876	3368	3370	3374	rVB2	326	219	0.01%	0.002%
81	12.091	3430	3437	3439	rBV	457	424	0.03%	0.003%
82	12.120	3443	3446	3450	rVV2	258	212	0.01%	0.002%
83	12.236	3477	3482	3488	rVV3	915	1074	0.07%	0.008%
84	12.284	3493	3497	3502	rBV3	251	259	0.02%	0.002%
85	12.374	3523	3525	3530	rVB3	337	230	0.01%	0.002%
86	12.439	3542	3545	3549	rBV2	292	229	0.01%	0.002%
87	12.496	3560	3563	3567	rBV3	355	290	0.02%	0.002%
88	12.541	3573	3577	3579	rBV3	431	250	0.02%	0.002%
89	12.638	3597	3607	3614	rBV5	1995	2857	0.18%	0.022%
90	12.709	3625	3629	3632	rBV2	468	348	0.02%	0.003%
91	12.998	3713	3719	3720	rBV3	351	343	0.02%	0.003%
92	13.056	3735	3737	3740	rBV2	393	334	0.02%	0.003%
93	13.082	3742	3745	3750	rBV3	515	436	0.03%	0.003%
94	13.249	3791	3797	3808	rVB6	2450	3826	0.25%	0.030%
95	13.368	3832	3834	3839	rVB4	498	313	0.02%	0.002%
96	13.419	3848	3850	3852	rBV2	445	197	0.01%	0.002%
97	13.500	3863	3875	3885	rBV	6272	10994	0.71%	0.086%
98	13.731	3942	3947	3957	rBV5	2452	3721	0.24%	0.029%
99	13.847	3981	3983	3986	rBV2	388	214	0.01%	0.002%
100	14.181	4083	4087	4089	rBV3	812	614	0.04%	0.005%

Sum of corrected areas: 12834877




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
Data File : VV029487.D
Acq On : 08 Dec 2022 20:56
Operator : SY/MD
Sample : N5920-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EJ8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

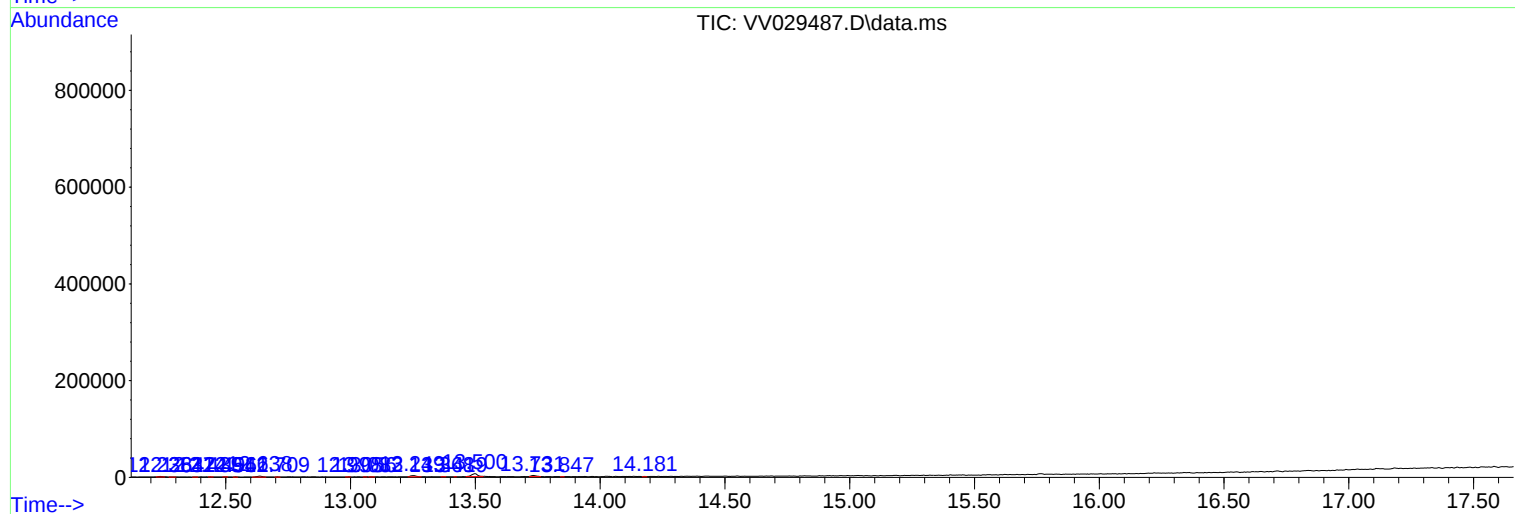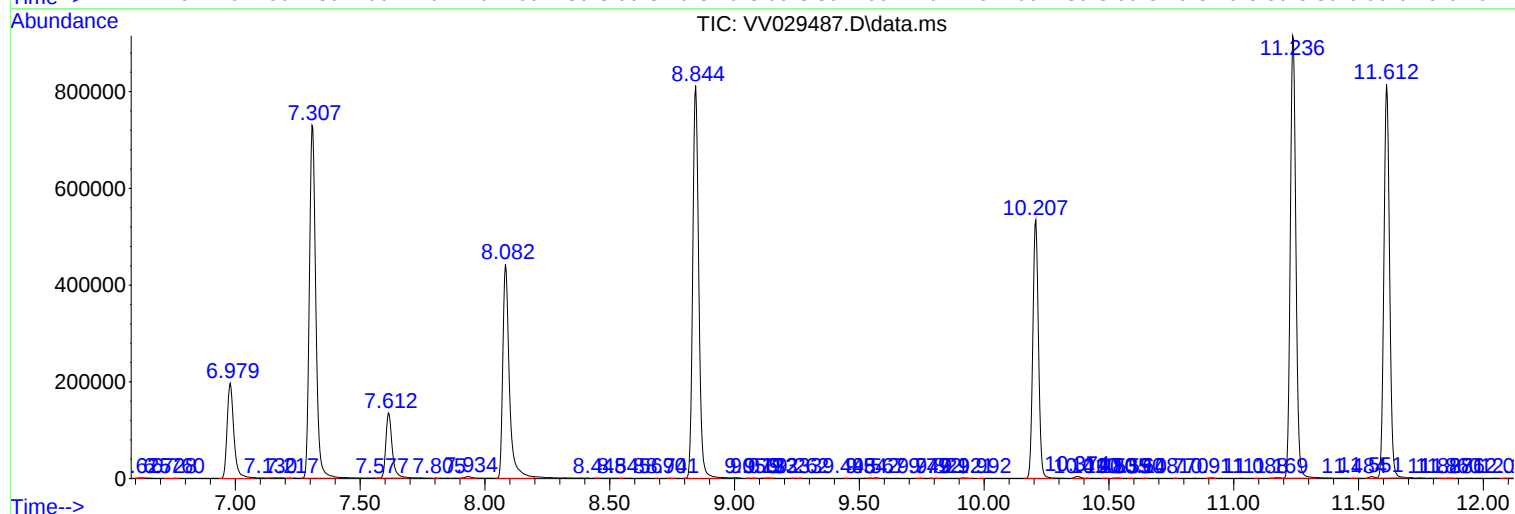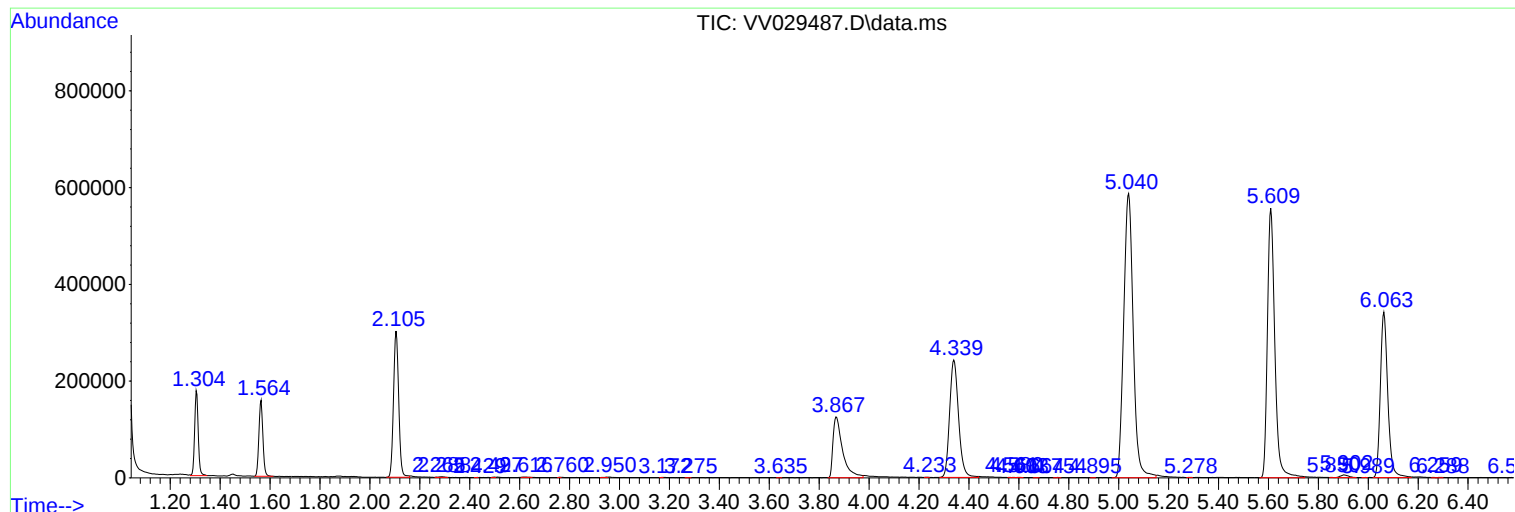

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
Data File : VV029487.D
Acq On : 08 Dec 2022 20:56
Operator : SY/MD
Sample : N5920-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EJ8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
Data File : VV029487.D
Acq On : 08 Dec 2022 20:56
Operator : SY/MD
Sample : N5920-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EJ8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc