

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
 Data File : VV029488.D
 Acq On : 08 Dec 2022 21:19
 Operator : SY/MD
 Sample : N5929-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ96

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029488.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	100	rVB	172490	172817	2.61%	0.644%
2	1.564	155	163	180	rVB	157295	179356	2.71%	0.669%
3	1.703	201	206	213	rVB	13009	14582	0.22%	0.054%
4	1.751	216	221	236	rVB3	19094	33360	0.50%	0.124%
5	2.114	320	334	359	rBV4	1258668	2001474	30.28%	7.460%
6	2.378	413	416	418	rBV2	347	234	0.00%	0.001%
7	2.413	424	427	429	rBV3	280	156	0.00%	0.001%
8	2.503	448	455	463	rBV5	1852	2807	0.04%	0.010%
9	2.555	469	471	472	rBV	264	121	0.00%	0.000%
10	2.654	499	502	507	rVB2	302	228	0.00%	0.001%
11	2.677	507	509	515	rVB2	181	151	0.00%	0.001%
12	2.706	515	518	521	rBV2	270	164	0.00%	0.001%
13	2.757	522	534	559	rVV	40986	74265	1.12%	0.277%
14	2.857	562	565	566	rBV	177	94	0.00%	0.000%
15	2.886	571	574	576	rBV2	248	159	0.00%	0.001%
16	2.953	593	595	599	rBV2	179	101	0.00%	0.000%
17	3.082	632	635	639	rVB2	261	138	0.00%	0.001%
18	3.182	650	666	691	rBV	914336	1911613	28.92%	7.125%
19	3.535	774	776	778	rBV	286	137	0.00%	0.001%
20	3.587	790	792	796	rVB	214	105	0.00%	0.000%
21	3.609	796	799	800	rBV	235	112	0.00%	0.000%
22	3.667	815	817	821	rVB	138	94	0.00%	0.000%
23	3.690	821	824	827	rBV2	95	76	0.00%	0.000%
24	3.706	827	829	833	rBV	179	113	0.00%	0.000%
25	3.780	849	852	853	rBV	171	72	0.00%	0.000%
26	3.902	870	890	932	rBV2	491619	1491699	22.57%	5.560%
27	4.339	1011	1026	1056	rBV	250900	641895	9.71%	2.393%
28	4.600	1086	1107	1142	rBV	2628586	6608906	100.00%	24.634%
29	5.040	1226	1244	1271	rBV2	582681	1531642	23.18%	5.709%
30	5.432	1363	1366	1370	rVB	320	222	0.00%	0.001%
31	5.455	1371	1373	1377	rVV3	315	187	0.00%	0.001%
32	5.484	1377	1382	1386	rVV3	400	403	0.01%	0.002%
33	5.506	1386	1389	1392	rVB2	262	151	0.00%	0.001%
34	5.609	1406	1421	1451	rBV	549933	1115155	16.87%	4.157%
35	5.908	1499	1514	1548	rBV	570141	1145002	17.33%	4.268%
36	6.063	1549	1562	1587	rVV	335910	686044	10.38%	2.557%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120822\
 Data File : VW029488.D
 Acq On : 08 Dec 2022 21:19
 Operator : SY/MD
 Sample : N5929-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ96

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.268	1624	1626	1631	rVB2	371	219	0.00%	0.001%
38	6.355	1650	1653	1655	rBV2	201	140	0.00%	0.001%
39	6.378	1658	1660	1661	rBV	256	83	0.00%	0.000%
40	6.423	1672	1674	1676	rVB	297	111	0.00%	0.000%
41	6.474	1688	1690	1694	rVB	245	159	0.00%	0.001%
42	6.513	1699	1702	1703	rBV	233	151	0.00%	0.001%
43	6.548	1707	1713	1715	rBV3	269	248	0.00%	0.001%
44	6.622	1728	1736	1738	rBV3	1260	1347	0.02%	0.005%
45	6.696	1757	1759	1765	rVB3	277	152	0.00%	0.001%
46	6.744	1770	1774	1775	rBV2	348	244	0.00%	0.001%
47	6.802	1789	1792	1796	rBV2	345	222	0.00%	0.001%
48	6.821	1796	1798	1800	rBV	298	147	0.00%	0.001%
49	6.857	1806	1809	1812	rBV2	415	281	0.00%	0.001%
50	6.911	1823	1826	1827	rBV2	343	205	0.00%	0.001%
51	6.979	1833	1847	1873	rBV	193297	356962	5.40%	1.331%
52	7.307	1937	1949	1983	rBV	713485	1272606	19.26%	4.743%
53	7.612	2034	2044	2070	rBV	133412	235722	3.57%	0.879%
54	7.834	2103	2113	2129	rVB3	23808	41707	0.63%	0.155%
55	7.966	2137	2154	2177	rBV	1055420	1785819	27.02%	6.656%
56	8.082	2180	2190	2229	rVV	445845	790413	11.96%	2.946%
57	8.564	2337	2340	2344	rBV4	414	398	0.01%	0.001%
58	8.615	2352	2356	2357	rBV2	418	308	0.00%	0.001%
59	8.641	2362	2364	2367	rVB3	517	285	0.00%	0.001%
60	8.670	2370	2373	2376	rBV2	355	219	0.00%	0.001%
61	8.706	2381	2384	2385	rBV2	323	156	0.00%	0.001%
62	8.792	2409	2411	2412	rBV2	204	86	0.00%	0.000%
63	8.844	2415	2427	2456	rVV	807707	1322659	20.01%	4.930%
64	9.069	2493	2497	2501	rBV3	470	518	0.01%	0.002%
65	9.172	2527	2529	2531	rBV3	323	167	0.00%	0.001%
66	9.230	2544	2547	2548	rBV2	256	144	0.00%	0.001%
67	9.329	2576	2578	2581	rVB2	190	105	0.00%	0.000%
68	9.349	2581	2584	2587	rBV	191	173	0.00%	0.001%
69	9.397	2597	2599	2600	rBV	159	66	0.00%	0.000%
70	9.451	2613	2616	2617	rBV	127	67	0.00%	0.000%
71	9.609	2659	2665	2670	rBV2	192	269	0.00%	0.001%
72	9.686	2685	2689	2690	rBV2	137	89	0.00%	0.000%
73	9.715	2695	2698	2699	rBV	198	102	0.00%	0.000%
74	9.844	2733	2738	2740	rBV	223	167	0.00%	0.001%
75	9.882	2747	2750	2753	rBV	250	164	0.00%	0.001%
76	9.966	2773	2776	2779	rBV2	396	288	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
 Data File : VV029488.D
 Acq On : 08 Dec 2022 21:19
 Operator : SY/MD
 Sample : N5929-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ96

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.056	2800	2804	2807	rBV	253	208	0.00%	0.001%
78	10.207	2835	2851	2877	rBV	530122	832038	12.59%	3.101%
79	10.377	2894	2904	2915	rVB2	5995	10103	0.15%	0.038%
80	10.496	2937	2941	2942	rBV	351	216	0.00%	0.001%
81	10.564	2960	2962	2965	rBV	223	82	0.00%	0.000%
82	10.686	2997	3000	3001	rBV	213	124	0.00%	0.000%
83	10.792	3029	3033	3035	rBV	350	296	0.00%	0.001%
84	10.837	3045	3047	3050	rBV2	388	263	0.00%	0.001%
85	10.947	3078	3081	3084	rBV2	253	167	0.00%	0.001%
86	10.963	3084	3086	3088	rBV3	211	134	0.00%	0.000%
87	10.988	3088	3094	3096	rVV2	214	246	0.00%	0.001%
88	11.175	3147	3152	3159	rVB3	1053	1372	0.02%	0.005%
89	11.236	3159	3171	3194	rBV	865545	1338109	20.25%	4.988%
90	11.554	3262	3270	3275	rBV5	1680	2622	0.04%	0.010%
91	11.612	3276	3288	3315	rVV	779721	1213991	18.37%	4.525%
92	11.754	3329	3332	3335	rBV4	588	384	0.01%	0.001%
93	11.956	3394	3395	3396	rBV	234	71	0.00%	0.000%
94	12.001	3407	3409	3411	rBV2	258	101	0.00%	0.000%
95	12.082	3432	3434	3436	rBV3	249	113	0.00%	0.000%
96	12.339	3512	3514	3515	rBV	251	71	0.00%	0.000%
97	12.602	3595	3596	3599	rBV2	255	102	0.00%	0.000%
98	12.615	3599	3600	3601	rBV	237	67	0.00%	0.000%
99	12.786	3650	3653	3658	rBV3	418	321	0.00%	0.001%
100	13.461	3861	3863	3864	rBV	565	216	0.00%	0.001%




Sum of corrected areas: 26828620

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
Data File : VV029488.D
Acq On : 08 Dec 2022 21:19
Operator : SY/MD
Sample : N5929-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ96

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

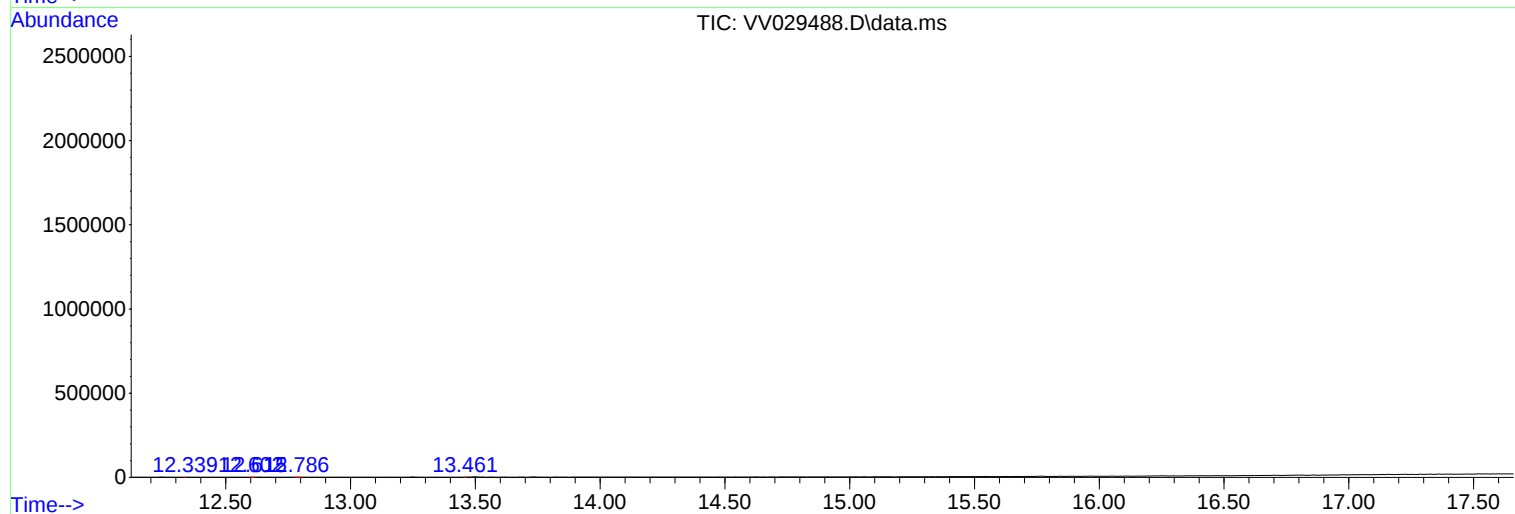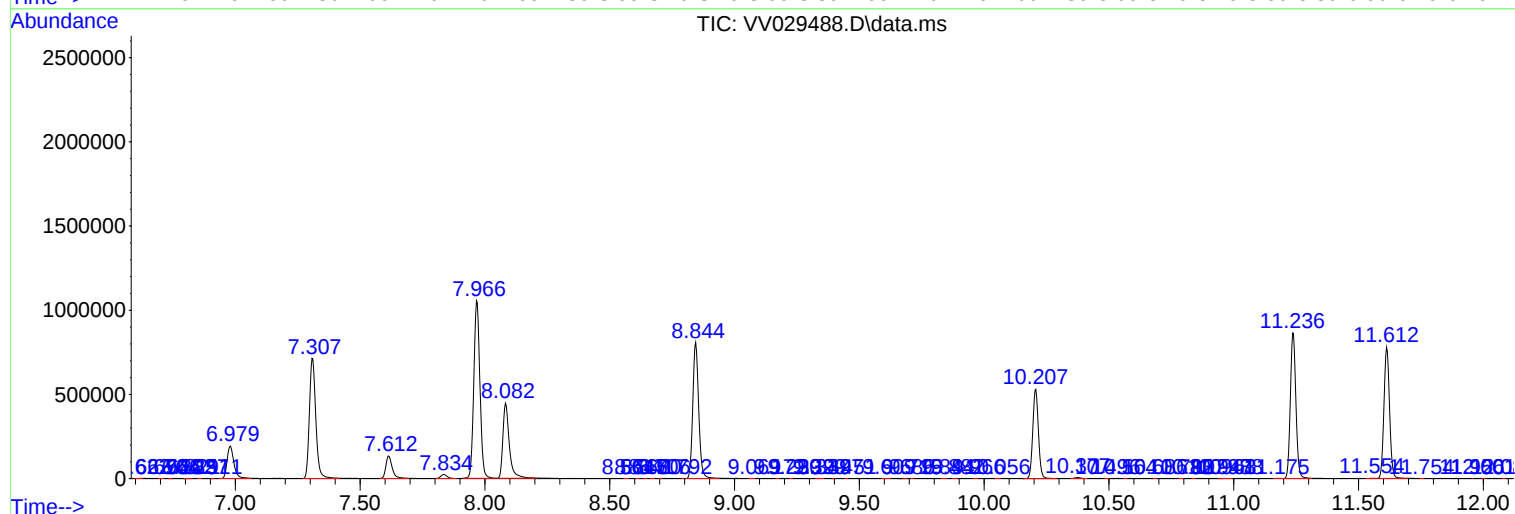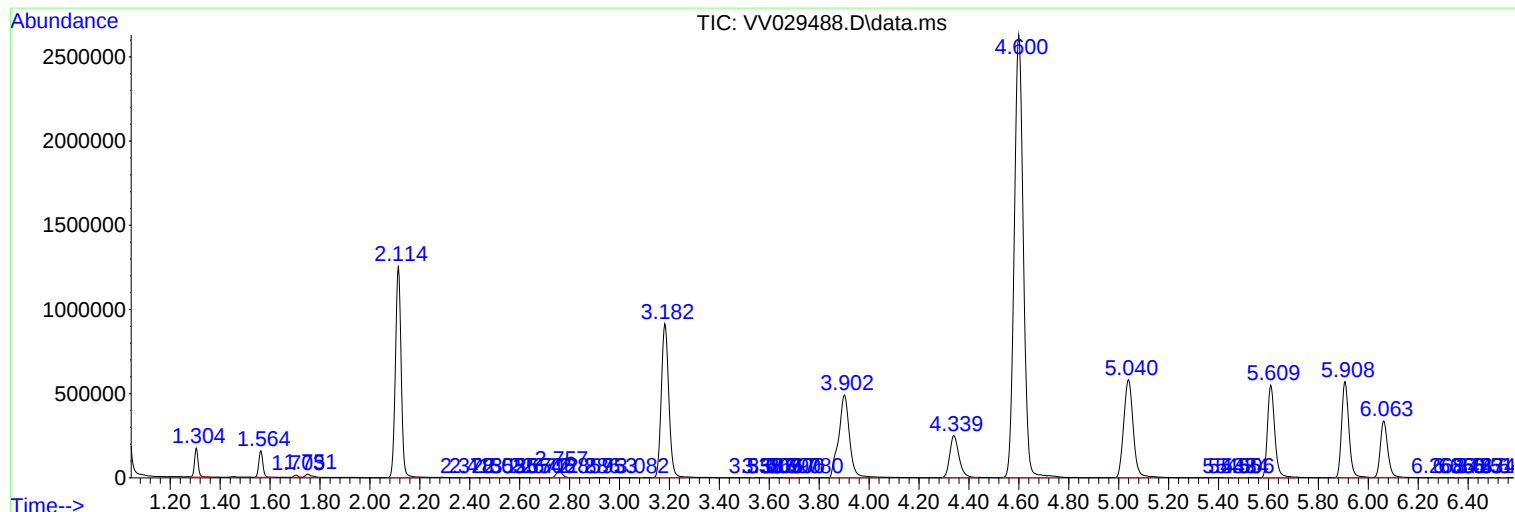

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
Data File : VV029488.D
Acq On : 08 Dec 2022 21:19
Operator : SY/MD
Sample : N5929-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ96

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
Data File : VV029488.D
Acq On : 08 Dec 2022 21:19
Operator : SY/MD
Sample : N5929-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ96

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------