

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120822\
 Data File : VW029489.D
 Acq On : 08 Dec 2022 21:43
 Operator : SY/MD
 Sample : N5929-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ97

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VW029489.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	96	rVB	177018	178793	3.56%	0.705%
2	1.564	155	163	179	rVB	154655	176110	3.51%	0.695%
3	1.703	201	206	213	rVB	7474	8111	0.16%	0.032%
4	1.751	214	221	226	rBV	15404	19388	0.39%	0.076%
5	2.114	319	334	358	rBV4	1169688	1866848	37.16%	7.365%
6	2.349	404	407	414	rVB2	452	362	0.01%	0.001%
7	2.407	420	425	428	rVB2	359	287	0.01%	0.001%
8	2.510	448	457	462	rVB4	1538	2316	0.05%	0.009%
9	2.558	467	472	474	rBV2	302	225	0.00%	0.001%
10	2.654	497	502	505	rBV2	252	232	0.00%	0.001%
11	2.757	523	534	547	rBV2	24359	43322	0.86%	0.171%
12	3.072	631	632	641	rVB2	206	230	0.00%	0.001%
13	3.182	645	666	695	rBV	582967	1230309	24.49%	4.854%
14	3.902	871	890	933	rBV2	672072	1908763	38.00%	7.530%
15	4.262	999	1002	1005	rVB3	465	317	0.01%	0.001%
16	4.339	1009	1026	1058	rVV	244339	652549	12.99%	2.574%
17	4.600	1086	1107	1145	rBV	2006402	5023214	100.00%	19.817%
18	4.873	1190	1192	1195	rVB2	491	256	0.01%	0.001%
19	4.892	1195	1198	1203	rVB3	271	238	0.00%	0.001%
20	4.924	1205	1208	1212	rBV2	331	243	0.00%	0.001%
21	4.947	1213	1215	1219	rVB2	421	262	0.01%	0.001%
22	5.040	1226	1244	1302	rBV2	575796	1530269	30.46%	6.037%
23	5.281	1316	1319	1323	rBV2	340	267	0.01%	0.001%
24	5.387	1349	1352	1356	rVB3	352	245	0.00%	0.001%
25	5.410	1356	1359	1363	rVB2	369	289	0.01%	0.001%
26	5.439	1363	1368	1370	rBV3	402	381	0.01%	0.002%
27	5.487	1377	1383	1388	rVB3	484	601	0.01%	0.002%
28	5.609	1407	1421	1470	rBV	551724	1127411	22.44%	4.448%
29	5.905	1500	1513	1548	rBV	988346	1943939	38.70%	7.669%
30	6.063	1549	1562	1588	rVV	326437	667340	13.29%	2.633%
31	6.403	1665	1668	1671	rVV3	505	436	0.01%	0.002%
32	6.519	1701	1704	1711	rVB3	398	399	0.01%	0.002%
33	6.622	1725	1736	1740	rBV6	1556	2306	0.05%	0.009%
34	6.722	1766	1767	1771	rVB2	423	265	0.01%	0.001%
35	6.744	1771	1774	1777	rBV2	431	281	0.01%	0.001%
36	6.812	1793	1795	1801	rVB3	378	284	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120822\
 Data File : VW029489.D
 Acq On : 08 Dec 2022 21:43
 Operator : SY/MD
 Sample : N5929-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ97

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.979	1834	1847	1869	rBV	188289	347017	6.91%	1.369%
38	7.182	1907	1910	1912	rBV3	469	314	0.01%	0.001%
39	7.307	1937	1949	1986	rBV	695060	1252704	24.94%	4.942%
40	7.458	1994	1996	2006	rVB6	663	940	0.02%	0.004%
41	7.612	2034	2044	2071	rVV	133571	233615	4.65%	0.922%
42	7.834	2103	2113	2126	rBV2	24681	42078	0.84%	0.166%
43	7.966	2137	2154	2179	rBV	859403	1471997	29.30%	5.807%
44	8.082	2180	2190	2228	rVV	423721	776412	15.46%	3.063%
45	8.329	2265	2267	2271	rVB3	400	268	0.01%	0.001%
46	8.510	2321	2323	2327	rVB2	445	257	0.01%	0.001%
47	8.529	2327	2329	2332	rBV3	498	334	0.01%	0.001%
48	8.571	2339	2342	2344	rVB3	463	289	0.01%	0.001%
49	8.590	2344	2348	2350	rBV2	351	242	0.00%	0.001%
50	8.651	2362	2367	2372	rBV4	436	447	0.01%	0.002%
51	8.718	2382	2388	2390	rBV3	321	252	0.01%	0.001%
52	8.760	2400	2401	2407	rVB2	359	252	0.01%	0.001%
53	8.799	2407	2413	2415	rBV2	495	422	0.01%	0.002%
54	8.844	2415	2427	2453	rBV	808802	1324058	26.36%	5.223%
55	9.136	2516	2518	2525	rVB6	566	670	0.01%	0.003%
56	9.326	2570	2577	2581	rBV2	445	422	0.01%	0.002%
57	9.538	2638	2643	2644	rBV3	424	343	0.01%	0.001%
58	9.670	2681	2684	2688	rBV	395	308	0.01%	0.001%
59	9.812	2721	2728	2732	rBV4	396	548	0.01%	0.002%
60	9.931	2759	2765	2766	rVV2	361	385	0.01%	0.002%
61	9.995	2782	2785	2788	rBV3	439	297	0.01%	0.001%
62	10.207	2836	2851	2868	rBV	514139	809399	16.11%	3.193%
63	10.371	2894	2902	2915	rBV2	3520	5974	0.12%	0.024%
64	10.455	2924	2928	2930	rBV2	342	260	0.01%	0.001%
65	10.493	2935	2940	2942	rVV2	285	314	0.01%	0.001%
66	10.529	2947	2951	2954	rBV4	741	805	0.02%	0.003%
67	10.561	2958	2961	2965	rBV3	483	449	0.01%	0.002%
68	10.734	3011	3015	3018	rVB2	253	256	0.01%	0.001%
69	10.844	3046	3049	3056	rVB3	338	324	0.01%	0.001%
70	11.030	3103	3107	3111	rVB3	315	283	0.01%	0.001%
71	11.056	3111	3115	3119	rBV2	264	285	0.01%	0.001%
72	11.098	3124	3128	3134	rBV3	389	530	0.01%	0.002%
73	11.172	3147	3151	3153	rBV4	656	547	0.01%	0.002%
74	11.239	3159	3172	3200	rBV	896998	1405805	27.99%	5.546%
75	11.490	3246	3250	3253	rBV3	486	406	0.01%	0.002%
76	11.558	3262	3271	3275	rVV7	1666	2405	0.05%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120822\
 Data File : VW029489.D
 Acq On : 08 Dec 2022 21:43
 Operator : SY/MD
 Sample : N5929-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ97

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	11.612	3275	3288	3322	rVB	801637	1264589	25.17%	4.989%
78	11.934	3385	3388	3391	rBV2	384	232	0.00%	0.001%
79	11.969	3395	3399	3405	rBV3	508	755	0.02%	0.003%
80	12.037	3418	3420	3423	rBV2	529	307	0.01%	0.001%
81	12.165	3455	3460	3464	rVB2	467	358	0.01%	0.001%
82	12.220	3469	3477	3478	rBV2	598	604	0.01%	0.002%
83	12.271	3490	3493	3496	rBV3	354	264	0.01%	0.001%
84	12.304	3500	3503	3505	rBV3	359	260	0.01%	0.001%
85	12.326	3508	3510	3514	rVB2	455	314	0.01%	0.001%
86	12.355	3514	3519	3523	rBV2	552	530	0.01%	0.002%
87	12.468	3549	3554	3559	rBV3	464	423	0.01%	0.002%
88	12.532	3571	3574	3577	rVB3	370	246	0.00%	0.001%
89	12.554	3577	3581	3583	rBV2	308	284	0.01%	0.001%
90	12.638	3604	3607	3612	rVB4	1194	1018	0.02%	0.004%
91	12.776	3647	3650	3655	rBV3	414	419	0.01%	0.002%
92	13.001	3716	3720	3722	rBV2	397	293	0.01%	0.001%
93	13.133	3757	3761	3764	rBV3	456	420	0.01%	0.002%
94	13.201	3779	3782	3784	rBV2	586	428	0.01%	0.002%
95	13.252	3792	3798	3803	rBV6	1665	1907	0.04%	0.008%
96	13.493	3866	3873	3875	rBV4	2218	2048	0.04%	0.008%
97	13.654	3919	3923	3926	rBV3	374	387	0.01%	0.002%
98	13.734	3942	3948	3953	rVB7	1046	1533	0.03%	0.006%
99	14.098	4059	4061	4063	rBV3	465	267	0.01%	0.001%
100	14.336	4132	4135	4137	rBV4	575	389	0.01%	0.002%




Sum of corrected areas: 25348276

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
Data File : VV029489.D
Acq On : 08 Dec 2022 21:43
Operator : SY/MD
Sample : N5929-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ97

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

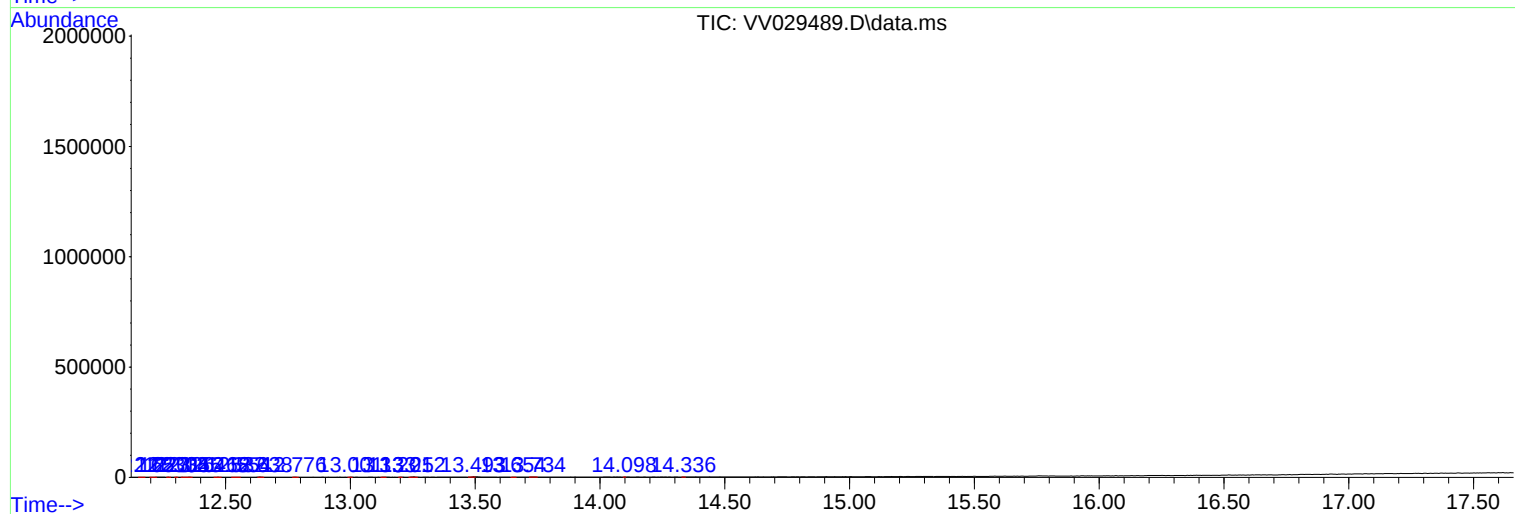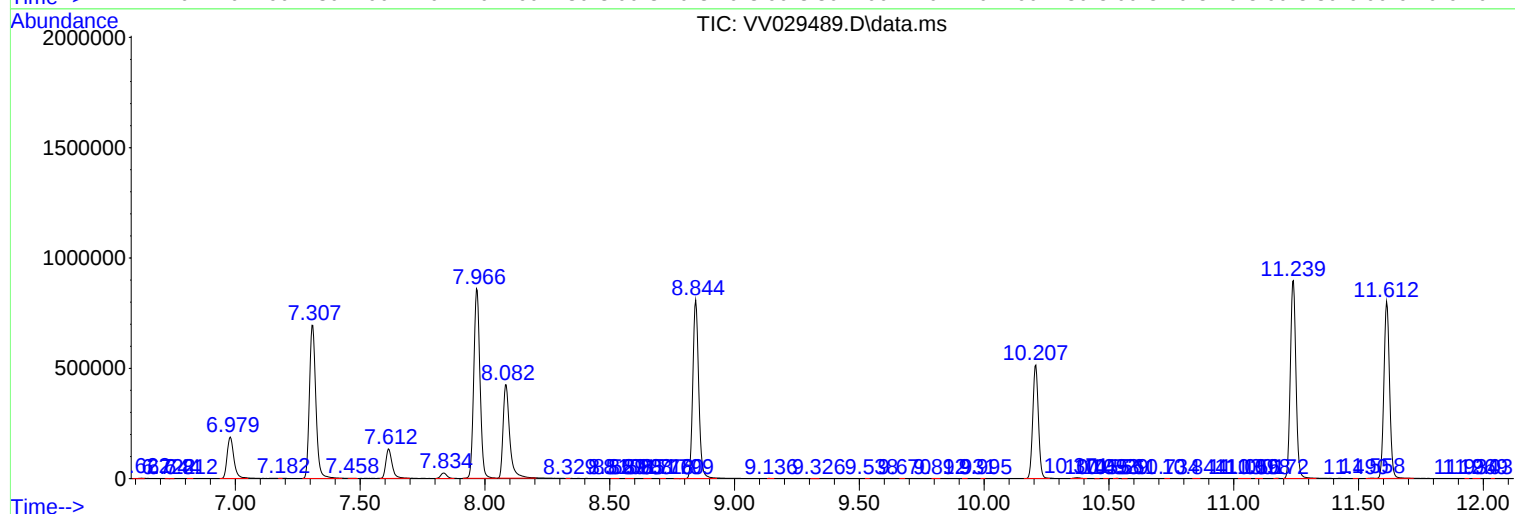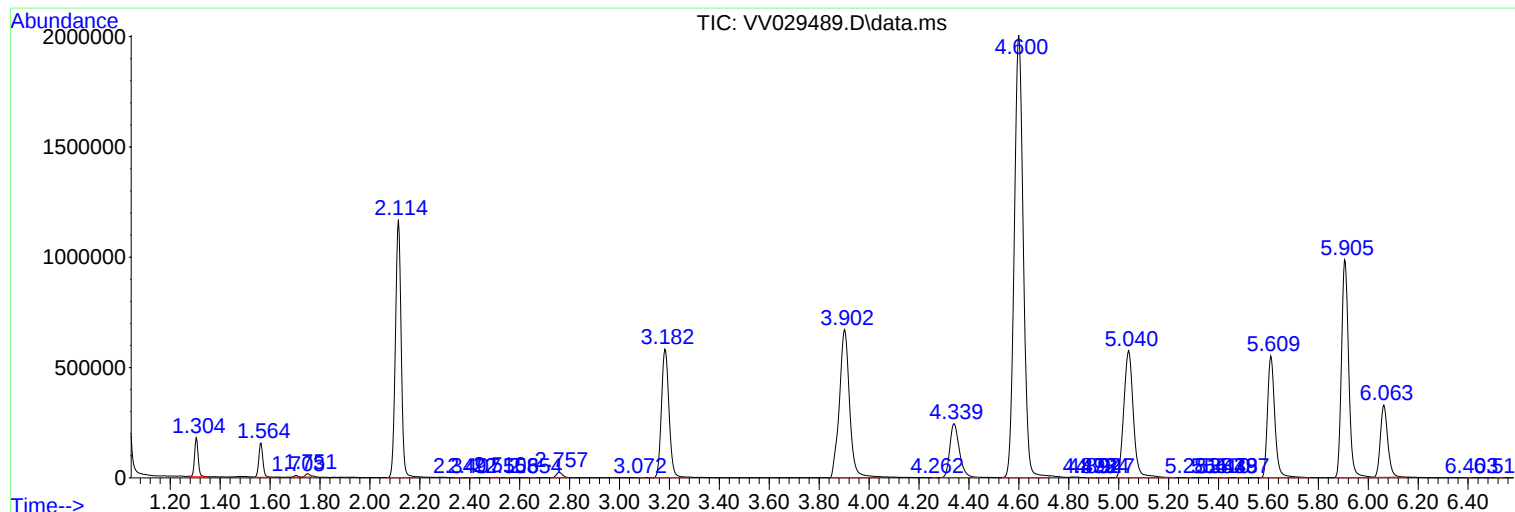

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
Data File : VV029489.D
Acq On : 08 Dec 2022 21:43
Operator : SY/MD
Sample : N5929-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ97

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
Data File : VV029489.D
Acq On : 08 Dec 2022 21:43
Operator : SY/MD
Sample : N5929-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ97

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------