

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120822\
 Data File : VW029490.D
 Acq On : 08 Dec 2022 22:06
 Operator : SY/MD
 Sample : N5929-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ98

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M

Title : VOC Analysis

Signal : TIC: VW029490.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	100	rVB	176999	176965	11.25%	1.278%
2	1.565	155	163	179	rVB	155770	176905	11.24%	1.277%
3	2.040	308	311	314	rBV3	647	460	0.03%	0.003%
4	2.105	319	331	345	rBV	306691	448858	28.53%	3.240%
5	2.410	422	426	429	rVB3	405	322	0.02%	0.002%
6	2.503	447	455	463	rVB4	1191	1981	0.13%	0.014%
7	2.545	463	468	470	rBV3	312	235	0.01%	0.002%
8	2.703	513	517	522	rVV3	273	262	0.02%	0.002%
9	2.757	522	534	555	rVB2	23929	43310	2.75%	0.313%
10	2.880	568	572	577	rBV2	337	271	0.02%	0.002%
11	2.918	581	584	589	rVB	352	242	0.02%	0.002%
12	3.002	604	610	613	rBV2	341	388	0.02%	0.003%
13	3.185	652	667	690	rBV2	37277	79062	5.03%	0.571%
14	3.317	706	708	713	rVV4	390	278	0.02%	0.002%
15	3.355	716	720	726	rVV2	338	334	0.02%	0.002%
16	3.635	805	807	813	rVB2	251	227	0.01%	0.002%
17	3.687	813	823	827	rBV2	153	263	0.02%	0.002%
18	3.899	870	889	930	rVV2	184223	727353	46.23%	5.251%
19	4.095	948	950	955	rVB5	506	343	0.02%	0.002%
20	4.339	1007	1026	1058	rBV	244822	621483	39.50%	4.487%
21	4.600	1090	1107	1128	rVV2	70937	180872	11.50%	1.306%
22	4.825	1172	1177	1182	rBV4	352	341	0.02%	0.002%
23	5.040	1226	1244	1296	rBV2	587139	1573342	100.00%	11.358%
24	5.298	1321	1324	1328	rBV2	304	259	0.02%	0.002%
25	5.349	1336	1340	1345	rVB3	283	235	0.01%	0.002%
26	5.461	1372	1375	1378	rBV3	371	321	0.02%	0.002%
27	5.609	1408	1421	1445	rBV	573682	1154060	73.35%	8.331%
28	5.912	1501	1515	1538	rVV2	81637	171677	10.91%	1.239%
29	6.063	1548	1562	1599	rBV	338723	702327	44.64%	5.070%
30	6.249	1617	1620	1623	rVB3	586	336	0.02%	0.002%
31	6.272	1623	1627	1631	rVB3	306	328	0.02%	0.002%
32	6.326	1640	1644	1647	rBV2	410	334	0.02%	0.002%
33	6.455	1681	1684	1688	rVB2	483	289	0.02%	0.002%
34	6.500	1694	1698	1701	rBV3	677	662	0.04%	0.005%
35	6.625	1725	1737	1738	rBV5	1380	1805	0.11%	0.013%
36	6.822	1794	1798	1803	rVB2	397	301	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120822\
 Data File : VW029490.D
 Acq On : 08 Dec 2022 22:06
 Operator : SY/MD
 Sample : N5929-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ98

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.844	1803	1805	1808	rBV2	384	306	0.02%	0.002%
38	6.979	1835	1847	1877	rBV	192935	356860	22.68%	2.576%
39	7.105	1884	1886	1889	rVB2	680	382	0.02%	0.003%
40	7.127	1889	1893	1896	rBV4	460	441	0.03%	0.003%
41	7.159	1900	1903	1906	rVB3	746	492	0.03%	0.004%
42	7.236	1924	1927	1928	rBV3	487	264	0.02%	0.002%
43	7.307	1937	1949	1980	rBV	719384	1276418	81.13%	9.215%
44	7.465	1996	1998	2000	rVB2	620	293	0.02%	0.002%
45	7.613	2026	2044	2072	rBV2	148180	273491	17.38%	1.974%
46	7.838	2113	2114	2119	rVB2	552	379	0.02%	0.003%
47	7.969	2137	2155	2177	rVB	110959	199270	12.67%	1.439%
48	8.082	2180	2190	2226	rBV	440847	808237	51.37%	5.835%
49	8.400	2287	2289	2292	rBV	456	277	0.02%	0.002%
50	8.458	2303	2307	2311	rVB3	356	262	0.02%	0.002%
51	8.844	2415	2427	2465	rBV	838919	1381371	87.80%	9.972%
52	9.050	2487	2491	2492	rBV3	333	251	0.02%	0.002%
53	9.120	2508	2513	2514	rBV	397	283	0.02%	0.002%
54	9.137	2514	2518	2521	rVV3	639	579	0.04%	0.004%
55	9.153	2521	2523	2526	rVB	554	229	0.01%	0.002%
56	9.182	2526	2532	2533	rBV2	373	319	0.02%	0.002%
57	9.220	2539	2544	2551	rVB4	398	442	0.03%	0.003%
58	9.384	2591	2595	2600	rVB3	266	266	0.02%	0.002%
59	9.477	2618	2624	2628	rBV2	281	308	0.02%	0.002%
60	9.532	2638	2641	2642	rBV3	454	270	0.02%	0.002%
61	9.924	2760	2763	2766	rVV2	643	486	0.03%	0.004%
62	10.207	2838	2851	2871	rBV	530217	841556	53.49%	6.075%
63	10.374	2896	2903	2914	rVB3	3904	6470	0.41%	0.047%
64	10.465	2927	2931	2937	rVB	363	348	0.02%	0.003%
65	10.529	2947	2951	2956	rVV2	354	288	0.02%	0.002%
66	10.551	2956	2958	2964	rVB3	343	241	0.02%	0.002%
67	10.590	2964	2970	2974	rVB2	387	454	0.03%	0.003%
68	10.709	3002	3007	3013	rBV3	334	445	0.03%	0.003%
69	10.760	3020	3023	3027	rBV2	267	215	0.01%	0.002%
70	10.809	3031	3038	3041	rBV	318	371	0.02%	0.003%
71	10.908	3063	3069	3076	rVB4	624	909	0.06%	0.007%
72	11.027	3101	3106	3109	rBV2	230	220	0.01%	0.002%
73	11.178	3149	3153	3157	rVB5	677	690	0.04%	0.005%
74	11.236	3157	3171	3195	rBV	887653	1385980	88.09%	10.005%
75	11.429	3228	3231	3237	rBV3	335	358	0.02%	0.003%
76	11.481	3244	3247	3250	rBV2	273	266	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
 Data File : VV029490.D
 Acq On : 08 Dec 2022 22:06
 Operator : SY/MD
 Sample : N5929-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ98

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	11.561	3269	3272	3275	rVV3	630	387	0.02%	0.003%
78	11.612	3275	3288	3310	rVV	795607	1230450	78.21%	8.883%
79	11.927	3380	3386	3390	rBV2	456	430	0.03%	0.003%
80	11.953	3390	3394	3396	rBV2	360	245	0.02%	0.002%
81	12.059	3424	3427	3432	rBV2	268	221	0.01%	0.002%
82	12.178	3461	3464	3469	rVV2	273	284	0.02%	0.002%
83	12.243	3475	3484	3492	rVB6	1130	1965	0.12%	0.014%
84	12.426	3537	3541	3543	rBV4	398	299	0.02%	0.002%
85	12.542	3573	3577	3581	rBV4	390	263	0.02%	0.002%
86	12.606	3593	3597	3600	rBV3	428	346	0.02%	0.002%
87	12.635	3601	3606	3613	rVB4	682	837	0.05%	0.006%
88	12.825	3661	3665	3672	rVB4	590	571	0.04%	0.004%
89	12.870	3675	3679	3680	rBV2	326	214	0.01%	0.002%
90	13.246	3793	3796	3798	rBV2	922	759	0.05%	0.005%
91	13.342	3815	3826	3830	rBV5	726	1328	0.08%	0.010%
92	13.365	3830	3833	3837	rBV3	388	360	0.02%	0.003%
93	13.493	3866	3873	3880	rBV3	1266	1630	0.10%	0.012%
94	13.725	3943	3945	3954	rVB6	1019	1151	0.07%	0.008%
95	13.776	3958	3961	3963	rBV3	473	345	0.02%	0.002%
96	13.812	3970	3972	3976	rBV4	344	243	0.02%	0.002%
97	13.831	3976	3978	3981	rBV3	445	266	0.02%	0.002%
98	13.895	3995	3998	4002	rBV2	471	393	0.02%	0.003%
99	13.918	4002	4005	4007	rBV3	818	408	0.03%	0.003%
100	14.744	4260	4262	4268	rBV4	810	794	0.05%	0.006%

Sum of corrected areas: 13852207




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
Data File : VV029490.D
Acq On : 08 Dec 2022 22:06
Operator : SY/MD
Sample : N5929-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ98

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

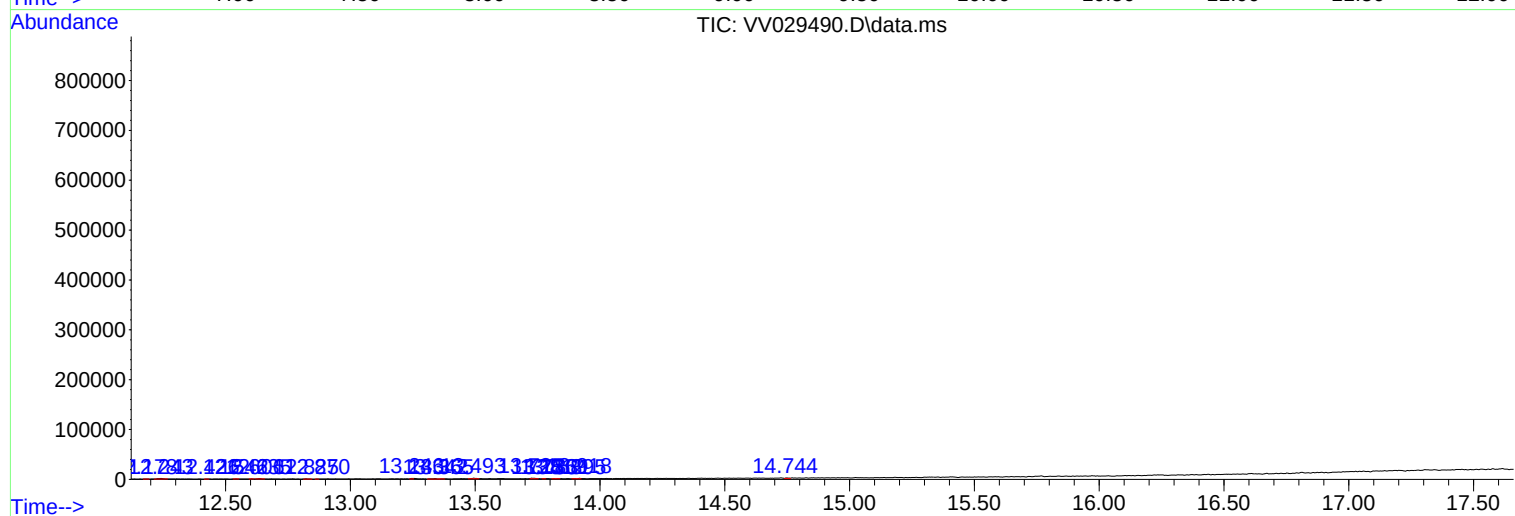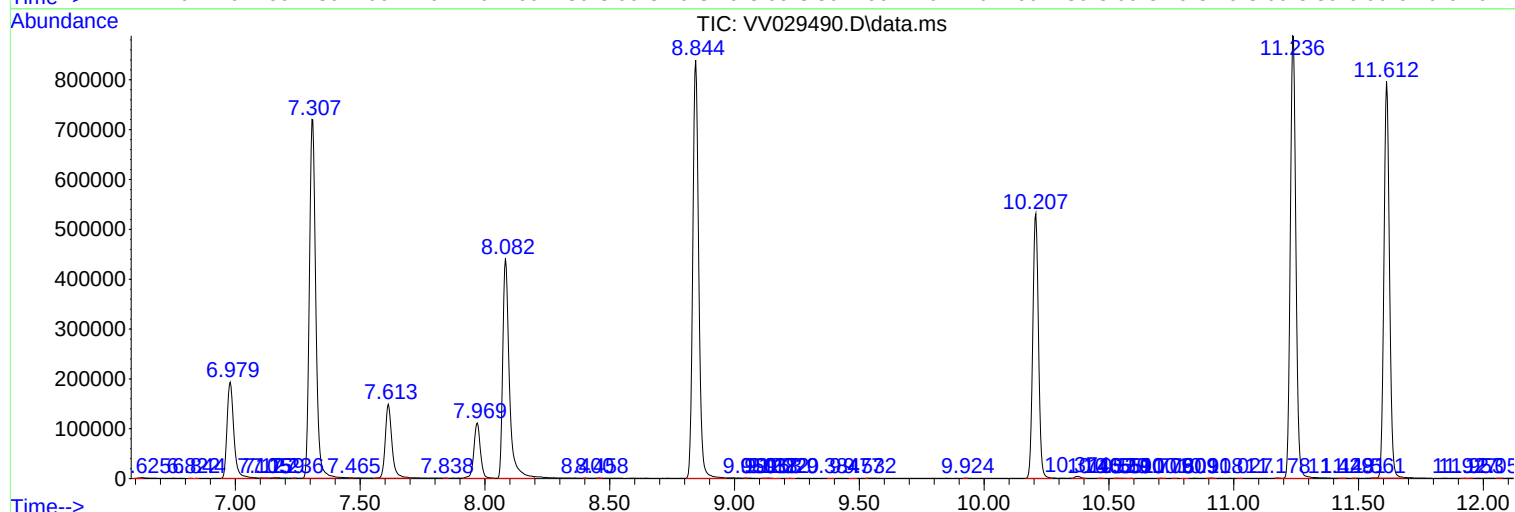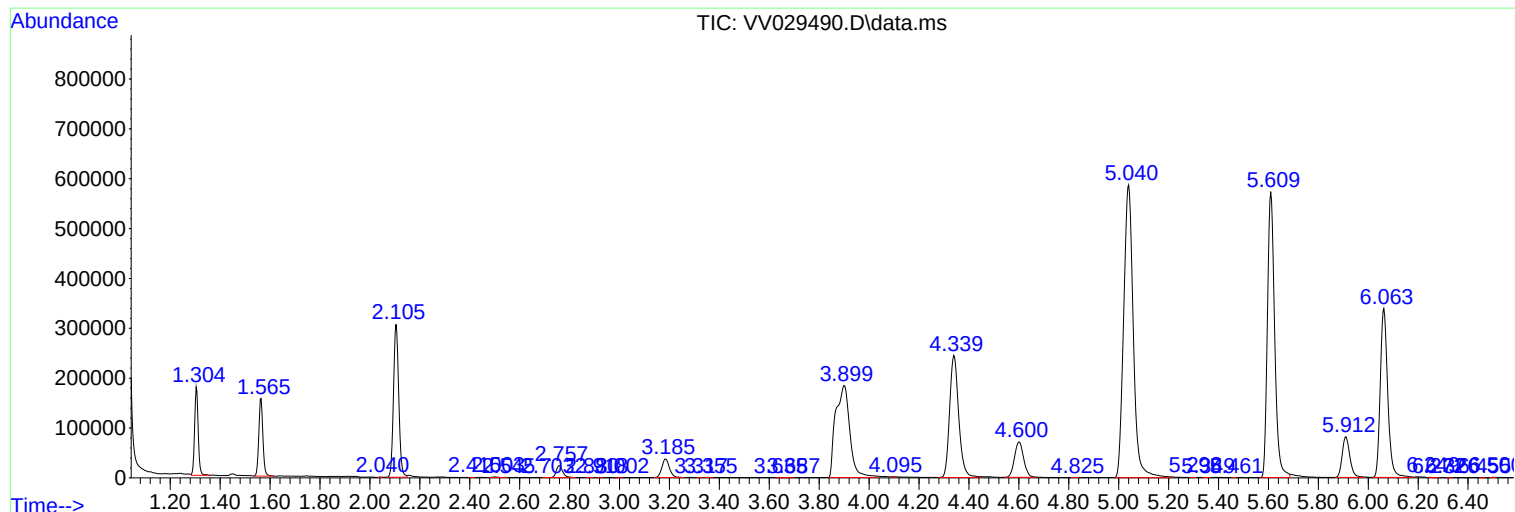

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
Data File : VV029490.D
Acq On : 08 Dec 2022 22:06
Operator : SY/MD
Sample : N5929-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ98

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
Data File : VV029490.D
Acq On : 08 Dec 2022 22:06
Operator : SY/MD
Sample : N5929-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ98

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
