

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120822\
 Data File : VW029493.D
 Acq On : 08 Dec 2022 23:17
 Operator : SY/MD
 Sample : N5915-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5N02

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VW029493.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	99	rVB	158134	159136	11.06%	1.203%
2	1.564	156	163	180	rVB	142705	162917	11.32%	1.232%
3	2.108	321	332	347	rBV3	342292	556566	38.68%	4.207%
4	2.712	516	520	525	rBV3	284	262	0.02%	0.002%
5	2.767	532	537	540	rVB3	365	360	0.03%	0.003%
6	2.854	561	564	566	rBV	146	100	0.01%	0.001%
7	2.947	592	593	595	rBV	205	42	0.00%	0.000%
8	2.963	596	598	605	rVB2	515	357	0.02%	0.003%
9	2.995	605	608	609	rBV2	144	72	0.01%	0.001%
10	3.024	615	617	619	rBV	260	119	0.01%	0.001%
11	3.088	635	637	639	rBV	178	88	0.01%	0.001%
12	3.137	649	652	654	rBV	216	144	0.01%	0.001%
13	3.269	691	693	697	rVB2	175	111	0.01%	0.001%
14	3.288	697	699	700	rBV	196	82	0.01%	0.001%
15	3.378	725	727	731	rBV	207	128	0.01%	0.001%
16	3.397	731	733	736	rVB2	198	92	0.01%	0.001%
17	3.445	746	748	751	rBV2	270	169	0.01%	0.001%
18	3.506	764	767	769	rBV	209	146	0.01%	0.001%
19	3.564	783	785	786	rBV	162	49	0.00%	0.000%
20	3.667	815	817	819	rBV	162	72	0.01%	0.001%
21	3.754	840	844	845	rBV2	230	169	0.01%	0.001%
22	3.825	862	866	870	rBV2	251	242	0.02%	0.002%
23	3.870	870	880	910	rBV	111333	299095	20.78%	2.261%
24	4.339	1008	1026	1049	rBV	227982	560102	38.92%	4.234%
25	4.658	1120	1125	1128	rBV3	555	411	0.03%	0.003%
26	4.728	1145	1147	1148	rBV	101	39	0.00%	0.000%
27	4.841	1179	1182	1183	rBV	126	73	0.01%	0.001%
28	4.863	1188	1189	1192	rVB	212	81	0.01%	0.001%
29	4.886	1192	1196	1199	rBV	306	233	0.02%	0.002%
30	4.902	1199	1201	1202	rBV2	90	42	0.00%	0.000%
31	4.924	1205	1208	1209	rBV	307	190	0.01%	0.001%
32	5.040	1226	1244	1293	rBV2	543423	1439035	100.00%	10.878%
33	5.400	1353	1356	1360	rBV2	482	507	0.04%	0.004%
34	5.445	1368	1370	1372	rBV	154	68	0.00%	0.001%
35	5.468	1372	1377	1381	rBV3	427	411	0.03%	0.003%
36	5.532	1396	1397	1398	rVB3	99	19	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120822\
 Data File : VW029493.D
 Acq On : 08 Dec 2022 23:17
 Operator : SY/MD
 Sample : N5915-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5N02

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	5.542	1398	1400	1402	rBV	58	27	0.00%	0.000%
38	5.555	1402	1404	1405	rBV	94	45	0.00%	0.000%
39	5.609	1408	1421	1464	rBV	534743	1093532	75.99%	8.267%
40	5.908	1499	1514	1547	rBV	603792	1220570	84.82%	9.227%
41	6.063	1550	1562	1591	rVB	315122	639550	44.44%	4.835%
42	6.291	1631	1633	1637	rVB3	325	262	0.02%	0.002%
43	6.326	1642	1644	1645	rBV	197	85	0.01%	0.001%
44	6.407	1664	1669	1671	rBV3	342	305	0.02%	0.002%
45	6.442	1677	1680	1683	rBV2	255	158	0.01%	0.001%
46	6.471	1687	1689	1693	rVB	172	115	0.01%	0.001%
47	6.538	1707	1710	1713	rBV	240	209	0.01%	0.002%
48	6.567	1717	1719	1720	rBV	115	28	0.00%	0.000%
49	6.628	1728	1738	1743	rBV4	1112	1992	0.14%	0.015%
50	6.722	1765	1767	1769	rVB2	226	80	0.01%	0.001%
51	6.757	1774	1778	1780	rVB2	252	146	0.01%	0.001%
52	6.786	1780	1787	1792	rBV3	586	733	0.05%	0.006%
53	6.837	1799	1803	1804	rBV	390	259	0.02%	0.002%
54	6.908	1822	1825	1828	rBV2	151	104	0.01%	0.001%
55	6.979	1836	1847	1875	rBV	172688	317935	22.09%	2.403%
56	7.307	1937	1949	1983	rBV	665915	1181862	82.13%	8.934%
57	7.612	2034	2044	2071	rBV	119521	213162	14.81%	1.611%
58	7.773	2092	2094	2098	rBV2	380	276	0.02%	0.002%
59	7.879	2125	2127	2130	rBV2	397	279	0.02%	0.002%
60	8.082	2180	2190	2222	rBV	400892	729274	50.68%	5.513%
61	8.336	2267	2269	2271	rBV3	478	271	0.02%	0.002%
62	8.593	2342	2349	2354	rBV4	578	802	0.06%	0.006%
63	8.664	2369	2371	2372	rBV2	211	79	0.01%	0.001%
64	8.780	2405	2407	2410	rBV	321	205	0.01%	0.002%
65	8.844	2415	2427	2447	rBV	794790	1286301	89.39%	9.724%
66	9.162	2524	2526	2529	rVB2	345	192	0.01%	0.001%
67	9.188	2529	2534	2536	rBV2	413	326	0.02%	0.002%
68	9.214	2540	2542	2545	rVV	310	165	0.01%	0.001%
69	9.230	2545	2547	2550	rVB2	297	154	0.01%	0.001%
70	9.275	2559	2561	2562	rBV	124	32	0.00%	0.000%
71	9.291	2562	2566	2568	rVV3	441	271	0.02%	0.002%
72	9.513	2632	2635	2638	rBV2	353	168	0.01%	0.001%
73	9.590	2656	2659	2663	rBV	244	170	0.01%	0.001%
74	9.638	2673	2674	2678	rVB2	247	112	0.01%	0.001%
75	9.673	2683	2685	2687	rBV	119	49	0.00%	0.000%
76	9.706	2691	2695	2697	rBV	322	227	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
 Data File : VV029493.D
 Acq On : 08 Dec 2022 23:17
 Operator : SY/MD
 Sample : N5915-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5N02

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	9.760	2709	2712	2717	rBV2	207	227	0.02%	0.002%
78	9.789	2718	2721	2723	rBV2	331	217	0.02%	0.002%
79	10.062	2804	2806	2807	rBV2	140	63	0.00%	0.000%
80	10.165	2829	2838	2840	rBV4	6313	7652	0.53%	0.058%
81	10.207	2840	2851	2876	rVB	496314	778445	54.09%	5.885%
82	10.371	2894	2902	2914	rVB3	7651	12709	0.88%	0.096%
83	10.570	2956	2964	2972	rBV5	2141	3396	0.24%	0.026%
84	10.673	2993	2996	2998	rBV2	273	185	0.01%	0.001%
85	10.686	2998	3000	3004	rVV2	284	176	0.01%	0.001%
86	10.747	3015	3019	3020	rBV	652	405	0.03%	0.003%
87	10.850	3047	3051	3054	rBV3	512	414	0.03%	0.003%
88	10.876	3058	3059	3060	rBV3	106	25	0.00%	0.000%
89	10.985	3091	3093	3097	rBV2	466	359	0.02%	0.003%
90	11.024	3102	3105	3113	rVB3	370	454	0.03%	0.003%
91	11.146	3139	3143	3145	rBV2	280	268	0.02%	0.002%
92	11.239	3160	3172	3202	rBV	869187	1353597	94.06%	10.232%
93	11.612	3276	3288	3310	rBV	759661	1196588	83.15%	9.046%
94	11.808	3347	3349	3354	rBV3	374	238	0.02%	0.002%
95	11.921	3382	3384	3386	rBV2	257	111	0.01%	0.001%
96	12.368	3518	3523	3525	rBV3	400	345	0.02%	0.003%
97	12.413	3533	3537	3538	rBV2	416	296	0.02%	0.002%




Sum of corrected areas: 13228411

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
Data File : VV029493.D
Acq On : 08 Dec 2022 23:17
Operator : SY/MD
Sample : N5915-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5N02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

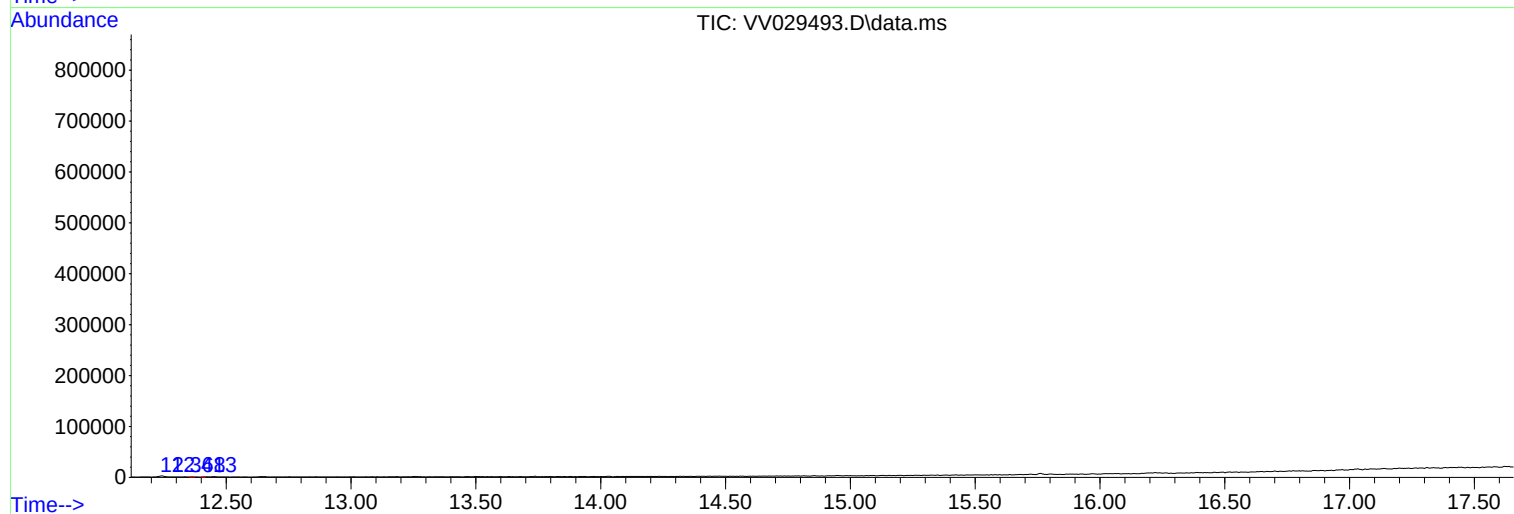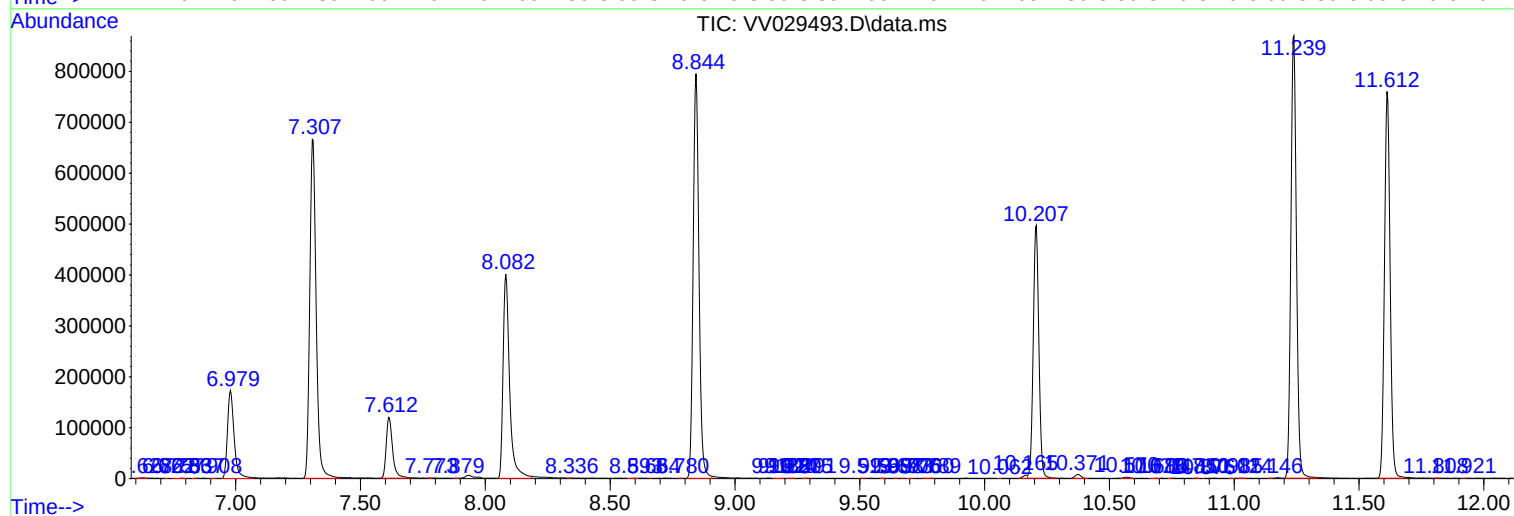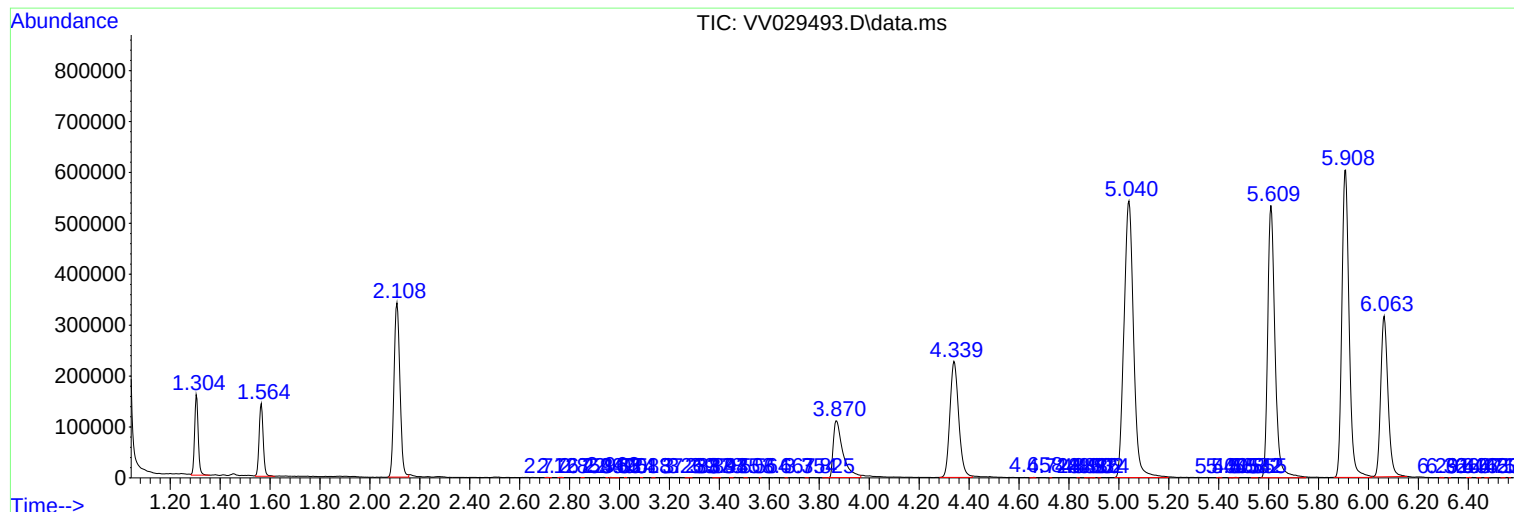

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
Data File : VV029493.D
Acq On : 08 Dec 2022 23:17
Operator : SY/MD
Sample : N5915-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5N02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
Data File : VV029493.D
Acq On : 08 Dec 2022 23:17
Operator : SY/MD
Sample : N5915-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5N02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------