

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120822\
 Data File : VW029496.D
 Acq On : 09 Dec 2022 00:27
 Operator : SY/MD
 Sample : N5915-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5N05

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VW029496.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	94	rVB	177495	175742	10.97%	1.287%
2	1.564	155	163	179	rVB	149809	173399	10.82%	1.270%
3	1.873	253	259	268	rVB3	3540	5569	0.35%	0.041%
4	1.995	295	297	300	rVB2	763	364	0.02%	0.003%
5	2.105	320	331	344	rBV2	301772	448254	27.97%	3.284%
6	2.265	378	381	385	rBV4	933	751	0.05%	0.006%
7	2.500	449	454	455	rBV4	1267	967	0.06%	0.007%
8	2.616	486	490	494	rBV	500	457	0.03%	0.003%
9	2.757	529	534	546	rVB6	1713	3134	0.20%	0.023%
10	3.172	653	663	675	rBV2	4423	9021	0.56%	0.066%
11	3.365	719	723	731	rVB2	468	488	0.03%	0.004%
12	3.449	744	749	755	rBV3	257	384	0.02%	0.003%
13	3.870	869	880	929	rBV2	147052	605561	37.79%	4.436%
14	4.339	1008	1026	1062	rBV	233659	588021	36.70%	4.307%
15	4.654	1122	1124	1127	rBV2	398	317	0.02%	0.002%
16	4.770	1156	1160	1169	rBV4	335	562	0.04%	0.004%
17	5.040	1226	1244	1280	rBV2	568470	1507715	94.09%	11.045%
18	5.436	1363	1367	1371	rVB3	393	326	0.02%	0.002%
19	5.461	1371	1375	1380	rBV3	445	418	0.03%	0.003%
20	5.519	1390	1393	1397	rVB2	441	373	0.02%	0.003%
21	5.609	1405	1421	1450	rBV	583623	1178973	73.58%	8.636%
22	5.912	1502	1515	1542	rVB4	22015	48833	3.05%	0.358%
23	6.063	1548	1562	1597	rBV	329576	684997	42.75%	5.018%
24	6.310	1631	1639	1641	rBV3	427	422	0.03%	0.003%
25	6.378	1654	1660	1663	rBV3	305	340	0.02%	0.002%
26	6.625	1731	1737	1741	rBV3	803	1135	0.07%	0.008%
27	6.738	1767	1772	1775	rBV3	382	357	0.02%	0.003%
28	6.899	1817	1822	1824	rBV2	319	300	0.02%	0.002%
29	6.979	1835	1847	1872	rBV	169117	312548	19.51%	2.290%
30	7.156	1899	1902	1903	rBV3	472	289	0.02%	0.002%
31	7.243	1926	1929	1936	rVB5	427	504	0.03%	0.004%
32	7.307	1936	1949	1992	rBV	697515	1249588	77.98%	9.154%
33	7.612	2034	2044	2067	rBV	121477	214057	13.36%	1.568%
34	7.789	2094	2099	2105	rBV5	550	876	0.05%	0.006%
35	7.857	2116	2120	2122	rVB2	494	410	0.03%	0.003%
36	7.879	2122	2127	2131	rBV2	401	405	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120822\
 Data File : VW029496.D
 Acq On : 09 Dec 2022 00:27
 Operator : SY/MD
 Sample : N5915-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5N05

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	7.969	2135	2155	2174	rVB3	65723	118870	7.42%	0.871%
38	8.082	2178	2190	2226	rBV	524544	946189	59.05%	6.931%
39	8.481	2312	2314	2317	rVV2	511	326	0.02%	0.002%
40	8.500	2317	2320	2321	rVV2	596	312	0.02%	0.002%
41	8.538	2330	2332	2337	rVB3	529	403	0.03%	0.003%
42	8.664	2368	2371	2375	rVB3	427	325	0.02%	0.002%
43	8.686	2375	2378	2381	rBV3	343	282	0.02%	0.002%
44	8.709	2381	2385	2391	rBV3	513	528	0.03%	0.004%
45	8.844	2414	2427	2459	rBV	860680	1428416	89.14%	10.464%
46	9.130	2513	2516	2518	rBV4	560	368	0.02%	0.003%
47	9.201	2536	2538	2545	rVV4	591	714	0.04%	0.005%
48	9.236	2545	2549	2553	rVB4	364	294	0.02%	0.002%
49	9.291	2562	2566	2571	rVV3	388	341	0.02%	0.002%
50	9.352	2581	2585	2587	rBV3	330	282	0.02%	0.002%
51	9.535	2635	2642	2646	rBV4	898	1031	0.06%	0.008%
52	9.690	2683	2690	2692	rBV3	267	308	0.02%	0.002%
53	9.715	2692	2698	2701	rVV4	485	401	0.03%	0.003%
54	9.783	2715	2719	2725	rBV2	307	342	0.02%	0.003%
55	9.857	2736	2742	2745	rVB2	519	561	0.04%	0.004%
56	9.892	2749	2753	2756	rVV3	391	323	0.02%	0.002%
57	9.924	2760	2763	2772	rVB4	634	738	0.05%	0.005%
58	9.998	2780	2786	2790	rBV3	509	498	0.03%	0.004%
59	10.018	2790	2792	2797	rVB2	421	303	0.02%	0.002%
60	10.165	2828	2838	2840	rBV2	12801	16486	1.03%	0.121%
61	10.207	2841	2851	2871	rVB	542074	854972	53.36%	6.263%
62	10.378	2890	2904	2915	rVB3	4588	8404	0.52%	0.062%
63	10.423	2915	2918	2927	rVB5	474	548	0.03%	0.004%
64	10.535	2945	2953	2956	rBV3	601	763	0.05%	0.006%
65	10.571	2956	2964	2971	rBV2	4466	6730	0.42%	0.049%
66	10.641	2980	2986	2990	rBV3	351	406	0.03%	0.003%
67	10.908	3061	3069	3076	rBV4	1195	1574	0.10%	0.012%
68	10.982	3090	3092	3096	rBV2	373	305	0.02%	0.002%
69	11.172	3139	3151	3160	rBV	38273	61887	3.86%	0.453%
70	11.236	3160	3171	3195	rVV	962002	1602382	100.00%	11.738%
71	11.455	3237	3239	3244	rVB3	529	350	0.02%	0.003%
72	11.516	3256	3258	3261	rBV3	452	384	0.02%	0.003%
73	11.554	3263	3270	3276	rVV7	1905	3076	0.19%	0.023%
74	11.612	3276	3288	3319	rVB	806138	1342394	83.77%	9.834%
75	11.776	3337	3339	3345	rVB3	688	488	0.03%	0.004%
76	11.812	3345	3350	3352	rBV4	688	601	0.04%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
 Data File : VV029496.D
 Acq On : 09 Dec 2022 00:27
 Operator : SY/MD
 Sample : N5915-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5N05

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	11.898	3372	3377	3381	rBV4	882	840	0.05%	0.006%
78	12.005	3402	3410	3417	rBV2	1733	2430	0.15%	0.018%
79	12.120	3442	3446	3449	rBV3	1030	975	0.06%	0.007%
80	12.236	3475	3482	3490	rVB8	2061	3065	0.19%	0.022%
81	12.304	3500	3503	3511	rVB5	1403	1292	0.08%	0.009%
82	12.403	3526	3534	3540	rBV3	2356	3123	0.19%	0.023%
83	12.451	3544	3549	3557	rVB4	1229	1565	0.10%	0.011%
84	12.519	3566	3570	3572	rBV3	368	347	0.02%	0.003%
85	12.577	3586	3588	3593	rVB3	392	295	0.02%	0.002%
86	12.609	3593	3598	3601	rBV3	393	414	0.03%	0.003%
87	12.635	3601	3606	3611	rBV4	404	534	0.03%	0.004%
88	12.873	3671	3680	3689	rVV4	3588	5380	0.34%	0.039%
89	12.985	3713	3715	3720	rVB4	431	368	0.02%	0.003%
90	13.156	3765	3768	3771	rBV2	498	436	0.03%	0.003%
91	13.255	3790	3799	3807	rVV6	2689	4388	0.27%	0.032%
92	13.326	3819	3821	3827	rBV4	842	456	0.03%	0.003%
93	13.387	3838	3840	3843	rVB3	552	284	0.02%	0.002%
94	13.445	3855	3858	3861	rBV4	306	281	0.02%	0.002%
95	13.731	3940	3947	3954	rBV8	805	1289	0.08%	0.009%
96	14.043	4041	4044	4046	rBV3	849	569	0.04%	0.004%
97	14.168	4080	4083	4089	rVB6	1220	1233	0.08%	0.009%
98	14.358	4138	4142	4144	rBV5	742	672	0.04%	0.005%
99	14.648	4230	4232	4237	rVB4	756	452	0.03%	0.003%
100	14.892	4305	4308	4310	rBV3	1025	699	0.04%	0.005%


Sum of corrected areas: 13651149

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
Data File : VV029496.D
Acq On : 09 Dec 2022 00:27
Operator : SY/MD
Sample : N5915-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5N05

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

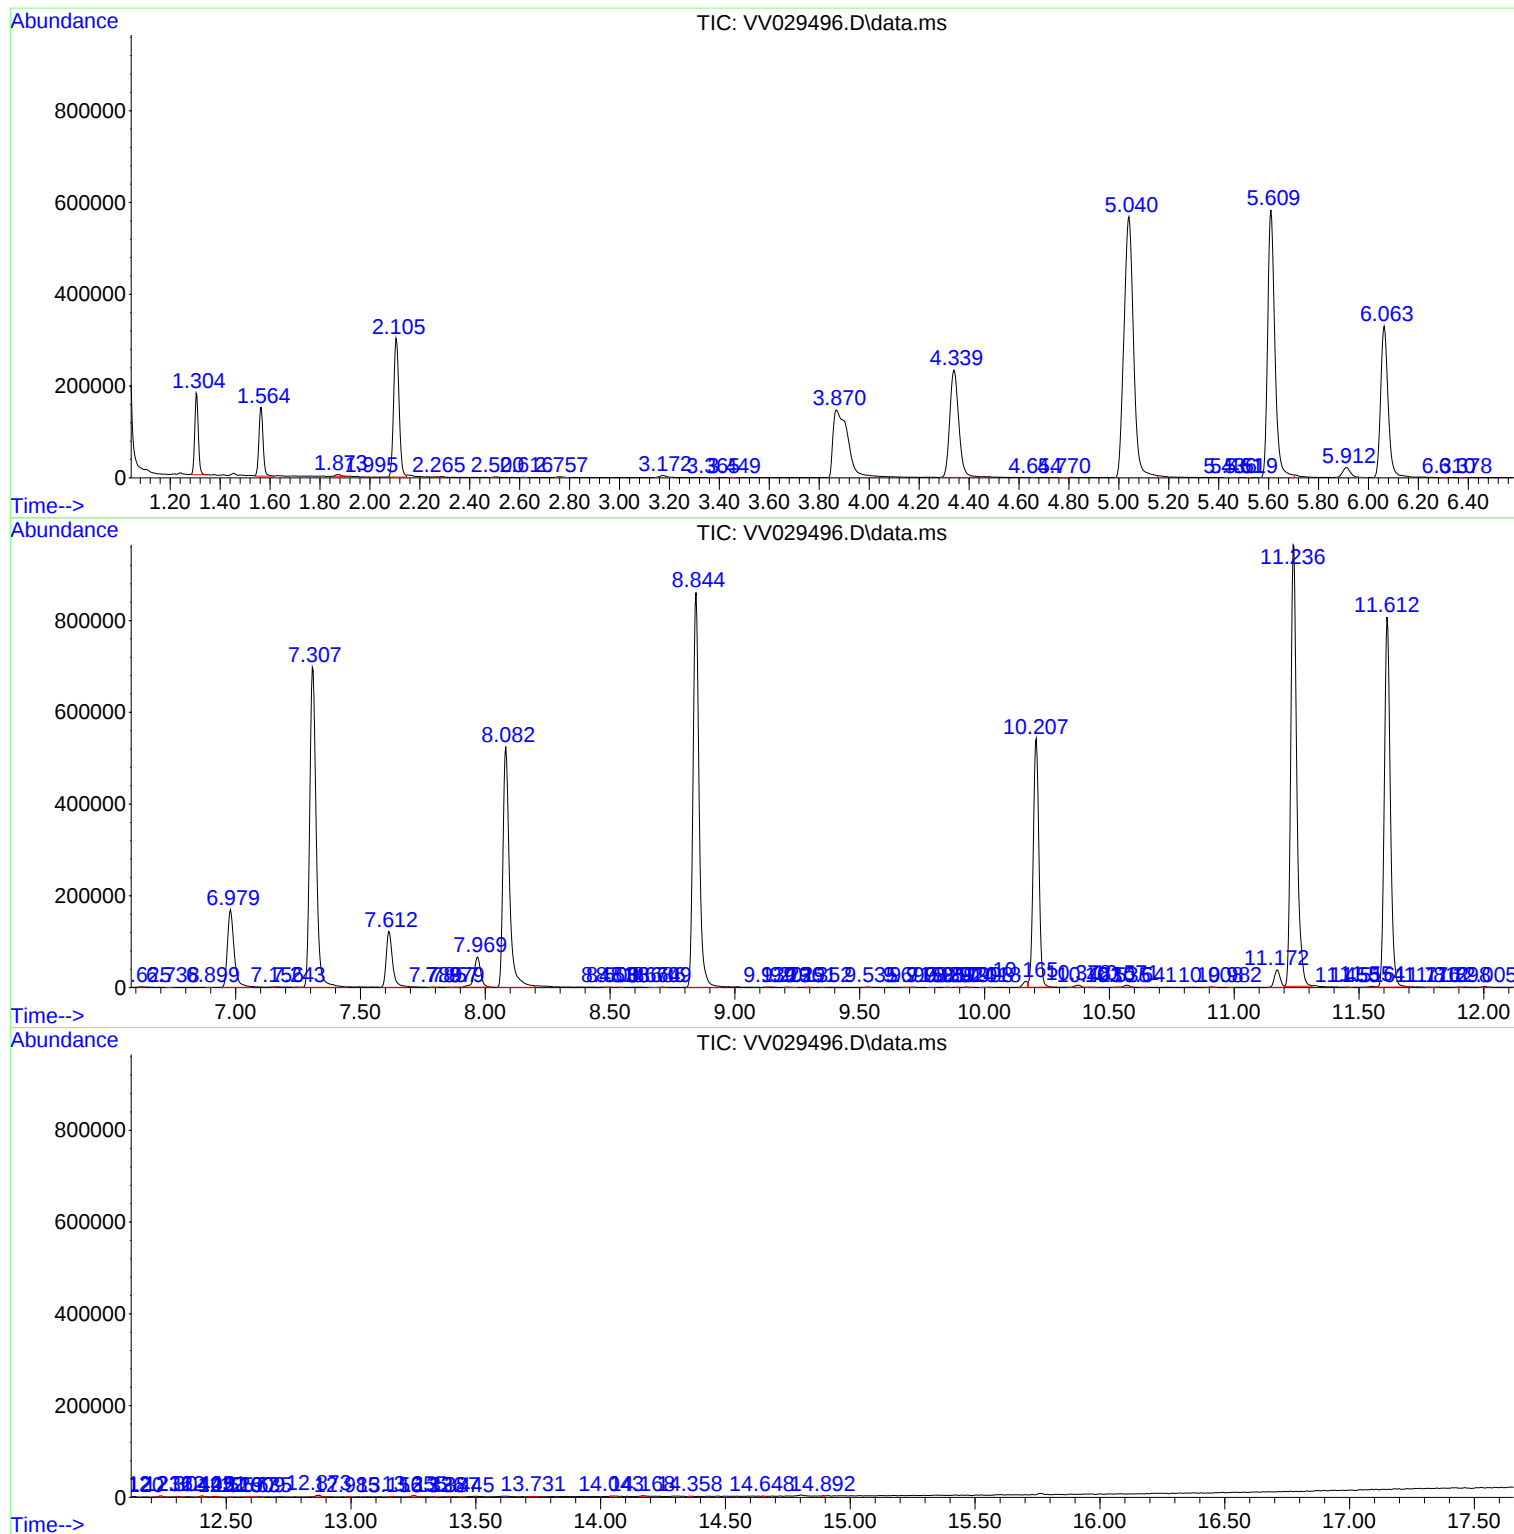

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
Data File : VV029496.D
Acq On : 09 Dec 2022 00:27
Operator : SY/MD
Sample : N5915-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5N05

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
Data File : VV029496.D
Acq On : 09 Dec 2022 00:27
Operator : SY/MD
Sample : N5915-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5N05

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------