

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
 Data File : VV029497.D
 Acq On : 09 Dec 2022 00:51
 Operator : SY/MD
 Sample : N5915-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5N06

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029497.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	100	rVB	169113	170921	11.10%	1.303%
2	1.564	155	163	180	rVB	155305	175521	11.40%	1.338%
3	2.018	301	304	305	rBV2	514	323	0.02%	0.002%
4	2.105	320	331	352	rBV2	304441	453102	29.42%	3.454%
5	2.269	379	382	384	rBV4	433	287	0.02%	0.002%
6	2.503	448	455	463	rBV5	1060	1619	0.11%	0.012%
7	2.590	478	482	486	rBV3	394	385	0.02%	0.003%
8	2.635	491	496	500	rVV2	483	407	0.03%	0.003%
9	2.687	509	512	518	rVB3	370	372	0.02%	0.003%
10	2.767	524	537	553	rVV3	12360	26096	1.69%	0.199%
11	2.937	585	590	595	rBV	428	356	0.02%	0.003%
12	3.043	619	623	628	rBV3	406	475	0.03%	0.004%
13	3.108	641	643	654	rVB3	361	551	0.04%	0.004%
14	3.188	654	668	679	rBV3	2209	4346	0.28%	0.033%
15	3.252	685	688	693	rBV3	378	270	0.02%	0.002%
16	3.333	710	713	720	rVB3	458	533	0.03%	0.004%
17	3.400	731	734	739	rVB2	280	252	0.02%	0.002%
18	3.468	751	755	758	rBV2	364	341	0.02%	0.003%
19	3.523	769	772	775	rBV	351	302	0.02%	0.002%
20	3.616	798	801	804	rVB3	434	297	0.02%	0.002%
21	3.870	870	880	921	rBV	124845	398600	25.88%	3.039%
22	4.336	1009	1025	1056	rVV	241421	603461	39.18%	4.601%
23	4.600	1102	1107	1110	rVB2	314	265	0.02%	0.002%
24	4.683	1131	1133	1137	rVB4	461	294	0.02%	0.002%
25	4.757	1151	1156	1157	rBV	305	261	0.02%	0.002%
26	4.889	1194	1197	1202	rVB3	279	287	0.02%	0.002%
27	5.040	1223	1244	1286	rBV2	576147	1540140	100.00%	11.742%
28	5.535	1394	1398	1401	rBV3	394	307	0.02%	0.002%
29	5.609	1407	1421	1453	rBV	577784	1175266	76.31%	8.960%
30	5.908	1500	1514	1530	rBV5	14880	33322	2.16%	0.254%
31	6.063	1547	1562	1598	rBV	338316	695772	45.18%	5.304%
32	6.448	1675	1682	1685	rVB3	452	519	0.03%	0.004%
33	6.497	1692	1697	1700	rVB3	267	246	0.02%	0.002%
34	6.522	1700	1705	1709	rBV3	279	309	0.02%	0.002%
35	6.590	1723	1726	1729	rBV2	437	396	0.03%	0.003%
36	6.625	1731	1737	1743	rBV5	1276	2062	0.13%	0.016%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120822\
 Data File : VW029497.D
 Acq On : 09 Dec 2022 00:51
 Operator : SY/MD
 Sample : N5915-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5N06

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.696	1754	1759	1762	rVB3	446	470	0.03%	0.004%
38	6.870	1810	1813	1818	rVB3	372	289	0.02%	0.002%
39	6.921	1825	1829	1832	rBV	331	284	0.02%	0.002%
40	6.979	1835	1847	1872	rBV	171429	317047	20.59%	2.417%
41	7.310	1937	1950	1987	rBV	713580	1265862	82.19%	9.651%
42	7.548	2021	2024	2025	rBV2	469	281	0.02%	0.002%
43	7.612	2034	2044	2069	rBV	122185	216424	14.05%	1.650%
44	7.764	2088	2091	2096	rBV5	373	385	0.02%	0.003%
45	7.934	2135	2144	2145	rBV3	4676	5558	0.36%	0.042%
46	7.969	2146	2155	2174	rVB	42002	73596	4.78%	0.561%
47	8.082	2179	2190	2235	rBV	436274	799871	51.93%	6.098%
48	8.493	2314	2318	2324	rVB4	740	941	0.06%	0.007%
49	8.529	2324	2329	2332	rBV3	516	461	0.03%	0.004%
50	8.583	2341	2346	2352	rBV4	532	718	0.05%	0.005%
51	8.612	2352	2355	2358	rBV3	482	380	0.02%	0.003%
52	8.657	2365	2369	2374	rBV2	461	470	0.03%	0.004%
53	8.844	2414	2427	2460	rBV	866953	1420090	92.21%	10.827%
54	9.130	2512	2516	2517	rBV3	376	249	0.02%	0.002%
55	9.140	2517	2519	2522	rVB2	527	292	0.02%	0.002%
56	9.323	2572	2576	2583	rVB3	343	384	0.02%	0.003%
57	9.365	2583	2589	2593	rBV2	364	318	0.02%	0.002%
58	9.403	2597	2601	2605	rVB2	390	311	0.02%	0.002%
59	9.532	2635	2641	2642	rBV3	328	298	0.02%	0.002%
60	9.628	2667	2671	2675	rVB3	352	276	0.02%	0.002%
61	9.661	2675	2681	2684	rBV3	304	305	0.02%	0.002%
62	9.863	2739	2744	2749	rVB4	334	318	0.02%	0.002%
63	9.921	2758	2762	2770	rVB3	579	686	0.04%	0.005%
64	9.953	2770	2772	2780	rVB4	393	483	0.03%	0.004%
65	10.162	2828	2837	2840	rBV2	12588	16279	1.06%	0.124%
66	10.207	2840	2851	2871	rVB	524415	831044	53.96%	6.336%
67	10.374	2891	2903	2915	rVB	6990	11442	0.74%	0.087%
68	10.532	2948	2952	2956	rBV4	365	439	0.03%	0.003%
69	10.567	2956	2963	2974	rVB	4729	7841	0.51%	0.060%
70	10.709	3003	3007	3011	rBV3	337	320	0.02%	0.002%
71	10.741	3011	3017	3021	rVB3	399	395	0.03%	0.003%
72	10.844	3045	3049	3056	rBV3	388	521	0.03%	0.004%
73	10.882	3056	3061	3064	rBV3	291	251	0.02%	0.002%
74	10.911	3064	3070	3077	rBV4	682	873	0.06%	0.007%
75	10.953	3077	3083	3085	rBV3	405	370	0.02%	0.003%
76	11.027	3103	3106	3110	rBV2	416	335	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
 Data File : VV029497.D
 Acq On : 09 Dec 2022 00:51
 Operator : SY/MD
 Sample : N5915-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5N06

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	11.098	3125	3128	3131	rBV2	530	248	0.02%	0.002%
78	11.175	3140	3152	3160	rBV	14476	22137	1.44%	0.169%
79	11.239	3160	3172	3198	rVV	945958	1514947	98.36%	11.550%
80	11.561	3264	3272	3276	rBV4	908	1575	0.10%	0.012%
81	11.612	3276	3288	3314	rVV	810078	1299502	84.38%	9.907%
82	11.808	3346	3349	3350	rBV2	585	296	0.02%	0.002%
83	12.001	3405	3409	3412	rBV2	434	332	0.02%	0.003%
84	12.162	3457	3459	3463	rBV	408	286	0.02%	0.002%
85	12.239	3479	3483	3491	rVB3	1992	2244	0.15%	0.017%
86	12.332	3510	3512	3514	rVB2	618	270	0.02%	0.002%
87	12.406	3533	3535	3540	rVB2	558	367	0.02%	0.003%
88	12.625	3598	3603	3605	rBV3	621	524	0.03%	0.004%
89	12.657	3610	3613	3618	rVB3	385	319	0.02%	0.002%
90	12.824	3660	3665	3668	rBV2	404	442	0.03%	0.003%
91	12.866	3674	3678	3682	rBV4	676	855	0.06%	0.007%
92	13.066	3737	3740	3743	rBV4	557	393	0.03%	0.003%
93	13.255	3789	3799	3807	rBV5	1494	2338	0.15%	0.018%
94	13.294	3807	3811	3814	rVB4	457	358	0.02%	0.003%
95	13.355	3824	3830	3834	rBV4	390	522	0.03%	0.004%
96	13.474	3864	3867	3870	rBV3	546	481	0.03%	0.004%
97	13.654	3920	3923	3925	rBV4	476	294	0.02%	0.002%
98	13.821	3972	3975	3977	rBV3	636	476	0.03%	0.004%
99	13.892	3995	3997	4002	rVB4	972	607	0.04%	0.005%
100	14.162	4077	4081	4085	rBV5	1313	1464	0.10%	0.011%




Sum of corrected areas: 13116697

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
Data File : VV029497.D
Acq On : 09 Dec 2022 00:51
Operator : SY/MD
Sample : N5915-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5N06

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

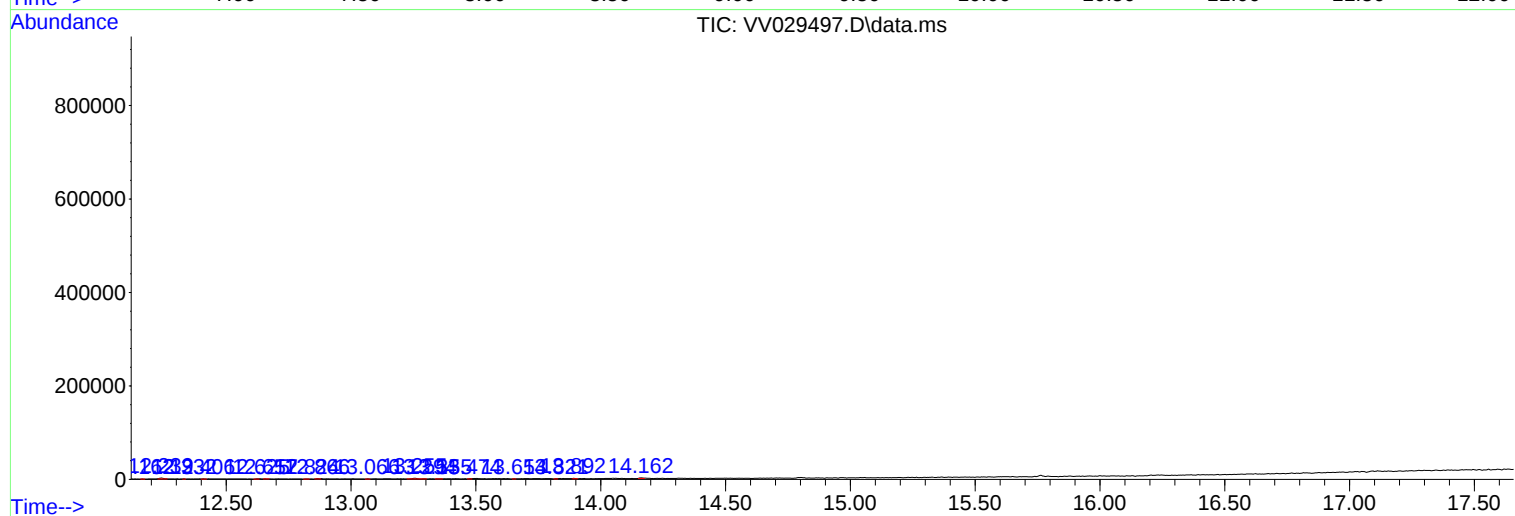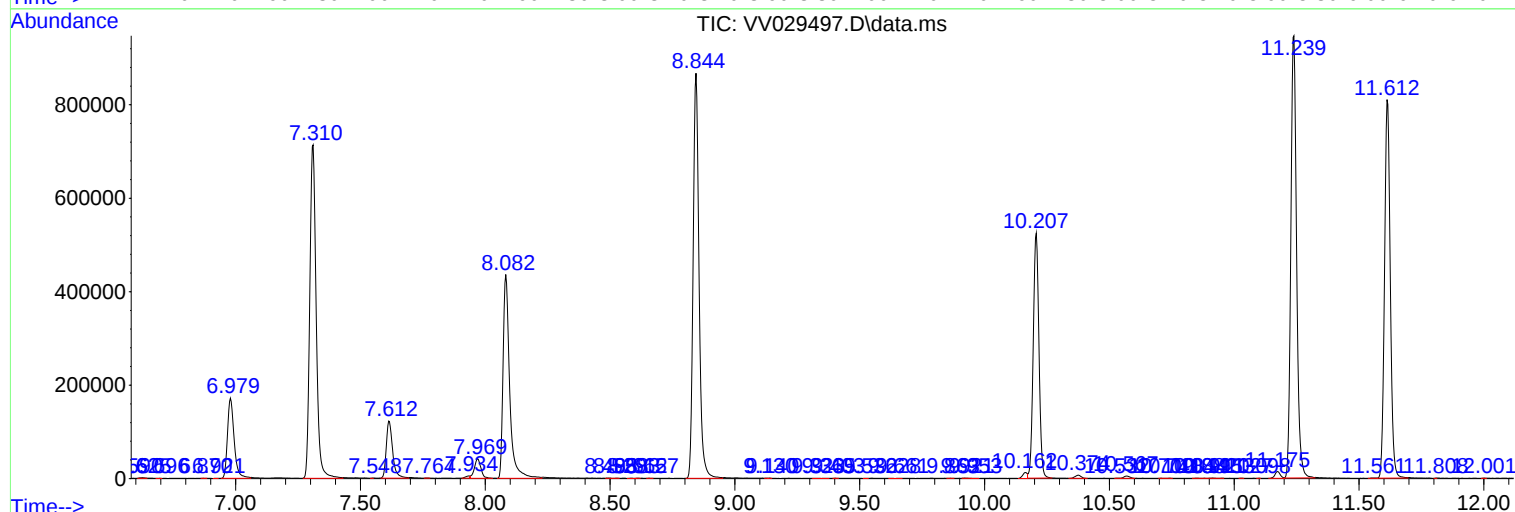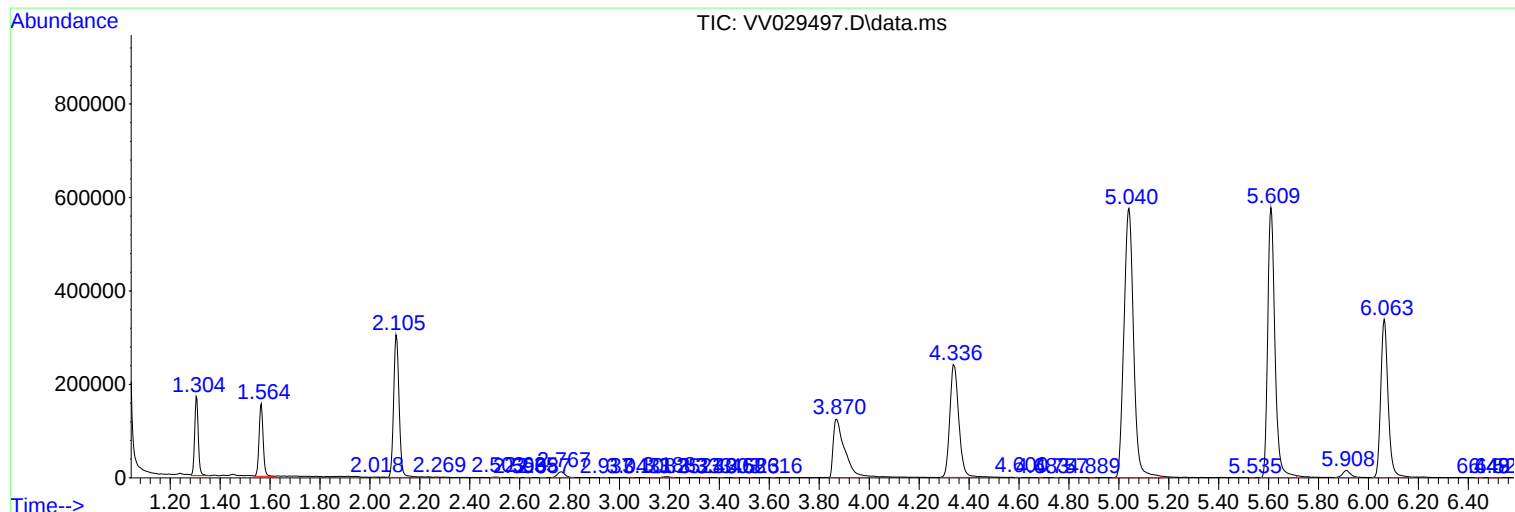

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
Data File : VV029497.D
Acq On : 09 Dec 2022 00:51
Operator : SY/MD
Sample : N5915-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5N06

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
Data File : VV029497.D
Acq On : 09 Dec 2022 00:51
Operator : SY/MD
Sample : N5915-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5N06

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc