

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
 Data File : VV029498.D
 Acq On : 09 Dec 2022 01:14
 Operator : SY/MD
 Sample : N5915-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5N07

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029498.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	100	rVB	166749	167064	11.02%	1.326%
2	1.564	156	163	176	rVB	146981	164566	10.86%	1.306%
3	2.105	321	331	345	rBV2	295279	434005	28.63%	3.445%
4	2.484	446	449	450	rBV2	422	233	0.02%	0.002%
5	2.764	523	536	549	rBV3	12474	25964	1.71%	0.206%
6	2.947	591	593	596	rBV	248	156	0.01%	0.001%
7	3.040	619	622	624	rBV2	226	168	0.01%	0.001%
8	3.079	631	634	639	rBV2	360	381	0.03%	0.003%
9	3.127	647	649	651	rVB	219	96	0.01%	0.001%
10	3.178	655	665	667	rBV3	1825	2171	0.14%	0.017%
11	3.236	679	683	689	rBV3	316	361	0.02%	0.003%
12	3.291	697	700	704	rVB	390	188	0.01%	0.001%
13	3.317	705	708	711	rVV2	230	131	0.01%	0.001%
14	3.362	719	722	728	rVB3	273	229	0.02%	0.002%
15	3.455	744	751	753	rBV2	171	201	0.01%	0.002%
16	3.506	765	767	768	rBV2	230	90	0.01%	0.001%
17	3.568	783	786	789	rBV2	154	131	0.01%	0.001%
18	3.661	812	815	817	rBV2	179	135	0.01%	0.001%
19	3.690	821	824	828	rVB2	295	169	0.01%	0.001%
20	3.709	828	830	835	rBV2	265	217	0.01%	0.002%
21	3.738	835	839	841	rBV	184	150	0.01%	0.001%
22	3.777	849	851	854	rVB	371	195	0.01%	0.002%
23	3.867	870	879	920	rBV	120874	356910	23.54%	2.833%
24	4.339	1010	1026	1060	rBV	235323	589373	38.88%	4.678%
25	4.580	1099	1101	1105	rBV2	349	186	0.01%	0.001%
26	4.654	1122	1124	1127	rVV2	283	132	0.01%	0.001%
27	4.744	1149	1152	1157	rVB2	271	187	0.01%	0.001%
28	4.773	1157	1161	1163	rBV2	120	99	0.01%	0.001%
29	4.789	1163	1166	1171	rVB2	249	155	0.01%	0.001%
30	4.844	1180	1183	1185	rBV	237	144	0.01%	0.001%
31	4.895	1197	1199	1201	rVB2	192	86	0.01%	0.001%
32	5.040	1225	1244	1298	rBV2	568794	1515972	100.00%	12.032%
33	5.336	1333	1336	1338	rVB2	333	170	0.01%	0.001%
34	5.410	1357	1359	1360	rBV	307	109	0.01%	0.001%
35	5.461	1373	1375	1376	rBV	300	150	0.01%	0.001%
36	5.500	1385	1387	1391	rVB3	413	256	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
 Data File : VV029498.D
 Acq On : 09 Dec 2022 01:14
 Operator : SY/MD
 Sample : N5915-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5N07

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	5.609	1408	1421	1460	rBV	568508	1158759	76.44%	9.197%
38	5.908	1504	1514	1531	rVB6	10203	24666	1.63%	0.196%
39	5.998	1538	1542	1546	rBV3	401	277	0.02%	0.002%
40	6.063	1548	1562	1600	rBV	330968	685795	45.24%	5.443%
41	6.346	1648	1650	1654	rVB2	392	206	0.01%	0.002%
42	6.374	1656	1659	1662	rBV	227	138	0.01%	0.001%
43	6.442	1678	1680	1682	rBV	292	140	0.01%	0.001%
44	6.455	1682	1684	1687	rVV2	217	107	0.01%	0.001%
45	6.490	1692	1695	1701	rVB3	387	284	0.02%	0.002%
46	6.574	1719	1721	1724	rBV2	213	116	0.01%	0.001%
47	6.609	1728	1732	1733	rBV	633	366	0.02%	0.003%
48	6.670	1749	1751	1752	rBV	350	103	0.01%	0.001%
49	6.702	1759	1761	1764	rVB2	275	109	0.01%	0.001%
50	6.773	1781	1783	1785	rBV2	274	151	0.01%	0.001%
51	6.809	1788	1794	1797	rVB2	257	295	0.02%	0.002%
52	6.821	1797	1798	1800	rBV	256	87	0.01%	0.001%
53	6.847	1802	1806	1809	rVB3	301	226	0.01%	0.002%
54	6.876	1812	1815	1818	rBV2	179	131	0.01%	0.001%
55	6.902	1821	1823	1825	rVB2	292	143	0.01%	0.001%
56	6.918	1825	1828	1831	rBV2	184	143	0.01%	0.001%
57	6.979	1834	1847	1881	rBV	168804	315409	20.81%	2.503%
58	7.262	1933	1935	1937	rBV2	262	123	0.01%	0.001%
59	7.307	1937	1949	1984	rBV	703232	1249529	82.42%	9.917%
60	7.612	2034	2044	2070	rBV	118689	211014	13.92%	1.675%
61	7.854	2117	2119	2122	rBV3	325	115	0.01%	0.001%
62	8.082	2179	2190	2225	rBV	433929	784167	51.73%	6.224%
63	8.545	2332	2334	2335	rBV	249	98	0.01%	0.001%
64	8.593	2345	2349	2352	rBV3	368	329	0.02%	0.003%
65	8.632	2358	2361	2362	rBV	370	249	0.02%	0.002%
66	8.670	2370	2373	2377	rBV3	409	335	0.02%	0.003%
67	8.693	2377	2380	2381	rBV	204	108	0.01%	0.001%
68	8.760	2397	2401	2403	rBV3	250	224	0.01%	0.002%
69	8.844	2414	2427	2460	rBV	854051	1399639	92.33%	11.109%
70	9.127	2514	2515	2518	rBV	403	260	0.02%	0.002%
71	9.198	2536	2537	2540	rVB	330	124	0.01%	0.001%
72	9.214	2540	2542	2543	rBV	182	83	0.01%	0.001%
73	9.271	2557	2560	2562	rBV2	369	194	0.01%	0.002%
74	9.291	2564	2566	2569	rVB2	291	122	0.01%	0.001%
75	9.323	2574	2576	2582	rVB2	310	259	0.02%	0.002%
76	9.435	2608	2611	2614	rVB2	249	162	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
 Data File : VV029498.D
 Acq On : 09 Dec 2022 01:14
 Operator : SY/MD
 Sample : N5915-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5N07

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	9.619	2666	2668	2669	rBV2	203	79	0.01%	0.001%
78	9.661	2675	2681	2685	rBV2	267	285	0.02%	0.002%
79	9.686	2686	2689	2692	rVB	345	213	0.01%	0.002%
80	9.722	2697	2700	2703	rBV3	196	160	0.01%	0.001%
81	9.799	2720	2724	2726	rBV2	245	162	0.01%	0.001%
82	9.866	2741	2745	2750	rBB3	216	181	0.01%	0.001%
83	10.059	2801	2805	2807	rBV2	196	175	0.01%	0.001%
84	10.162	2829	2837	2840	rBV2	12291	15746	1.04%	0.125%
85	10.207	2841	2851	2882	rVB	526845	828042	54.62%	6.572%
86	10.371	2897	2902	2915	rVB3	4974	7840	0.52%	0.062%
87	10.435	2920	2922	2924	rVB	260	112	0.01%	0.001%
88	10.519	2946	2948	2950	rBV	345	138	0.01%	0.001%
89	10.567	2956	2963	2976	rVB2	5024	7755	0.51%	0.062%
90	10.741	3015	3017	3019	rBV2	255	154	0.01%	0.001%
91	10.847	3043	3050	3054	rBV3	572	580	0.04%	0.005%
92	10.902	3064	3067	3069	rBV2	462	300	0.02%	0.002%
93	11.078	3120	3122	3127	rVB2	328	195	0.01%	0.002%
94	11.104	3127	3130	3132	rBV	260	146	0.01%	0.001%
95	11.172	3143	3151	3159	rBV2	7413	11712	0.77%	0.093%
96	11.239	3160	3172	3193	rVV	893144	1415077	93.34%	11.231%
97	11.480	3245	3247	3250	rVB2	252	122	0.01%	0.001%
98	11.506	3253	3255	3258	rBV3	302	158	0.01%	0.001%
99	11.612	3275	3288	3311	rBV	757341	1213829	80.07%	9.634%
100	12.175	3460	3463	3471	rVB3	422	445	0.03%	0.004%




Sum of corrected areas: 12599321

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
Data File : VV029498.D
Acq On : 09 Dec 2022 01:14
Operator : SY/MD
Sample : N5915-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5N07

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

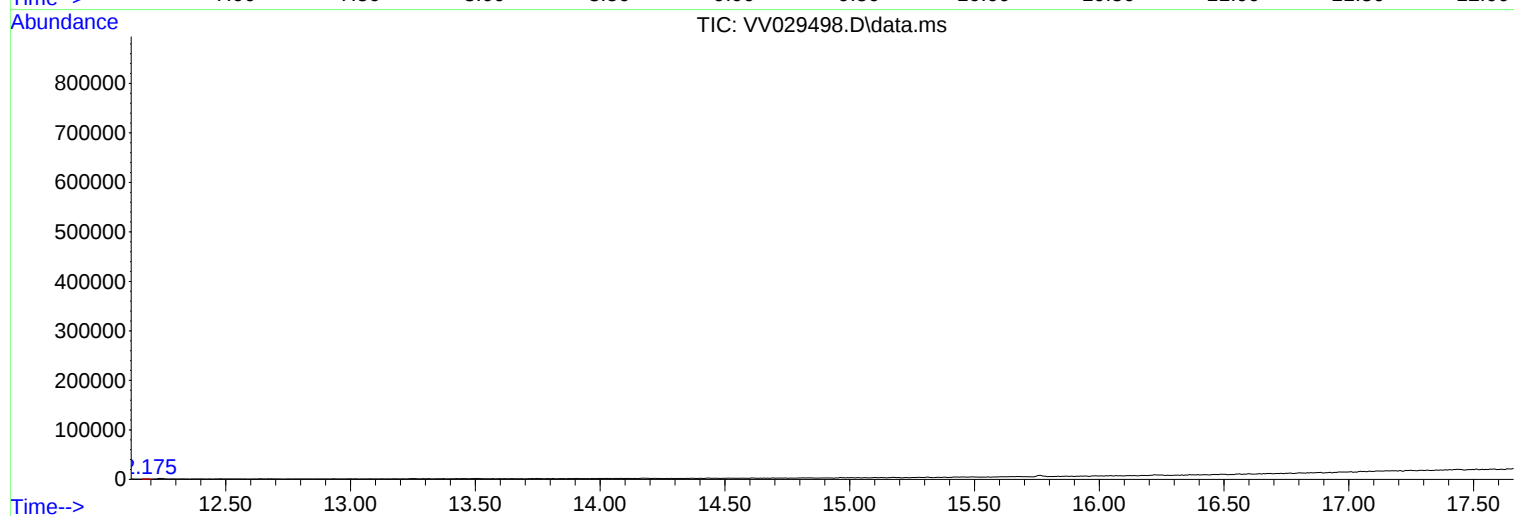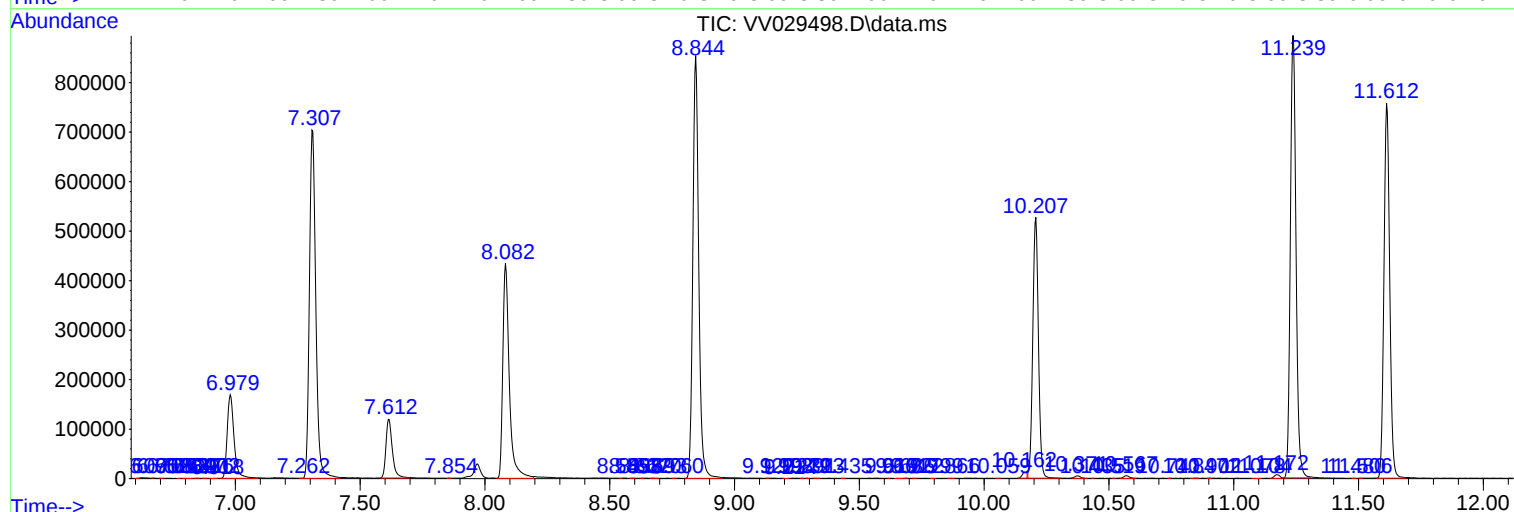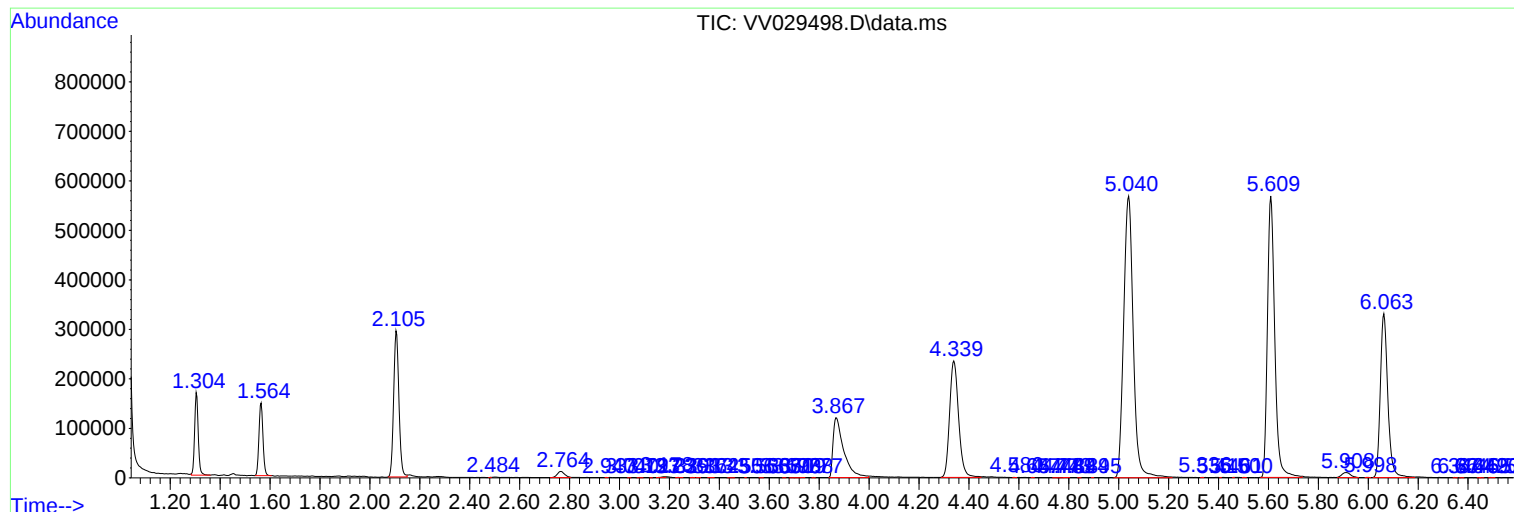

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
Data File : VV029498.D
Acq On : 09 Dec 2022 01:14
Operator : SY/MD
Sample : N5915-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5N07

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
Data File : VV029498.D
Acq On : 09 Dec 2022 01:14
Operator : SY/MD
Sample : N5915-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5N07

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc