

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
 Data File : VV029499.D
 Acq On : 09 Dec 2022 01:38
 Operator : SY/MD
 Sample : N5915-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5N08

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029499.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	101	rVB2	198544	207615	1.73%	0.781%
2	1.413	113	116	123	rVB	5175	4502	0.04%	0.017%
3	1.564	155	163	178	rVB	147639	165136	1.38%	0.621%
4	2.034	306	309	310	rBV	522	253	0.00%	0.001%
5	2.105	320	331	345	rBV	290335	425494	3.55%	1.601%
6	2.233	365	371	381	rVV2	3065	4831	0.04%	0.018%
7	2.291	384	389	397	rVB3	1471	2140	0.02%	0.008%
8	2.506	447	456	464	rVB2	2063	3318	0.03%	0.012%
9	2.616	478	490	506	rBV2	21879	46135	0.39%	0.174%
10	2.764	518	536	554	rBV	264674	545943	4.56%	2.054%
11	2.902	577	579	582	rVB2	529	275	0.00%	0.001%
12	2.947	582	593	611	rVB3	4172	10159	0.08%	0.038%
13	3.182	649	666	687	rBV	88429	187314	1.56%	0.705%
14	3.272	691	694	695	rBV3	995	563	0.00%	0.002%
15	3.902	870	890	933	rBV2	681555	1938398	16.18%	7.292%
16	4.336	1008	1025	1058	rBV2	266708	680526	5.68%	2.560%
17	4.667	1117	1128	1143	rBV8	4268	10555	0.09%	0.040%
18	4.780	1159	1163	1165	rBV3	602	397	0.00%	0.001%
19	4.879	1189	1194	1201	rBV2	284	366	0.00%	0.001%
20	5.040	1224	1244	1258	rBV2	555688	1472892	12.29%	5.541%
21	5.403	1354	1357	1359	rVV	415	270	0.00%	0.001%
22	5.477	1375	1380	1383	rBV3	327	277	0.00%	0.001%
23	5.609	1406	1421	1467	rBV	546155	1125875	9.40%	4.235%
24	5.764	1467	1469	1474	rVB2	727	480	0.00%	0.002%
25	5.908	1502	1514	1540	rBV	114720	238992	1.99%	0.899%
26	6.063	1548	1562	1594	rBV	322993	665294	5.55%	2.503%
27	6.198	1601	1604	1606	rBV3	645	475	0.00%	0.002%
28	6.381	1653	1661	1671	rBV4	1822	3446	0.03%	0.013%
29	6.474	1684	1690	1693	rBV2	306	273	0.00%	0.001%
30	6.622	1729	1736	1738	rBV2	1321	1464	0.01%	0.006%
31	6.683	1753	1755	1759	rVB3	402	247	0.00%	0.001%
32	6.931	1829	1832	1835	rBV	491	340	0.00%	0.001%
33	6.979	1835	1847	1872	rBV	171659	315180	2.63%	1.186%
34	7.140	1894	1897	1898	rBV	360	249	0.00%	0.001%
35	7.149	1898	1900	1902	rBV2	425	248	0.00%	0.001%
36	7.246	1928	1930	1937	rVB4	811	704	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
 Data File : VV029499.D
 Acq On : 09 Dec 2022 01:38
 Operator : SY/MD
 Sample : N5915-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5N08

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	7.307	1937	1949	1970	rBV	690710	1211774	10.11%	4.558%
38	7.612	2034	2044	2077	rBV	122868	216763	1.81%	0.815%
39	7.776	2091	2095	2098	rBV5	512	448	0.00%	0.002%
40	7.934	2134	2144	2146	rVV2	5420	7444	0.06%	0.028%
41	7.969	2148	2155	2174	rVB2	22593	40792	0.34%	0.153%
42	8.040	2174	2177	2179	rBV2	351	252	0.00%	0.001%
43	8.082	2179	2190	2230	rBV	422291	752193	6.28%	2.830%
44	8.326	2257	2266	2279	rVB2	5462	9999	0.08%	0.038%
45	8.455	2304	2306	2311	rVB3	477	353	0.00%	0.001%
46	8.484	2311	2315	2317	rBV2	368	315	0.00%	0.001%
47	8.715	2373	2387	2400	rBV	3810	7450	0.06%	0.028%
48	8.873	2415	2436	2473	rBV2	6624927	11982315	100.00%	45.074%
49	9.120	2506	2513	2514	rBV6	3097	2944	0.02%	0.011%
50	9.172	2526	2529	2531	rBV3	643	455	0.00%	0.002%
51	9.316	2571	2574	2579	rVB4	589	487	0.00%	0.002%
52	9.410	2597	2603	2606	rBV3	385	370	0.00%	0.001%
53	9.429	2606	2609	2613	rBV3	382	277	0.00%	0.001%
54	9.538	2634	2643	2655	rVB4	3675	6097	0.05%	0.023%
55	9.683	2685	2688	2691	rVB2	344	268	0.00%	0.001%
56	9.747	2703	2708	2711	rVB3	331	241	0.00%	0.001%
57	9.921	2753	2762	2776	rVB	13805	20852	0.17%	0.078%
58	10.085	2807	2813	2817	rBV4	320	349	0.00%	0.001%
59	10.107	2817	2820	2823	rBV3	388	278	0.00%	0.001%
60	10.162	2827	2837	2840	rVV4	15867	22169	0.19%	0.083%
61	10.207	2841	2851	2879	rVB	498956	792237	6.61%	2.980%
62	10.339	2888	2892	2893	rBV3	656	483	0.00%	0.002%
63	10.374	2893	2903	2911	rVV3	6438	10475	0.09%	0.039%
64	10.416	2911	2916	2925	rVB4	2426	3344	0.03%	0.013%
65	10.451	2925	2927	2931	rBV	372	241	0.00%	0.001%
66	10.567	2956	2963	2972	rBV2	3750	5283	0.04%	0.020%
67	10.725	3005	3012	3019	rBV3	912	1417	0.01%	0.005%
68	10.853	3048	3052	3054	rBV3	391	367	0.00%	0.001%
69	10.873	3054	3058	3061	rVV3	398	343	0.00%	0.001%
70	10.905	3064	3068	3073	rVV4	806	867	0.01%	0.003%
71	11.085	3117	3124	3128	rBV4	769	983	0.01%	0.004%
72	11.130	3135	3138	3139	rBV	499	258	0.00%	0.001%
73	11.169	3139	3150	3161	rBV	352118	538783	4.50%	2.027%
74	11.239	3161	3172	3174	rBV	1023732	1296957	10.82%	4.879%
75	11.439	3231	3234	3239	rBV4	594	444	0.00%	0.002%
76	11.519	3250	3259	3266	rBV3	5695	8422	0.07%	0.032%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
 Data File : VV029499.D
 Acq On : 09 Dec 2022 01:38
 Operator : SY/MD
 Sample : N5915-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5N08

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	11.612	3275	3288	3312	rBV2	819864	1558494	13.01%	5.863%
78	11.734	3322	3326	3335	rVB5	1137	1357	0.01%	0.005%
79	11.934	3384	3388	3390	rBV2	498	386	0.00%	0.001%
80	12.001	3407	3409	3414	rBV2	436	285	0.00%	0.001%
81	12.120	3434	3446	3456	rBV6	1683	3594	0.03%	0.014%
82	12.207	3468	3473	3475	rBV	358	312	0.00%	0.001%
83	12.239	3476	3483	3492	rVV3	2010	3074	0.03%	0.012%
84	12.394	3527	3531	3534	rBV3	401	426	0.00%	0.002%
85	12.445	3539	3547	3555	rVV4	1320	2382	0.02%	0.009%
86	12.599	3592	3595	3599	rVB4	547	341	0.00%	0.001%
87	12.641	3606	3608	3610	rVB2	531	278	0.00%	0.001%
88	12.869	3676	3679	3681	rBV2	623	458	0.00%	0.002%
89	12.930	3696	3698	3702	rVB2	540	350	0.00%	0.001%
90	12.953	3702	3705	3708	rBV2	527	442	0.00%	0.002%
91	13.040	3728	3732	3734	rBV3	460	393	0.00%	0.001%
92	13.120	3753	3757	3759	rBV2	387	290	0.00%	0.001%
93	13.242	3790	3795	3796	rBV	652	497	0.00%	0.002%
94	13.445	3855	3858	3863	rBV4	561	506	0.00%	0.002%
95	13.493	3870	3873	3877	rBV4	896	800	0.01%	0.003%
96	13.731	3945	3947	3952	rVB3	797	540	0.00%	0.002%
97	13.821	3971	3975	3978	rBV4	649	550	0.00%	0.002%
98	13.995	4025	4029	4030	rBV2	496	383	0.00%	0.001%
99	14.098	4058	4061	4065	rBV5	638	561	0.00%	0.002%
100	14.651	4229	4233	4234	rBV2	825	624	0.01%	0.002%




Sum of corrected areas: 26583738

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
Data File : VV029499.D
Acq On : 09 Dec 2022 01:38
Operator : SY/MD
Sample : N5915-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5N08

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

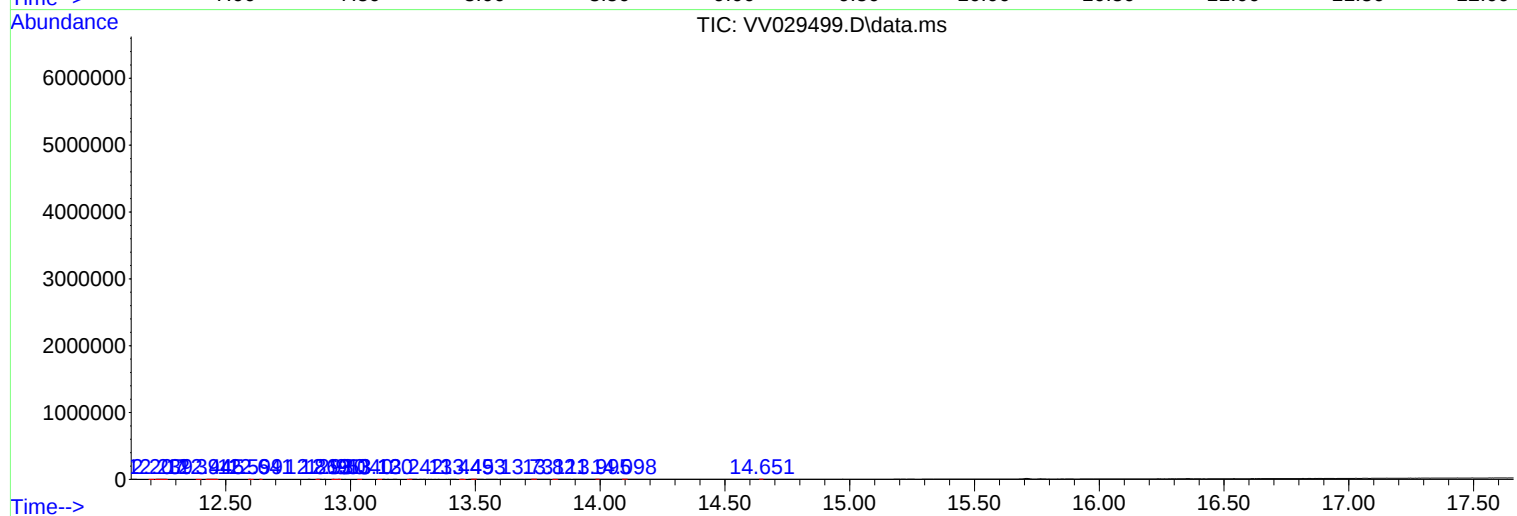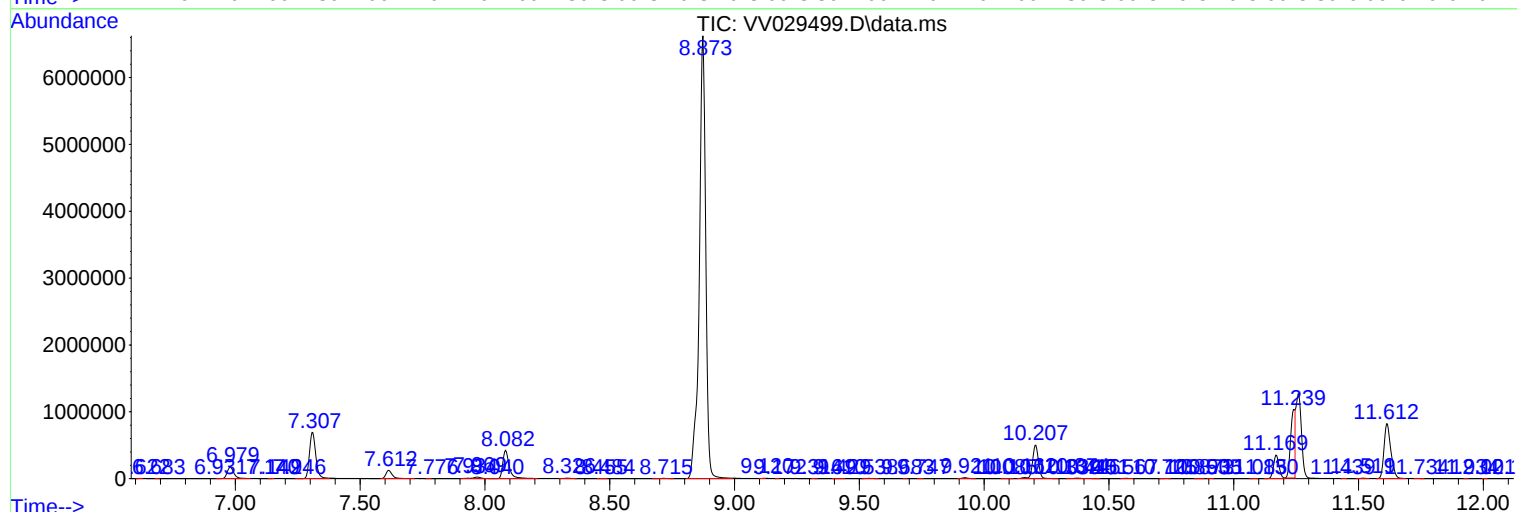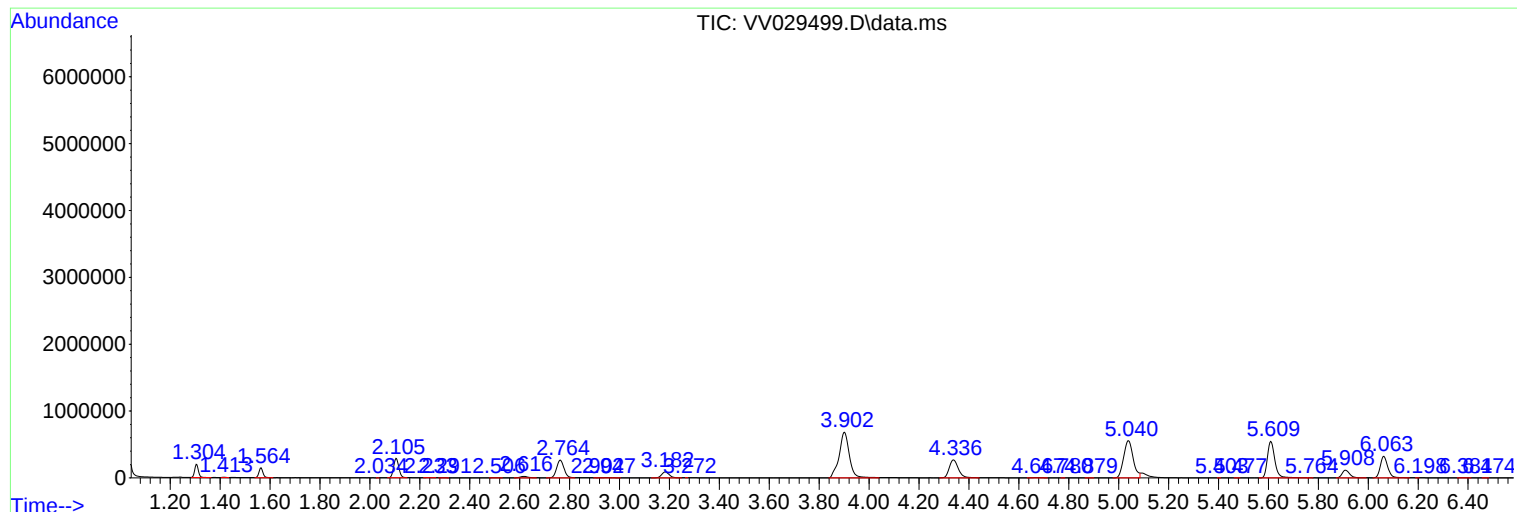

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
Data File : VV029499.D
Acq On : 09 Dec 2022 01:38
Operator : SY/MD
Sample : N5915-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5N08

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
Data File : VV029499.D
Acq On : 09 Dec 2022 01:38
Operator : SY/MD
Sample : N5915-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5N08

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------