

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
 Data File : VV029500.D
 Acq On : 09 Dec 2022 02:01
 Operator : SY/MD
 Sample : N5915-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5N09

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029500.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	100	rVB2	546996	566823	0.20%	0.093%
2	1.564	155	163	178	rVB	150691	172155	0.06%	0.028%
3	2.105	320	331	344	rBV	292278	424623	0.15%	0.070%
4	2.201	355	361	367	rBV	6059	8201	0.00%	0.001%
5	2.294	385	390	400	rVB	2169	3025	0.00%	0.000%
6	2.407	421	425	427	rBV2	263	212	0.00%	0.000%
7	2.503	446	455	464	rBV4	3337	5401	0.00%	0.001%
8	2.619	481	491	493	rBV5	1311	2124	0.00%	0.000%
9	2.703	513	517	521	rVB3	413	348	0.00%	0.000%
10	2.757	521	534	558	rBV	105747	188619	0.07%	0.031%
11	3.002	608	610	615	rVB2	344	209	0.00%	0.000%
12	3.027	615	618	623	rBV2	326	284	0.00%	0.000%
13	3.182	653	666	678	rBV3	8608	19283	0.01%	0.003%
14	3.285	696	698	707	rVB2	303	361	0.00%	0.000%
15	3.333	707	713	719	rBV3	367	466	0.00%	0.000%
16	3.542	775	778	785	rBV2	310	366	0.00%	0.000%
17	3.751	834	843	848	rBV4	826	1057	0.00%	0.000%
18	3.902	869	890	923	rBV2	440117	1327759	0.48%	0.218%
19	4.182	973	977	982	rVB3	432	518	0.00%	0.000%
20	4.339	1007	1026	1051	rBV	231632	574691	0.21%	0.094%
21	4.670	1117	1129	1142	rVV8	3457	7907	0.00%	0.001%
22	4.738	1148	1150	1159	rVB2	265	254	0.00%	0.000%
23	4.776	1159	1162	1166	rBV2	400	229	0.00%	0.000%
24	5.040	1226	1244	1251	rBV2	567858	1393848	0.50%	0.229%
25	5.092	1253	1260	1306	rVB	965140	2091724	0.75%	0.343%
26	5.326	1330	1333	1336	rBV3	680	518	0.00%	0.000%
27	5.362	1336	1344	1355	rVV3	4017	7944	0.00%	0.001%
28	5.471	1376	1378	1385	rVB	650	645	0.00%	0.000%
29	5.609	1408	1421	1474	rBV	578999	1186971	0.43%	0.195%
30	5.838	1490	1492	1499	rVB2	260	249	0.00%	0.000%
31	5.911	1504	1515	1531	rVB8	7797	17830	0.01%	0.003%
32	6.063	1548	1562	1593	rBV	324271	681910	0.24%	0.112%
33	6.236	1613	1616	1618	rVV2	497	301	0.00%	0.000%
34	6.320	1634	1642	1644	rBV3	402	444	0.00%	0.000%
35	6.365	1654	1656	1660	rVB2	442	228	0.00%	0.000%
36	6.391	1660	1664	1668	rBV3	374	335	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
 Data File : VV029500.D
 Acq On : 09 Dec 2022 02:01
 Operator : SY/MD
 Sample : N5915-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5N09

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.420	1671	1673	1676	rBV	375	219	0.00%	0.000%
38	6.458	1681	1685	1691	rVB2	290	247	0.00%	0.000%
39	6.558	1710	1716	1717	rBV2	410	259	0.00%	0.000%
40	6.625	1729	1737	1741	rBV4	1357	2175	0.00%	0.000%
41	6.699	1758	1760	1766	rVB4	660	651	0.00%	0.000%
42	6.735	1766	1771	1773	rBV	307	234	0.00%	0.000%
43	6.799	1781	1791	1802	rBV4	3340	6506	0.00%	0.001%
44	6.899	1816	1822	1825	rBV3	327	364	0.00%	0.000%
45	6.921	1825	1829	1833	rVB3	293	291	0.00%	0.000%
46	6.979	1836	1847	1871	rBV	163282	297056	0.11%	0.049%
47	7.149	1897	1900	1904	rBV2	737	770	0.00%	0.000%
48	7.169	1904	1906	1910	rVB2	580	375	0.00%	0.000%
49	7.239	1926	1928	1930	rBV2	500	223	0.00%	0.000%
50	7.310	1937	1950	1965	rBV	704874	1228211	0.44%	0.201%
51	7.384	1966	1973	1991	rVB	63694	116140	0.04%	0.019%
52	7.616	2033	2045	2068	rBV	114185	206987	0.07%	0.034%
53	7.741	2082	2084	2090	rVB3	481	504	0.00%	0.000%
54	7.818	2106	2108	2113	rVB2	436	272	0.00%	0.000%
55	7.857	2118	2120	2124	rBV2	368	240	0.00%	0.000%
56	7.937	2132	2145	2146	rBV3	5683	7713	0.00%	0.001%
57	7.973	2148	2156	2174	rVB2	26158	46607	0.02%	0.008%
58	8.085	2180	2191	2224	rBV	422240	782472	0.28%	0.128%
59	8.625	2356	2359	2364	rVB3	314	305	0.00%	0.000%
60	8.690	2377	2379	2384	rVB3	325	282	0.00%	0.000%
61	8.725	2384	2390	2394	rVB3	462	503	0.00%	0.000%
62	8.918	2416	2450	2476	rBV4	78314153	279272181	100.00%	45.802%
63	9.104	2501	2508	2526	rVB	113306	194781	0.07%	0.032%
64	9.538	2635	2643	2660	rVB2	24618	41945	0.02%	0.007%
65	9.924	2754	2763	2775	rVB2	42774	66132	0.02%	0.011%
66	10.120	2822	2824	2827	rBV3	453	300	0.00%	0.000%
67	10.162	2828	2837	2841	rVV3	23314	33174	0.01%	0.005%
68	10.207	2842	2851	2872	rVB	501249	787121	0.28%	0.129%
69	10.345	2880	2894	2910	rBV	341356	519885	0.19%	0.085%
70	10.419	2910	2917	2926	rVV3	13713	22352	0.01%	0.004%
71	10.468	2926	2932	2944	rVV	7892	12346	0.00%	0.002%
72	10.529	2947	2951	2952	rVV3	2251	1577	0.00%	0.000%
73	10.570	2956	2964	2974	rVB2	11058	18717	0.01%	0.003%
74	10.731	3002	3014	3031	rVB	436512	671398	0.24%	0.110%
75	10.908	3061	3069	3081	rVB2	20995	32242	0.01%	0.005%
76	11.050	3099	3113	3117	rBV	107571	161756	0.06%	0.027%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
 Data File : VV029500.D
 Acq On : 09 Dec 2022 02:01
 Operator : SY/MD
 Sample : N5915-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5N09

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	11.082	3118	3123	3138	rVB	148204	220766	0.08%	0.036%
78	11.175	3138	3152	3164	rBV	4248577	6643503	2.38%	1.090%
79	11.278	3164	3184	3229	rVB2	60791486	112882139	40.42%	18.513%
80	11.522	3248	3260	3279	rVB	1058805	2034925	0.73%	0.334%
81	11.664	3280	3304	3319	rVV4	79344299	190906873	68.36%	31.310%
82	11.738	3322	3327	3342	rVV2	170503	276187	0.10%	0.045%
83	11.812	3344	3350	3367	rVB	46617	79642	0.03%	0.013%
84	12.008	3399	3411	3419	rBV	680029	1076606	0.39%	0.177%
85	12.104	3431	3441	3452	rBV	291044	448578	0.16%	0.074%
86	12.233	3476	3481	3490	rBV7	3424	5652	0.00%	0.001%
87	12.294	3492	3500	3510	rVB4	16145	32239	0.01%	0.005%
88	12.403	3516	3534	3546	rVB	385479	607001	0.22%	0.100%
89	12.545	3567	3578	3582	rBV	35027	63598	0.02%	0.010%
90	12.654	3599	3612	3618	rBV3	17207	38806	0.01%	0.006%
91	12.869	3663	3679	3690	rBV2	442160	721026	0.26%	0.118%
92	12.988	3709	3716	3722	rBV2	15307	24884	0.01%	0.004%
93	13.033	3723	3730	3746	rVB2	57772	102377	0.04%	0.017%
94	13.172	3767	3773	3779	rBV7	2869	4428	0.00%	0.001%
95	13.255	3788	3799	3813	rBV3	54472	89361	0.03%	0.015%
96	13.323	3813	3820	3828	rBV5	6315	8680	0.00%	0.001%
97	13.387	3835	3840	3847	rVB	6707	8699	0.00%	0.001%
98	13.493	3861	3873	3898	rBV	129638	230179	0.08%	0.038%
99	14.175	4083	4085	4090	rBV4	920	889	0.00%	0.000%
100	14.220	4094	4099	4107	rVB3	4694	6295	0.00%	0.001%




Sum of corrected areas: 609736708

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
Data File : VV029500.D
Acq On : 09 Dec 2022 02:01
Operator : SY/MD
Sample : N5915-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5N09

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

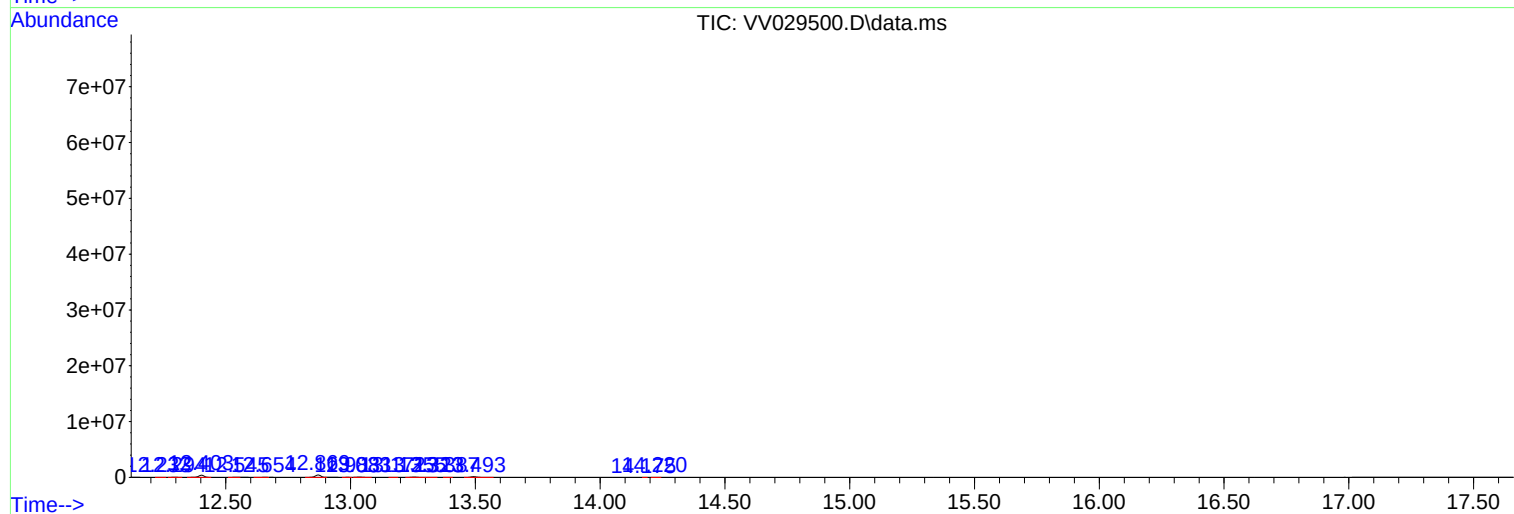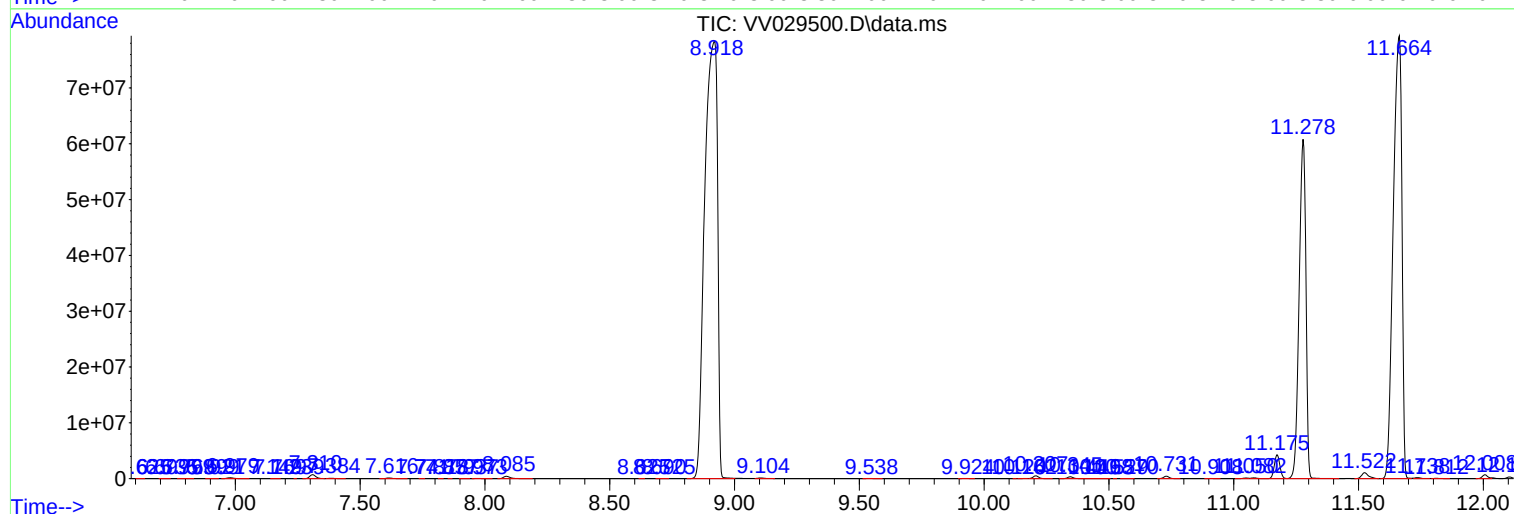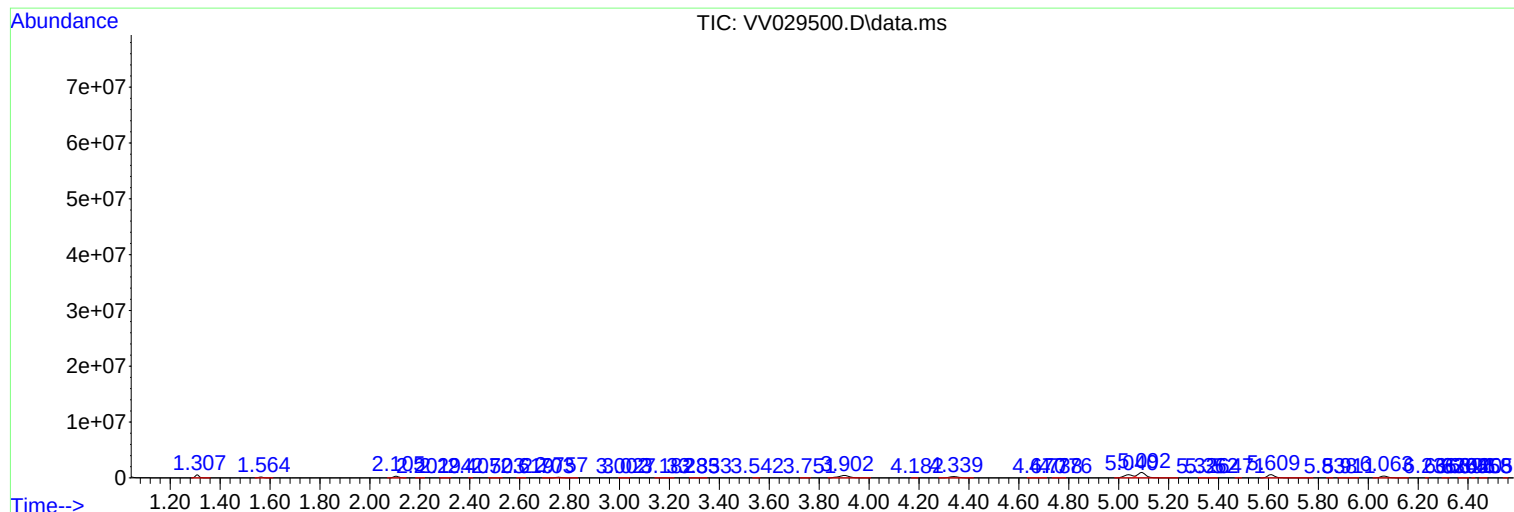

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
Data File : VV029500.D
Acq On : 09 Dec 2022 02:01
Operator : SY/MD
Sample : N5915-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5N09

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
Data File : VV029500.D
Acq On : 09 Dec 2022 02:01
Operator : SY/MD
Sample : N5915-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5N09

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------