

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
 Data File : VV029501.D
 Acq On : 09 Dec 2022 02:25
 Operator : SY/MD
 Sample : N5915-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5N12

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029501.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	100	rVB	143991	144610	5.46%	1.057%
2	1.561	155	162	177	rVB	137060	152787	5.77%	1.117%
3	2.105	321	331	342	rBV2	236896	344631	13.01%	2.519%
4	2.571	473	476	477	rBV	315	172	0.01%	0.001%
5	2.854	562	564	566	rBV2	249	109	0.00%	0.001%
6	2.966	596	599	601	rBV2	223	143	0.01%	0.001%
7	3.043	621	623	624	rBV2	248	99	0.00%	0.001%
8	3.150	652	656	659	rBV2	325	293	0.01%	0.002%
9	3.217	674	677	679	rBV2	214	176	0.01%	0.001%
10	3.397	732	733	735	rBV	178	83	0.00%	0.001%
11	3.494	761	763	765	rBV	191	130	0.00%	0.001%
12	3.529	770	774	776	rBV3	257	193	0.01%	0.001%
13	3.645	806	810	815	rBV3	230	318	0.01%	0.002%
14	3.719	828	833	836	rBV2	253	311	0.01%	0.002%
15	3.783	851	853	858	rBV2	252	194	0.01%	0.001%
16	3.870	870	880	916	rBV	112783	327726	12.37%	2.395%
17	4.240	992	995	998	rBV2	348	318	0.01%	0.002%
18	4.339	1009	1026	1051	rBV2	213052	532722	20.11%	3.893%
19	4.574	1096	1099	1102	rBV4	452	262	0.01%	0.002%
20	4.699	1135	1138	1142	rBV2	287	252	0.01%	0.002%
21	4.732	1146	1148	1149	rBV2	212	84	0.00%	0.001%
22	4.844	1181	1183	1185	rVB	318	117	0.00%	0.001%
23	4.870	1188	1191	1192	rBV	127	72	0.00%	0.001%
24	4.886	1192	1196	1198	rVV3	174	127	0.00%	0.001%
25	4.899	1198	1200	1202	rVV2	58	28	0.00%	0.000%
26	4.937	1209	1212	1213	rBV	207	102	0.00%	0.001%
27	4.963	1217	1220	1221	rBV2	246	142	0.01%	0.001%
28	5.040	1226	1244	1287	rBV2	502182	1342716	50.68%	9.813%
29	5.358	1340	1343	1344	rBV	292	170	0.01%	0.001%
30	5.442	1367	1369	1373	rVV3	243	132	0.00%	0.001%
31	5.465	1373	1376	1379	rVV2	234	147	0.01%	0.001%
32	5.484	1379	1382	1385	rVB3	341	258	0.01%	0.002%
33	5.522	1390	1394	1395	rBV2	216	149	0.01%	0.001%
34	5.609	1405	1421	1458	rBV	500885	1030783	38.90%	7.534%
35	5.912	1504	1515	1530	rVB8	8373	18794	0.71%	0.137%
36	5.985	1536	1538	1541	rBV2	290	167	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120822\
 Data File : VW029501.D
 Acq On : 09 Dec 2022 02:25
 Operator : SY/MD
 Sample : N5915-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5N12

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.063	1547	1562	1598	rBV	294753	614196	23.18%	4.489%
38	6.291	1631	1633	1634	rBV	334	111	0.00%	0.001%
39	6.362	1651	1655	1657	rBV2	365	201	0.01%	0.001%
40	6.442	1679	1680	1682	rBV2	216	89	0.00%	0.001%
41	6.474	1687	1690	1693	rBV	260	139	0.01%	0.001%
42	6.503	1696	1699	1701	rBV	230	118	0.00%	0.001%
43	6.516	1701	1703	1707	rVB2	561	328	0.01%	0.002%
44	6.542	1710	1711	1712	rBV2	196	39	0.00%	0.000%
45	6.555	1712	1715	1717	rBV2	195	139	0.01%	0.001%
46	6.587	1720	1725	1729	rVB3	514	352	0.01%	0.003%
47	6.609	1729	1732	1734	rBV2	720	504	0.02%	0.004%
48	6.728	1768	1769	1770	rBV2	138	45	0.00%	0.000%
49	6.760	1777	1779	1782	rBV	127	70	0.00%	0.001%
50	6.773	1782	1783	1787	rVB2	206	99	0.00%	0.001%
51	6.789	1787	1788	1789	rVB2	79	15	0.00%	0.000%
52	6.812	1789	1795	1798	rBV3	312	317	0.01%	0.002%
53	6.838	1800	1803	1804	rBV	201	142	0.01%	0.001%
54	6.883	1816	1817	1819	rVB	219	67	0.00%	0.000%
55	6.899	1819	1822	1824	rBV2	315	183	0.01%	0.001%
56	6.979	1836	1847	1878	rBV	149713	276209	10.42%	2.019%
57	7.149	1897	1900	1903	rBV3	716	605	0.02%	0.004%
58	7.223	1919	1923	1925	rBV3	842	625	0.02%	0.005%
59	7.307	1938	1949	1986	rBV	610260	1079312	40.73%	7.888%
60	7.612	2034	2044	2077	rBV	104939	187405	7.07%	1.370%
61	7.809	2102	2105	2106	rBV	439	198	0.01%	0.001%
62	8.082	2180	2190	2232	rBV	423813	743237	28.05%	5.432%
63	8.609	2348	2354	2356	rBV2	407	441	0.02%	0.003%
64	8.783	2406	2408	2411	rVB3	331	163	0.01%	0.001%
65	8.844	2414	2427	2431	rBV	781798	1214358	45.83%	8.875%
66	9.436	2608	2611	2614	rBV3	328	248	0.01%	0.002%
67	9.545	2641	2645	2651	rVB5	777	743	0.03%	0.005%
68	9.677	2684	2686	2691	rVB3	399	259	0.01%	0.002%
69	9.702	2691	2694	2696	rBV2	187	115	0.00%	0.001%
70	9.770	2714	2715	2717	rBV	183	80	0.00%	0.001%
71	9.876	2746	2748	2751	rBV2	177	153	0.01%	0.001%
72	9.895	2751	2754	2757	rBV	413	217	0.01%	0.002%
73	9.915	2757	2760	2762	rBV2	542	358	0.01%	0.003%
74	9.956	2771	2773	2774	rVB	341	97	0.00%	0.001%
75	9.966	2774	2776	2779	rBV2	240	160	0.01%	0.001%
76	10.011	2787	2790	2795	rBV3	439	426	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
 Data File : VV029501.D
 Acq On : 09 Dec 2022 02:25
 Operator : SY/MD
 Sample : N5915-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5N12

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.043	2797	2800	2801	rBV	184	112	0.00%	0.001%
78	10.098	2814	2817	2823	rVB3	311	351	0.01%	0.003%
79	10.124	2823	2825	2826	rBV	94	42	0.00%	0.000%
80	10.162	2826	2837	2841	rBV	18465	26452	1.00%	0.193%
81	10.207	2841	2851	2879	rVB	483471	766877	28.94%	5.605%
82	10.371	2887	2902	2914	rBV3	5926	10420	0.39%	0.076%
83	10.445	2924	2925	2930	rBV2	447	441	0.02%	0.003%
84	10.567	2955	2963	2981	rVB	9553	15751	0.59%	0.115%
85	10.664	2989	2993	2998	rBV4	463	436	0.02%	0.003%
86	10.686	2998	3000	3003	rVB2	198	108	0.00%	0.001%
87	10.702	3003	3005	3006	rBV	207	62	0.00%	0.000%
88	10.731	3006	3014	3021	rVB5	927	1462	0.06%	0.011%
89	10.760	3021	3023	3025	rBV3	205	104	0.00%	0.001%
90	10.831	3041	3045	3047	rBV3	353	295	0.01%	0.002%
91	10.876	3055	3059	3062	rBV3	489	475	0.02%	0.003%
92	10.966	3084	3087	3091	rBV3	449	307	0.01%	0.002%
93	11.043	3108	3111	3115	rVB3	856	572	0.02%	0.004%
94	11.172	3142	3151	3160	rBV	30385	47450	1.79%	0.347%
95	11.239	3161	3172	3202	rVB2	888348	2128255	80.32%	15.555%
96	11.628	3277	3293	3322	rBV2	1155711	2649620	100.00%	19.365%
97	12.005	3404	3410	3418	rBV2	3434	4917	0.19%	0.036%
98	12.104	3435	3441	3442	rBV3	1112	1201	0.05%	0.009%
99	12.185	3464	3466	3467	rBV	527	223	0.01%	0.002%
100	12.400	3527	3533	3542	rVB3	3375	4430	0.17%	0.032%




Sum of corrected areas: 13682443

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
Data File : VV029501.D
Acq On : 09 Dec 2022 02:25
Operator : SY/MD
Sample : N5915-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5N12

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

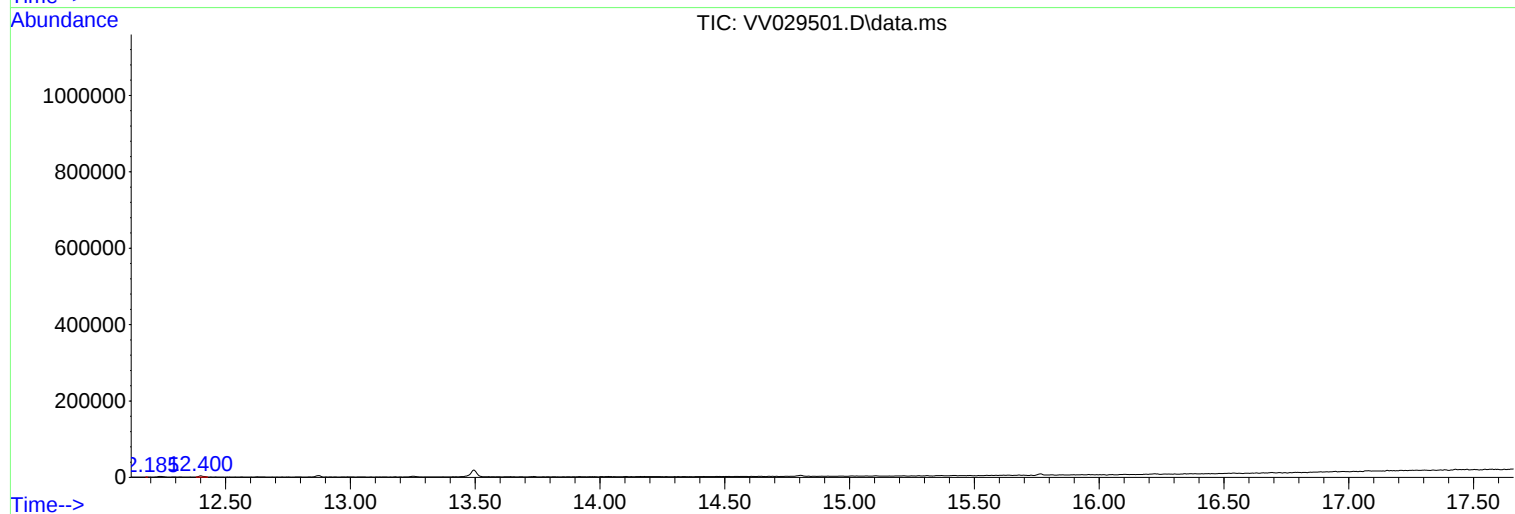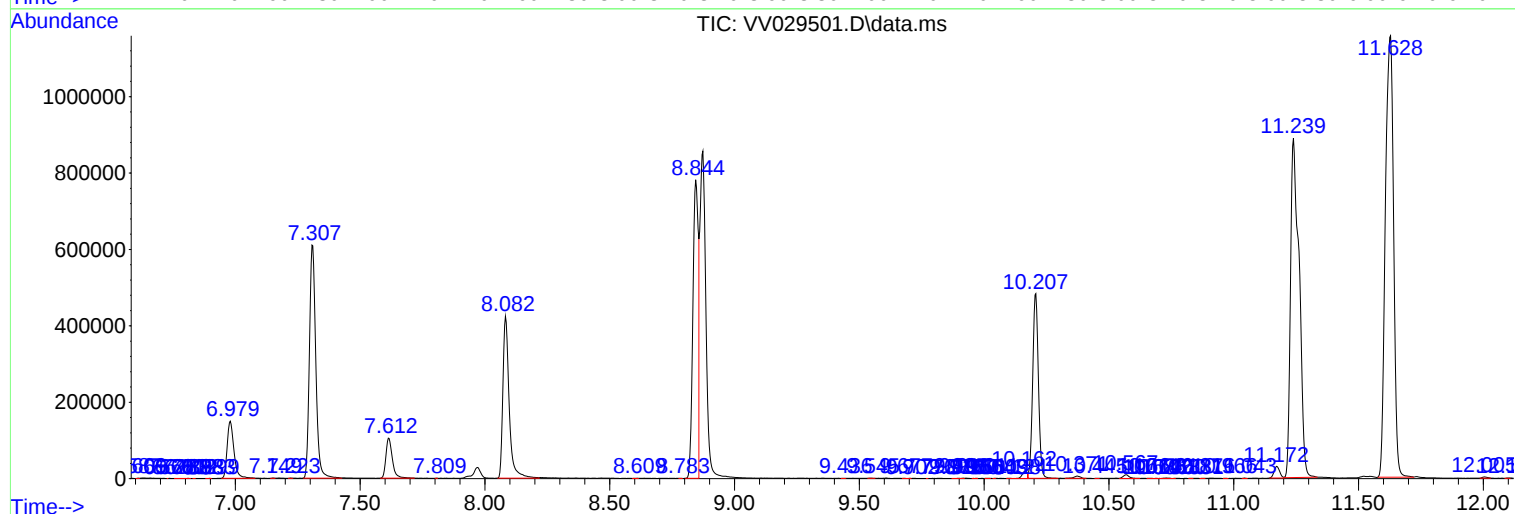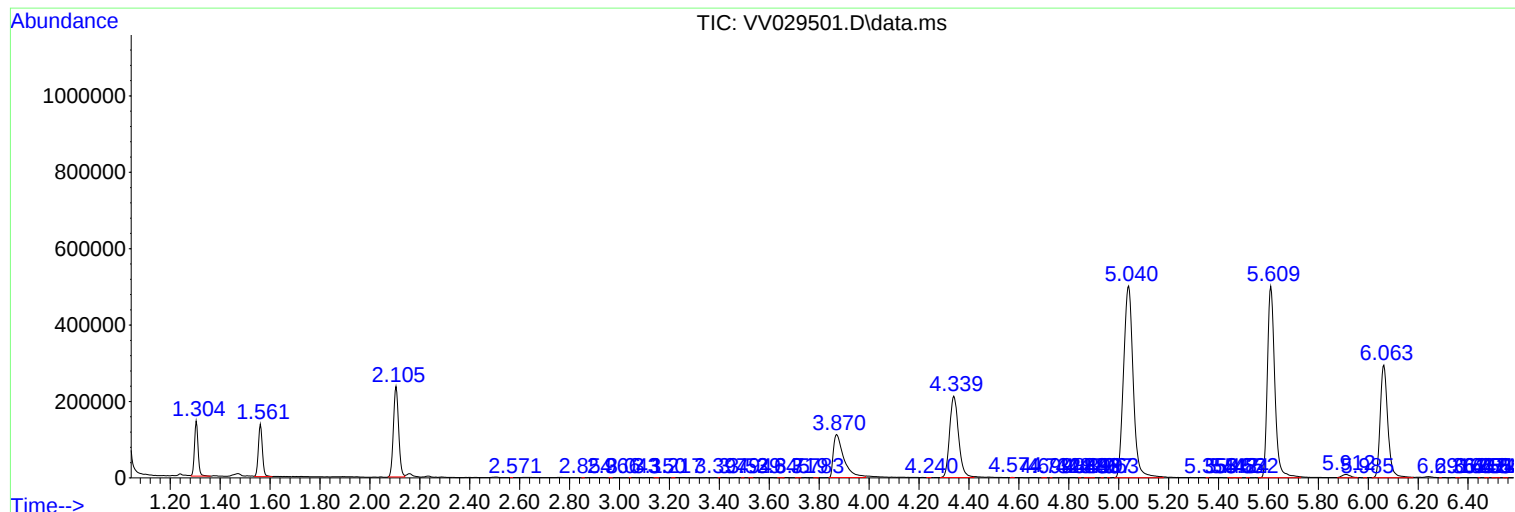

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
Data File : VV029501.D
Acq On : 09 Dec 2022 02:25
Operator : SY/MD
Sample : N5915-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5N12

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
Data File : VV029501.D
Acq On : 09 Dec 2022 02:25
Operator : SY/MD
Sample : N5915-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5N12

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------