

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
 Data File : VV029508.D
 Acq On : 09 Dec 2022 05:09
 Operator : SY/MD
 Sample : N5928-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ68

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029508.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	99	rBV2	875948	911757	7.64%	2.250%
2	1.564	155	163	166	rBV	244474	277277	2.32%	0.684%
3	1.706	201	207	214	rVB	10632	12184	0.10%	0.030%
4	1.751	216	221	226	rBV2	6063	7514	0.06%	0.019%
5	2.108	320	332	356	rBV3	527108	851563	7.13%	2.102%
6	2.507	449	456	462	rVB3	2447	3369	0.03%	0.008%
7	2.619	488	491	494	rBV3	422	368	0.00%	0.001%
8	2.757	519	534	553	rBV2	57905	105584	0.88%	0.261%
9	2.976	600	602	610	rVB4	518	584	0.00%	0.001%
10	3.182	649	666	706	rBV	1923644	4048723	33.91%	9.992%
11	3.568	782	786	791	rVB3	465	402	0.00%	0.001%
12	3.712	826	831	838	rVB3	478	424	0.00%	0.001%
13	3.822	851	865	870	rBV7	1536	3255	0.03%	0.008%
14	3.902	870	890	969	rVV	4808591	11938041	100.00%	29.462%
15	4.339	1010	1026	1061	rBV	290406	717892	6.01%	1.772%
16	4.600	1086	1107	1176	rBV	2960561	7485551	62.70%	18.474%
17	5.040	1225	1244	1298	rBV2	727607	1959920	16.42%	4.837%
18	5.609	1408	1421	1462	rBV	589378	1205341	10.10%	2.975%
19	5.908	1501	1514	1535	rBV	101186	207928	1.74%	0.513%
20	6.063	1548	1562	1597	rBV	398643	832771	6.98%	2.055%
21	6.281	1624	1630	1635	rVB4	536	687	0.01%	0.002%
22	6.346	1646	1650	1654	rVB4	479	409	0.00%	0.001%
23	6.542	1706	1711	1716	rBV3	435	344	0.00%	0.001%
24	6.622	1728	1736	1739	rBV5	1321	1841	0.02%	0.005%
25	6.979	1834	1847	1874	rBV	197150	362819	3.04%	0.895%
26	7.159	1898	1903	1909	rBV7	849	1174	0.01%	0.003%
27	7.256	1926	1933	1936	rVV5	920	1063	0.01%	0.003%
28	7.307	1937	1949	1987	rVV	911943	1621995	13.59%	4.003%
29	7.612	2034	2044	2069	rBV	138386	245580	2.06%	0.606%
30	7.834	2104	2113	2124	rVB5	3576	5807	0.05%	0.014%
31	7.969	2131	2155	2179	rBV	250369	443030	3.71%	1.093%
32	8.082	2179	2190	2227	rBV	488606	863617	7.23%	2.131%
33	8.339	2265	2270	2274	rBV4	1069	1220	0.01%	0.003%
34	8.509	2320	2323	2329	rVB4	612	594	0.00%	0.001%
35	8.538	2329	2332	2336	rVB4	506	400	0.00%	0.001%
36	8.751	2394	2398	2404	rBV4	590	601	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120822\
 Data File : VW029508.D
 Acq On : 09 Dec 2022 05:09
 Operator : SY/MD
 Sample : N5928-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ68

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	8.844	2414	2427	2466	rBV	859542	1464435	12.27%	3.614%
38	9.008	2470	2478	2487	rVB2	6294	10488	0.09%	0.026%
39	9.046	2487	2490	2492	rBV3	588	450	0.00%	0.001%
40	9.130	2504	2516	2530	rVB2	13751	25169	0.21%	0.062%
41	9.181	2530	2532	2538	rVB5	877	626	0.01%	0.002%
42	9.207	2538	2540	2544	rBV2	537	438	0.00%	0.001%
43	9.268	2556	2559	2563	rBV3	530	487	0.00%	0.001%
44	9.362	2582	2588	2591	rVB3	387	365	0.00%	0.001%
45	9.448	2610	2615	2616	rBV2	581	410	0.00%	0.001%
46	9.474	2616	2623	2624	rBV3	1018	970	0.01%	0.002%
47	9.538	2634	2643	2651	rBV3	7851	12769	0.11%	0.032%
48	9.696	2683	2692	2700	rVB4	5796	8446	0.07%	0.021%
49	9.924	2754	2763	2773	rBV	5843	8978	0.08%	0.022%
50	10.005	2782	2788	2795	rVB4	1061	1355	0.01%	0.003%
51	10.079	2804	2811	2816	rBV5	1373	1775	0.01%	0.004%
52	10.117	2816	2823	2829	rVV5	3148	4215	0.04%	0.010%
53	10.162	2829	2837	2841	rVV2	27799	40190	0.34%	0.099%
54	10.207	2841	2851	2874	rVB	583103	935267	7.83%	2.308%
55	10.342	2884	2893	2899	rBV	13952	21499	0.18%	0.053%
56	10.439	2914	2923	2930	rBV2	13232	23691	0.20%	0.058%
57	10.532	2943	2952	2957	rBV	18372	26793	0.22%	0.066%
58	10.567	2958	2963	2974	rVV	13762	20869	0.17%	0.052%
59	10.728	3004	3013	3029	rVB	24071	36695	0.31%	0.091%
60	10.853	3043	3052	3058	rBV5	2773	4322	0.04%	0.011%
61	10.905	3058	3068	3082	rVB	77025	115220	0.97%	0.284%
62	11.014	3096	3102	3105	rBV4	1121	1189	0.01%	0.003%
63	11.043	3105	3111	3115	rVV2	4590	6188	0.05%	0.015%
64	11.075	3115	3121	3133	rVB	15918	23626	0.20%	0.058%
65	11.181	3144	3154	3160	rBV4	7527	10749	0.09%	0.027%
66	11.236	3160	3171	3190	rVV	970992	1538388	12.89%	3.797%
67	11.326	3191	3199	3216	rVV	32254	53166	0.45%	0.131%
68	11.390	3216	3219	3225	rVV3	634	571	0.00%	0.001%
69	11.442	3229	3235	3242	rVB3	2012	2456	0.02%	0.006%
70	11.525	3250	3261	3268	rBV4	18499	37966	0.32%	0.094%
71	11.612	3277	3288	3316	rVB	976260	1620387	13.57%	3.999%
72	11.808	3340	3349	3359	rBV	7617	11386	0.10%	0.028%
73	11.915	3369	3382	3394	rBV3	28787	67493	0.57%	0.167%
74	12.127	3433	3448	3462	rBV3	13711	39943	0.33%	0.099%
75	12.236	3473	3482	3491	rBV5	3782	6766	0.06%	0.017%
76	12.300	3492	3502	3514	rVV5	5048	10130	0.08%	0.025%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
 Data File : VV029508.D
 Acq On : 09 Dec 2022 05:09
 Operator : SY/MD
 Sample : N5928-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ68

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	12.365	3518	3522	3524	rVV4	1133	900	0.01%	0.002%
78	12.400	3526	3533	3541	rVV3	4991	7492	0.06%	0.018%
79	12.455	3541	3550	3564	rVB3	9506	14571	0.12%	0.036%
80	12.541	3571	3577	3582	rBV3	2324	2552	0.02%	0.006%
81	12.599	3592	3595	3597	rBV2	496	370	0.00%	0.001%
82	12.628	3601	3604	3608	rBV7	1298	1224	0.01%	0.003%
83	12.670	3613	3617	3624	rVV6	2283	3075	0.03%	0.008%
84	12.712	3624	3630	3636	rVB5	2520	3133	0.03%	0.008%
85	12.834	3662	3668	3670	rBV3	1204	1140	0.01%	0.003%
86	12.869	3670	3679	3689	rVV4	17152	25915	0.22%	0.064%
87	12.934	3692	3699	3712	rVB4	5141	9760	0.08%	0.024%
88	13.001	3716	3720	3722	rVV3	695	561	0.00%	0.001%
89	13.033	3723	3730	3739	rVV5	6905	10748	0.09%	0.027%
90	13.072	3739	3742	3746	rVB3	833	635	0.01%	0.002%
91	13.207	3778	3784	3789	rVB5	1907	2768	0.02%	0.007%
92	13.259	3789	3800	3807	rBV7	3189	5367	0.04%	0.013%
93	13.287	3807	3809	3811	rBV3	903	523	0.00%	0.001%
94	13.355	3826	3830	3836	rVB5	1854	2133	0.02%	0.005%
95	13.435	3850	3855	3856	rBV5	1126	975	0.01%	0.002%
96	13.493	3864	3873	3892	rVB	42933	69887	0.59%	0.172%
97	13.869	3986	3990	3994	rBV6	1003	1037	0.01%	0.003%
98	14.056	4045	4048	4050	rBV4	1030	662	0.01%	0.002%
99	14.619	4215	4223	4232	rVB	12425	19103	0.16%	0.047%
100	14.802	4271	4280	4290	rVB3	10707	17227	0.14%	0.043%

Sum of corrected areas: 40519713




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
Data File : VV029508.D
Acq On : 09 Dec 2022 05:09
Operator : SY/MD
Sample : N5928-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ68

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

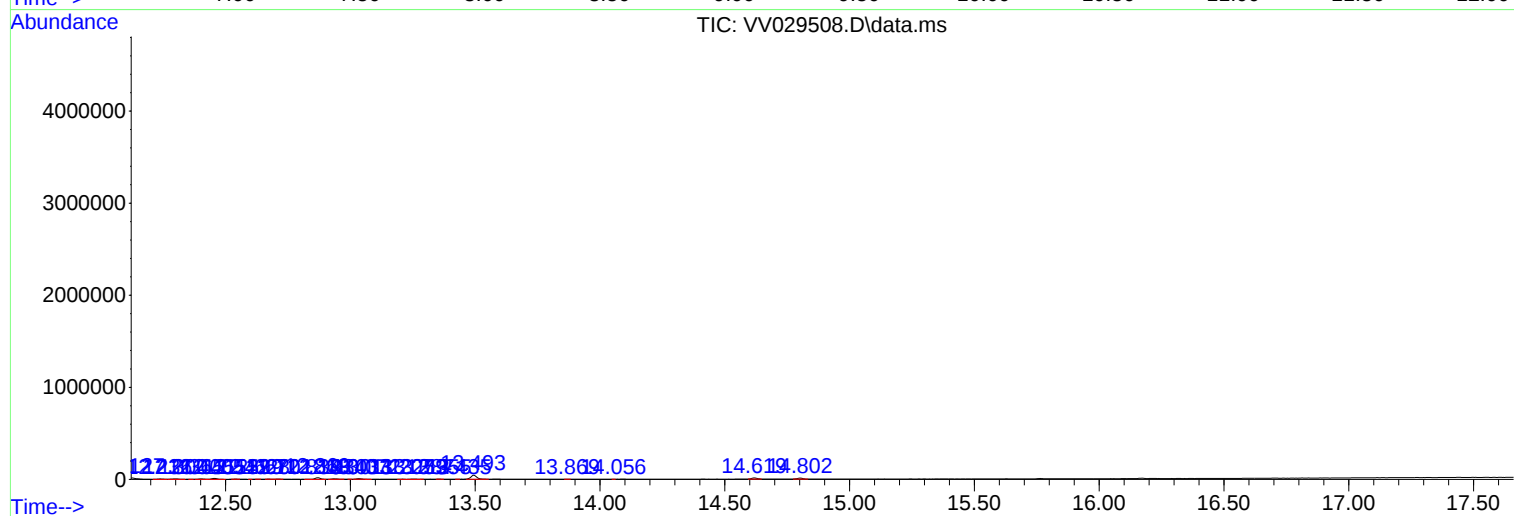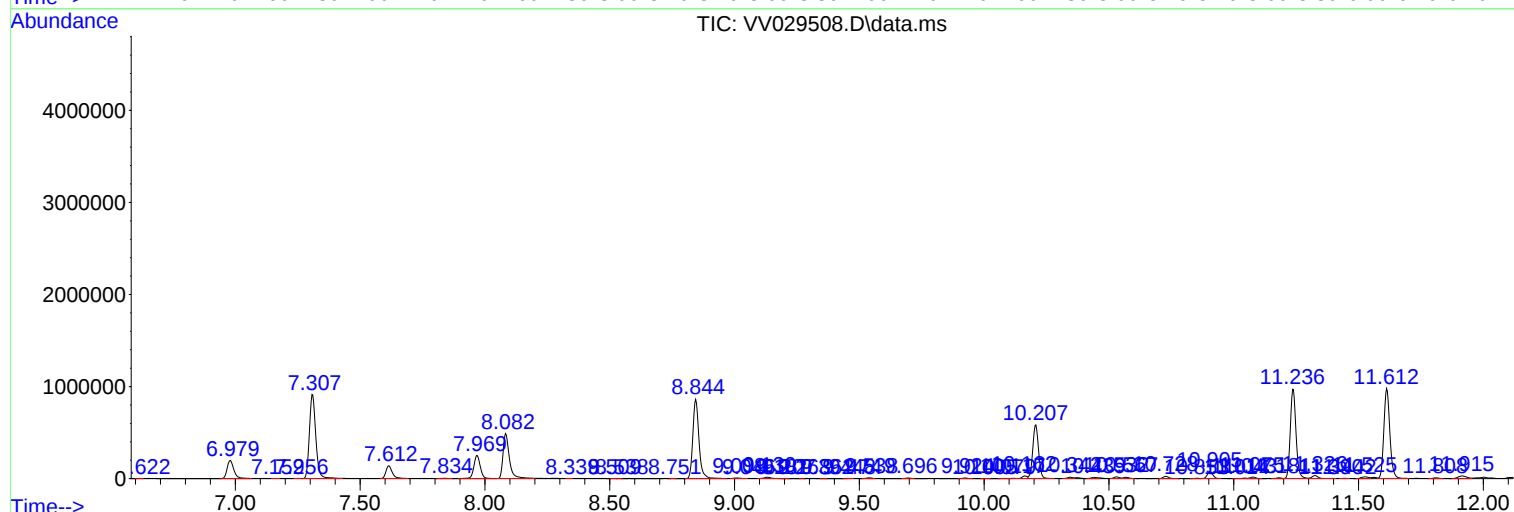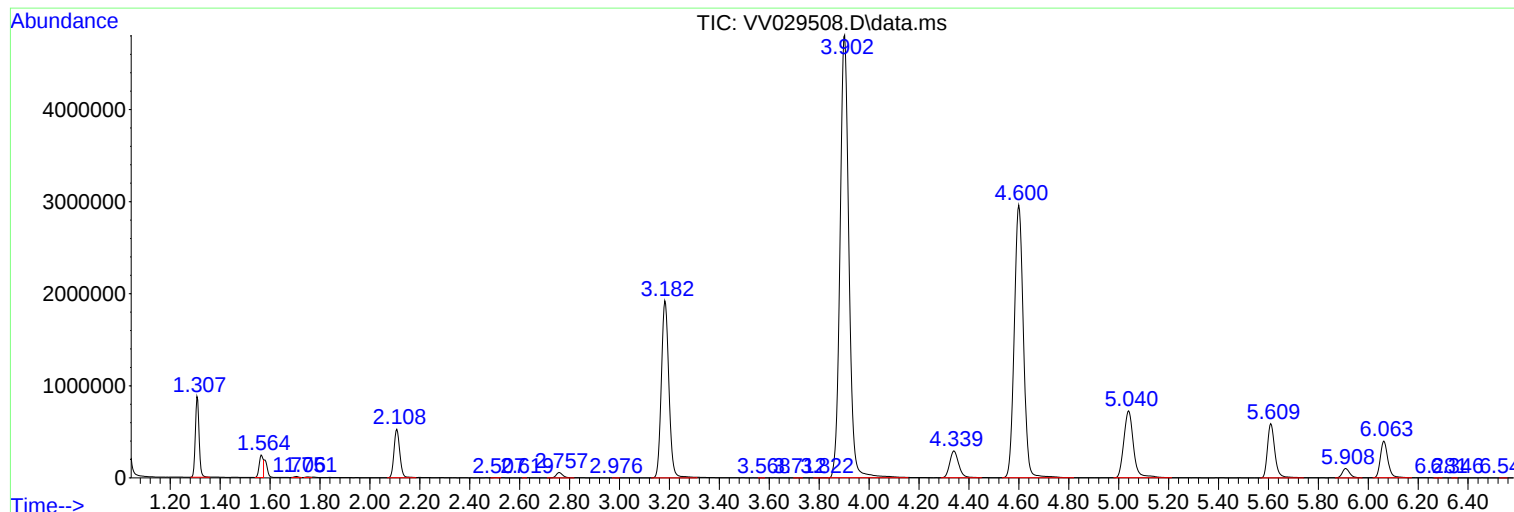

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
Data File : VV029508.D
Acq On : 09 Dec 2022 05:09
Operator : SY/MD
Sample : N5928-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ68

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
Data File : VV029508.D
Acq On : 09 Dec 2022 05:09
Operator : SY/MD
Sample : N5928-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ68

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc